

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012517\
 Data File : BG025643.D
 Acq On : 25 Jan 2017 20:59
 Operator : SJ/MA
 Sample : PB96323BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011817.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.508	110	114	122	rBV7	19184	33753	0.99%	0.106%
2	3.837	167	170	171	rBV2	7145	6235	0.18%	0.020%
3	4.284	243	246	249	rVB4	5564	6618	0.19%	0.021%
4	4.954	357	360	367	rVB6	7582	15455	0.45%	0.048%
5	5.253	409	411	415	rBV4	5813	6695	0.20%	0.021%
6	5.394	432	435	439	rVB3	5820	6809	0.20%	0.021%
7	5.500	450	453	457	rBV3	6487	9584	0.28%	0.030%
8	5.676	479	483	490	rVB6	6254	16152	0.47%	0.051%
9	6.276	582	585	588	rBV3	7765	7000	0.20%	0.022%
10	6.370	597	601	604	rBV4	6249	8186	0.24%	0.026%
11	6.569	629	635	638	rBV4	5914	12171	0.36%	0.038%
12	6.722	659	661	666	rVB4	4557	7030	0.21%	0.022%
13	6.804	670	675	678	rBV4	3137	6941	0.20%	0.022%
14	7.075	718	721	724	rVB4	6132	7590	0.22%	0.024%
15	7.216	739	745	753	rBV6	6162	11804	0.35%	0.037%
16	7.339	757	766	782	rBV	310387	680814	19.92%	2.132%
17	7.492	786	792	806	rVV	254710	454632	13.30%	1.424%
18	7.586	806	808	814	rVB5	7435	11255	0.33%	0.035%
19	7.709	822	829	840	rBV	326267	630039	18.43%	1.973%
20	7.979	870	875	877	rVB4	6433	6490	0.19%	0.020%
21	8.179	902	909	917	rBV	240279	456922	13.37%	1.431%
22	8.285	926	927	932	rVB3	5425	6935	0.20%	0.022%
23	8.397	943	946	948	rBV2	6678	8478	0.25%	0.027%
24	8.420	948	950	957	rVV5	8245	12840	0.38%	0.040%
25	8.514	963	966	975	rVV6	7023	11366	0.33%	0.036%
26	8.714	997	1000	1002	rVB4	6992	7053	0.21%	0.022%
27	8.802	1011	1015	1017	rBV2	5966	7529	0.22%	0.024%
28	8.896	1022	1031	1050	rBV2	400379	864202	25.28%	2.707%
29	9.049	1052	1057	1060	rBV6	3632	6045	0.18%	0.019%
30	9.360	1100	1110	1124	rBV	392565	753133	22.03%	2.359%
31	9.554	1140	1143	1147	rVB2	5360	7423	0.22%	0.023%
32	9.918	1202	1205	1211	rVB4	5913	11983	0.35%	0.038%
33	9.983	1211	1216	1219	rBV3	7190	10476	0.31%	0.033%
34	10.030	1219	1224	1226	rBV4	4700	6311	0.18%	0.020%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012517\
 Data File : BG025643.D
 Acq On : 25 Jan 2017 20:59
 Operator : SJ/MA
 Sample : PB96323BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011817.M
 Title : SVOA CALIBRATION

35	10.089	1226	1234	1249	rBV2	333853	700632	20.50%	2.194%
36	10.635	1317	1327	1354	rBV2	419878	920206	26.92%	2.882%
37	10.870	1364	1367	1372	rBV5	5483	6955	0.20%	0.022%
38	10.905	1372	1373	1380	rVB4	6170	11316	0.33%	0.035%
39	11.005	1380	1390	1402	rBV	373339	717039	20.97%	2.246%
40	11.152	1406	1415	1442	rBV2	401013	940570	27.51%	2.946%
41	11.487	1468	1472	1475	rBV3	6018	7653	0.22%	0.024%
42	11.892	1537	1541	1543	rBV2	8540	6959	0.20%	0.022%
43	11.945	1547	1550	1552	rBV2	5843	7037	0.21%	0.022%
44	12.033	1560	1565	1568	rVB3	4166	7072	0.21%	0.022%
45	12.221	1591	1597	1600	rBV6	5600	10746	0.31%	0.034%
46	12.245	1600	1601	1605	rVB2	6451	6364	0.19%	0.020%
47	12.556	1650	1654	1658	rBV5	3889	6381	0.19%	0.020%
48	12.609	1658	1663	1674	rVB8	8891	27681	0.81%	0.087%
49	13.385	1788	1795	1801	rBV4	6614	15432	0.45%	0.048%
50	13.479	1807	1811	1816	rBV4	4364	6088	0.18%	0.019%
51	13.726	1852	1853	1858	rBV4	5851	7554	0.22%	0.024%
52	13.890	1877	1881	1886	rBV2	5581	8148	0.24%	0.026%
53	14.202	1922	1934	1947	rBV	1077760	1725160	50.46%	5.403%
54	14.507	1975	1986	1997	rBV	1115888	1807815	52.88%	5.662%
55	14.807	2027	2037	2047	rBV	738806	1160099	33.94%	3.634%
56	15.042	2071	2077	2097	rBV3	277340	785046	22.96%	2.459%
57	15.371	2131	2133	2138	rVB5	4803	6235	0.18%	0.020%
58	15.576	2163	2168	2174	rVB6	5128	10342	0.30%	0.032%
59	15.794	2198	2205	2219	rBV	1520424	2408753	70.46%	7.545%
60	15.941	2222	2230	2241	rBV2	484348	902321	26.39%	2.826%
61	16.035	2244	2246	2254	rVB6	25173	36977	1.08%	0.116%
62	16.117	2259	2260	2267	rVB5	8412	10880	0.32%	0.034%
63	16.240	2277	2281	2285	rBV5	3638	7095	0.21%	0.022%
64	16.375	2299	2304	2309	rVV5	4754	8833	0.26%	0.028%
65	16.422	2309	2312	2318	rVV3	4555	9393	0.27%	0.029%
66	16.563	2335	2336	2342	rBV3	5836	9922	0.29%	0.031%
67	16.746	2360	2367	2372	rBV6	8147	17257	0.50%	0.054%
68	16.869	2385	2388	2395	rBV5	5711	9966	0.29%	0.031%
69	16.934	2396	2399	2404	rVB4	5227	7684	0.22%	0.024%
70	17.145	2434	2435	2439	rVB3	7140	7633	0.22%	0.024%
71	17.210	2443	2446	2452	rVV4	3949	7739	0.23%	0.024%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012517\
Data File : BG025643.D
Acq On : 25 Jan 2017 20:59
Operator : SJ/MA
Sample : PB96323BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.1
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011817.M
Title : SVOA CALIBRATION

72	17.351	2467	2470	2473	rVB3	7268	7966	0.23%	0.025%
73	17.398	2476	2478	2480	rBV2	9068	6846	0.20%	0.021%
74	17.551	2496	2504	2514	rBV	983614	1601411	46.84%	5.016%
75	17.656	2514	2522	2537	rVB	1634440	2804093	82.03%	8.783%
76	17.862	2556	2557	2564	rVB5	5202	6253	0.18%	0.020%
77	17.915	2564	2566	2570	rVB4	5898	6604	0.19%	0.021%
78	17.979	2574	2577	2583	rVB4	7948	12367	0.36%	0.039%
79	18.032	2583	2586	2589	rBV4	6815	6534	0.19%	0.020%
80	18.261	2622	2625	2629	rBV5	5494	8322	0.24%	0.026%
81	18.308	2629	2633	2637	rBV6	4990	8864	0.26%	0.028%
82	18.491	2660	2664	2668	rBV6	8341	8896	0.26%	0.028%
83	18.679	2693	2696	2701	rVB5	6122	8393	0.25%	0.026%
84	18.855	2725	2726	2730	rBV3	6083	7682	0.22%	0.024%
85	19.219	2785	2788	2790	rBV4	7415	6436	0.19%	0.020%
86	19.278	2796	2798	2803	rBV4	8567	8881	0.26%	0.028%
87	19.484	2831	2833	2835	rBV3	9220	7890	0.23%	0.025%
88	19.572	2845	2848	2857	rVB4	23290	35769	1.05%	0.112%
89	19.818	2886	2890	2898	rVB3	20379	28518	0.83%	0.089%
90	19.930	2902	2909	2921	rBV	2285164	3369438	98.56%	10.554%
91	20.100	2937	2938	2946	rVB7	9265	13609	0.40%	0.043%
92	20.218	2957	2958	2964	rBV6	10166	14012	0.41%	0.044%
93	20.271	2966	2967	2973	rBV6	9980	9374	0.27%	0.029%
94	20.318	2973	2975	2978	rBV4	7600	7766	0.23%	0.024%
95	21.340	3146	3149	3151	rBV4	12497	13614	0.40%	0.043%
96	21.846	3228	3235	3246	rBV	1045055	1924037	56.28%	6.026%
97	25.001	3760	3772	3784	rBV2	1092700	3418543	100.00%	10.707%
98	25.230	3800	3811	3826	rBV3	586422	1889858	55.28%	5.919%
99	26.258	3981	3986	3999	rVB3	39913	122279	3.58%	0.383%
100	27.662	4220	4225	4236	rVB3	32779	93609	2.74%	0.293%


Sum of corrected areas: 31926796

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012517\
Data File : BG025643.D
Acq On : 25 Jan 2017 20:59
Operator : SJ/MA
Sample : PB96323BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK23

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG011817.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

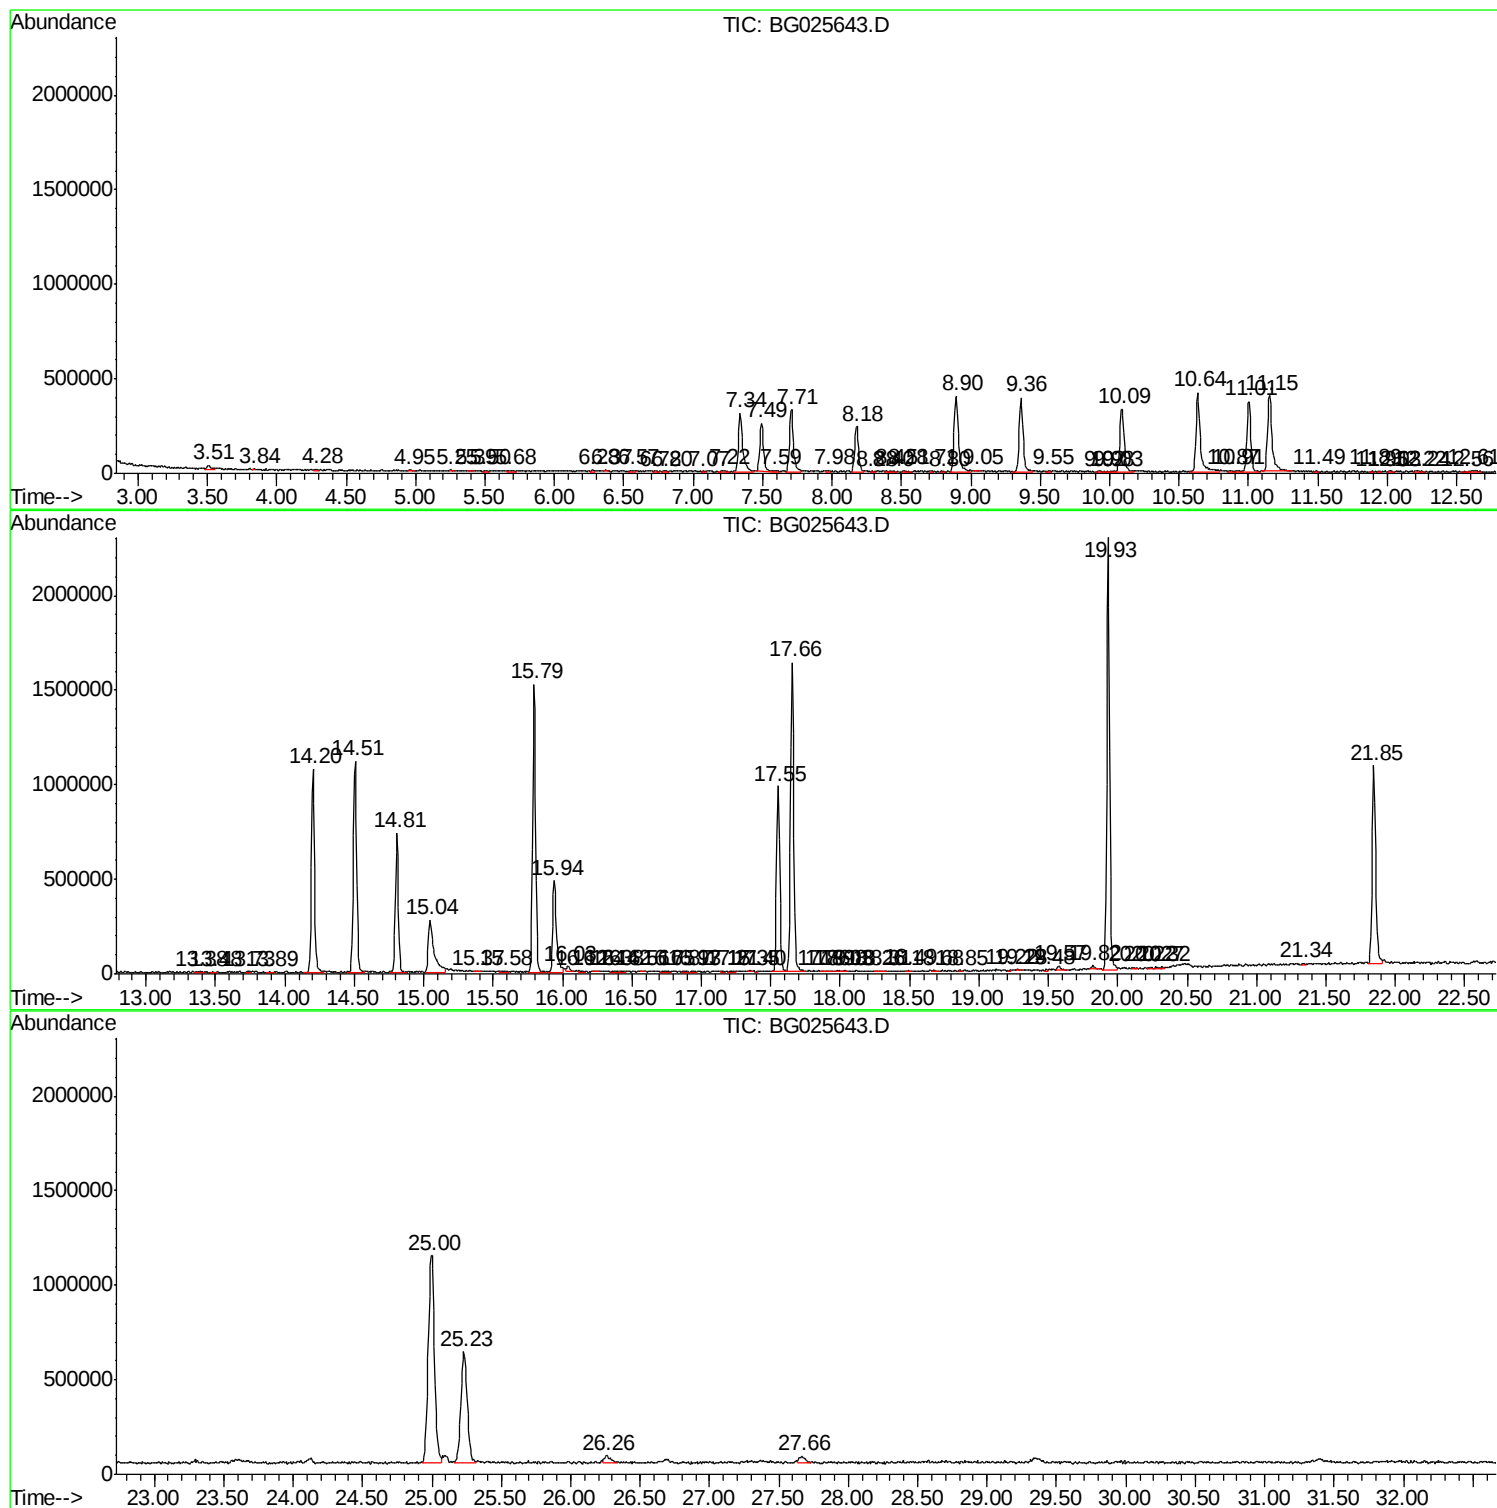

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012517\
Data File : BG025643.D
Acq On : 25 Jan 2017 20:59
Operator : SJ/MA
Sample : PB96323BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK23

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011817.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012517\
Data File : BG025643.D
Acq On : 25 Jan 2017 20:59
Operator : SJ/MA
Sample : PB96323BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK23

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011817.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc