
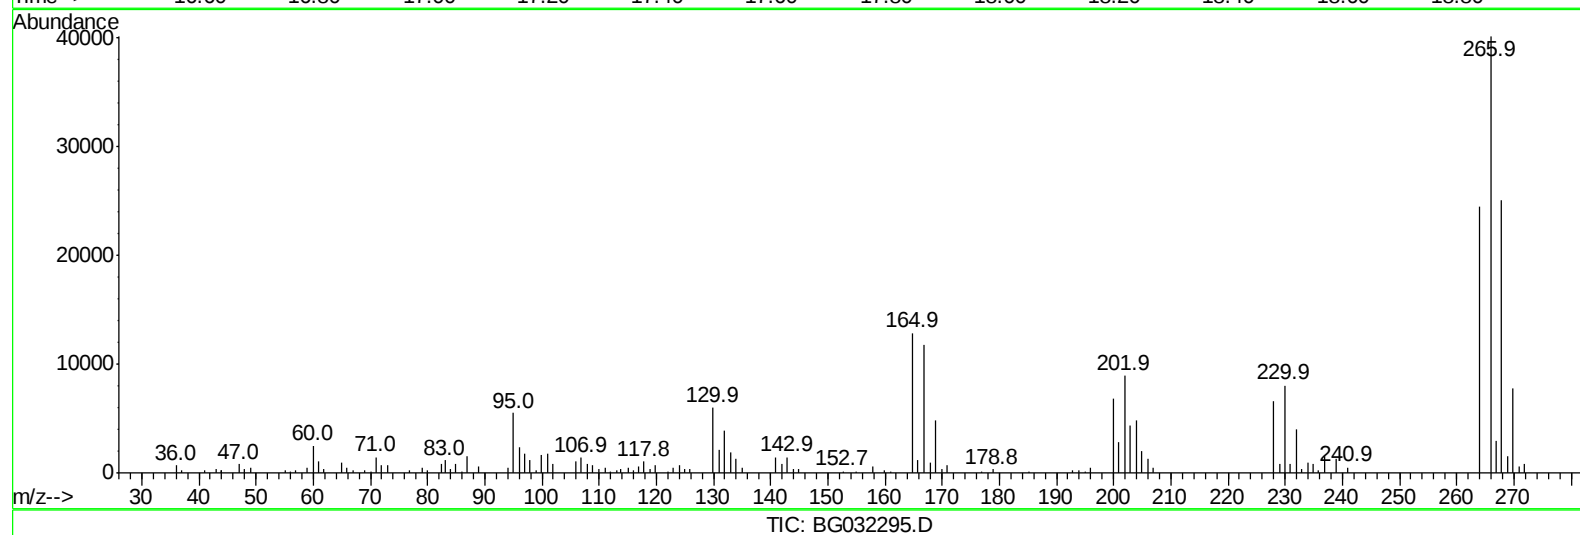


Data Path : U:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032295.D
Acq On : 25 Jan 2018 15:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 06:42:10 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

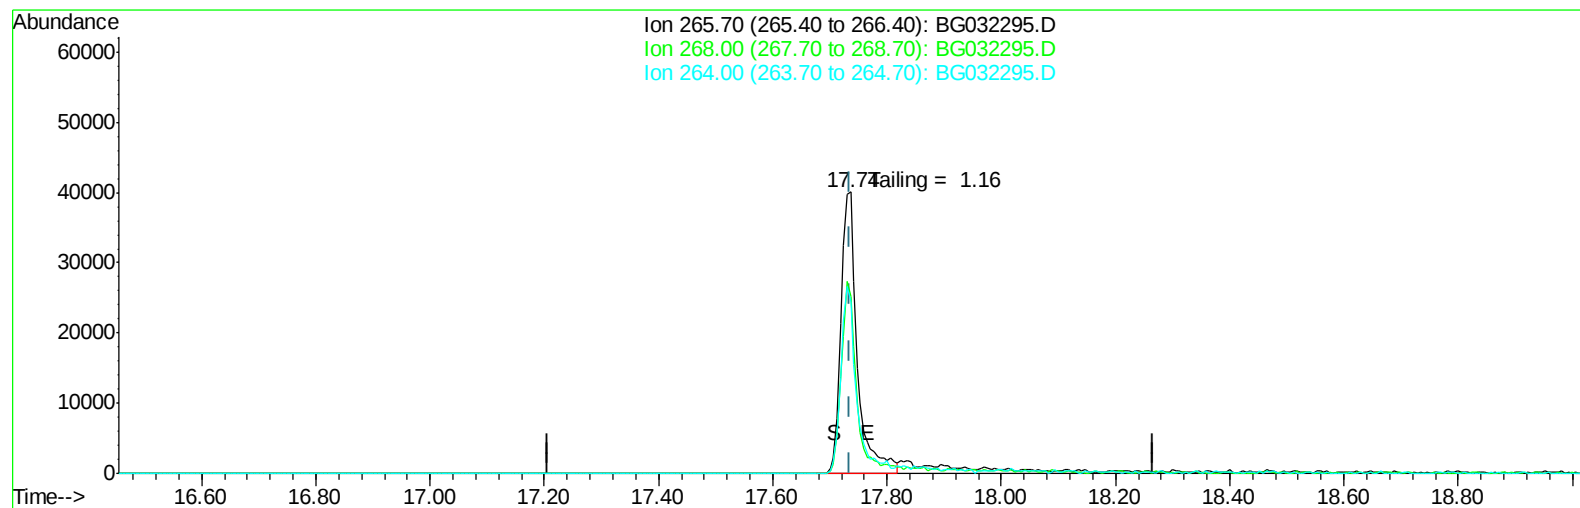

(69) Pentachlorophenol (C)



17.736min (-0.000) 100918.78ng

response 80217

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.56
264.00	62.00	60.95
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032295.D
Acq On : 25 Jan 2018 15:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 06:42:10 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

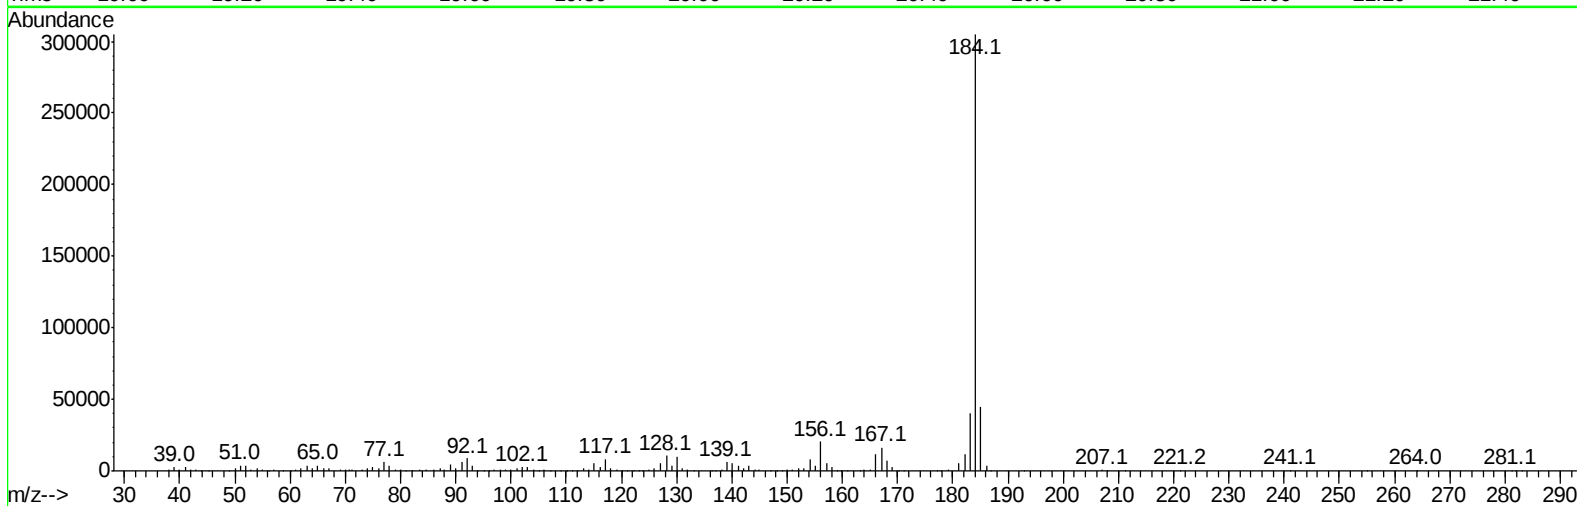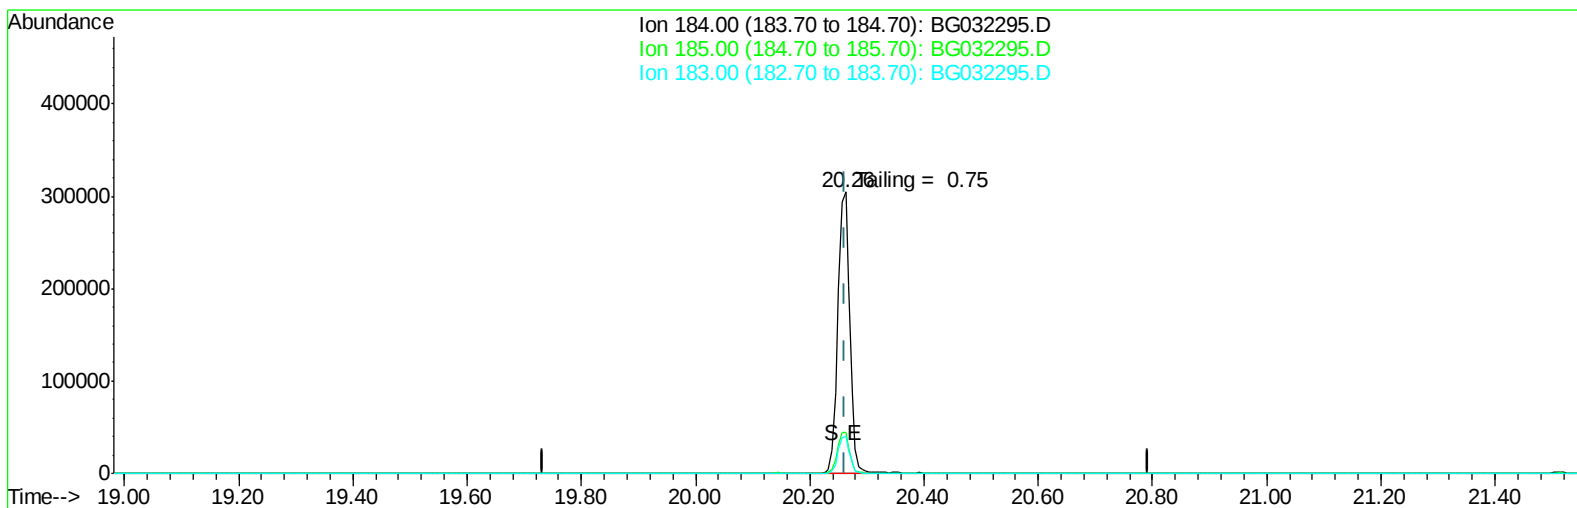

TIC: BG032295.D

(76) Benzidine

20.262min (-0.000) 327673.73ng

response 442469

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.69
183.00	13.30	13.25
0.00	0.00	0.00