
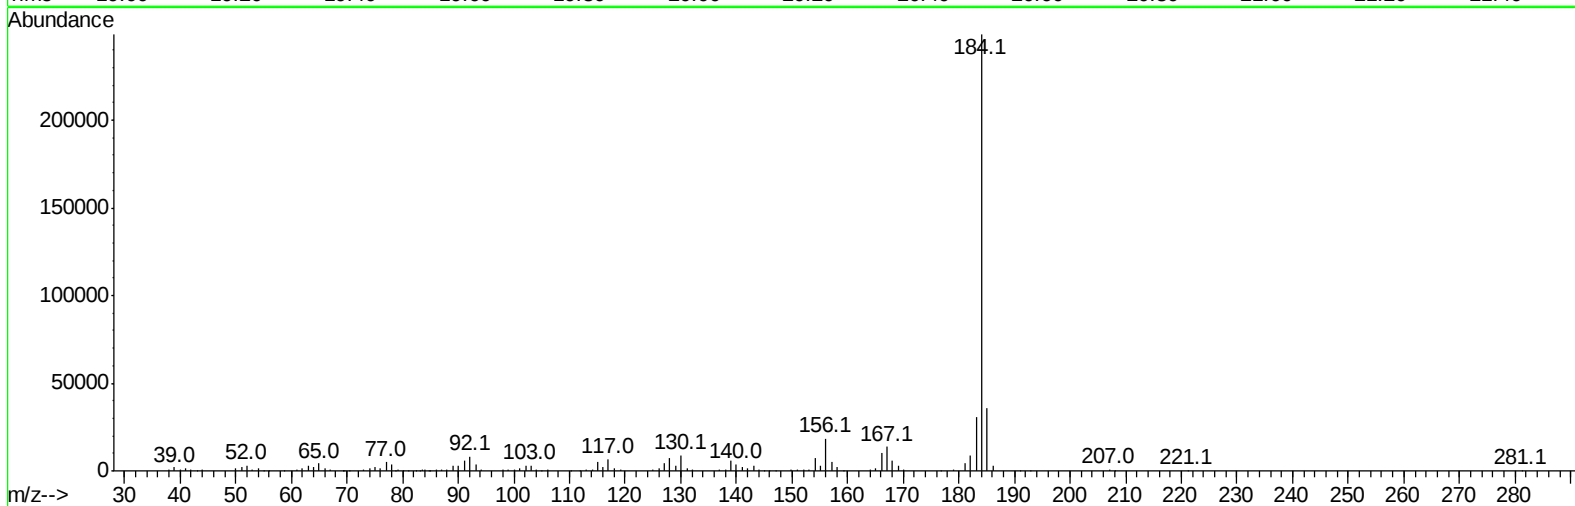


Data Path : U:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032313.D
Acq On : 26 Jan 2018 3:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 06:40:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

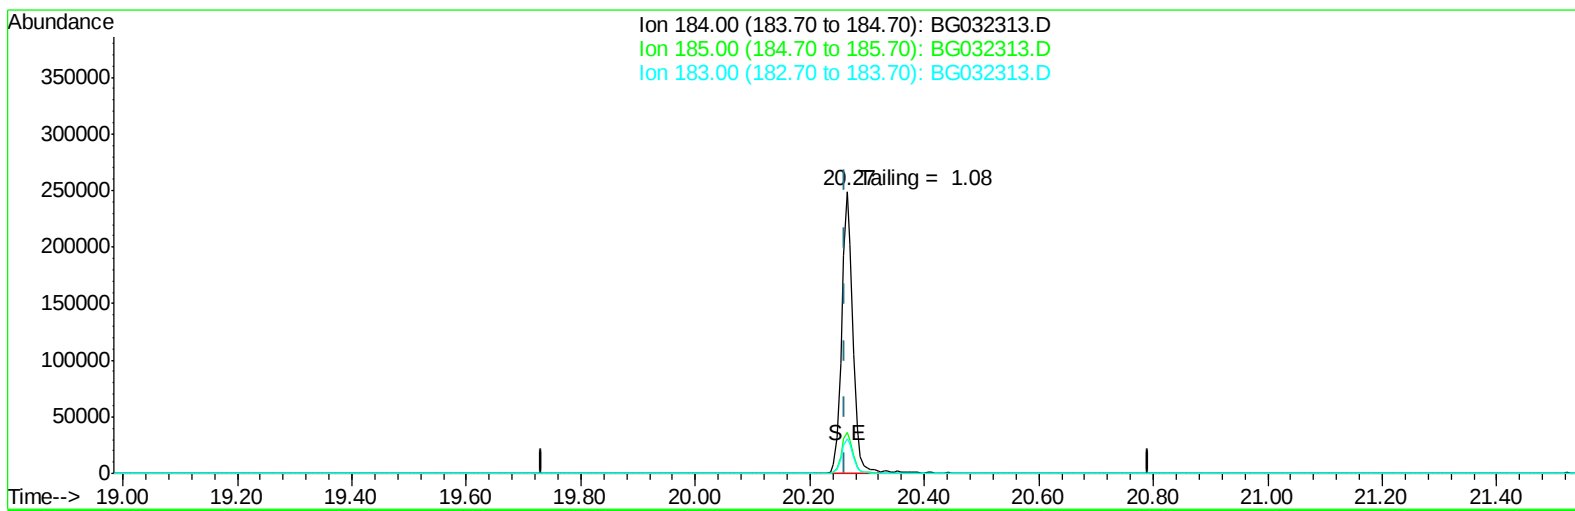

TIC: BG032313.D

(76) Benzidine



20.265min (+0.002) 0.00ng

response 342019

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.50
183.00	13.30	12.44
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032313.D
Acq On : 26 Jan 2018 3:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 06:40:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

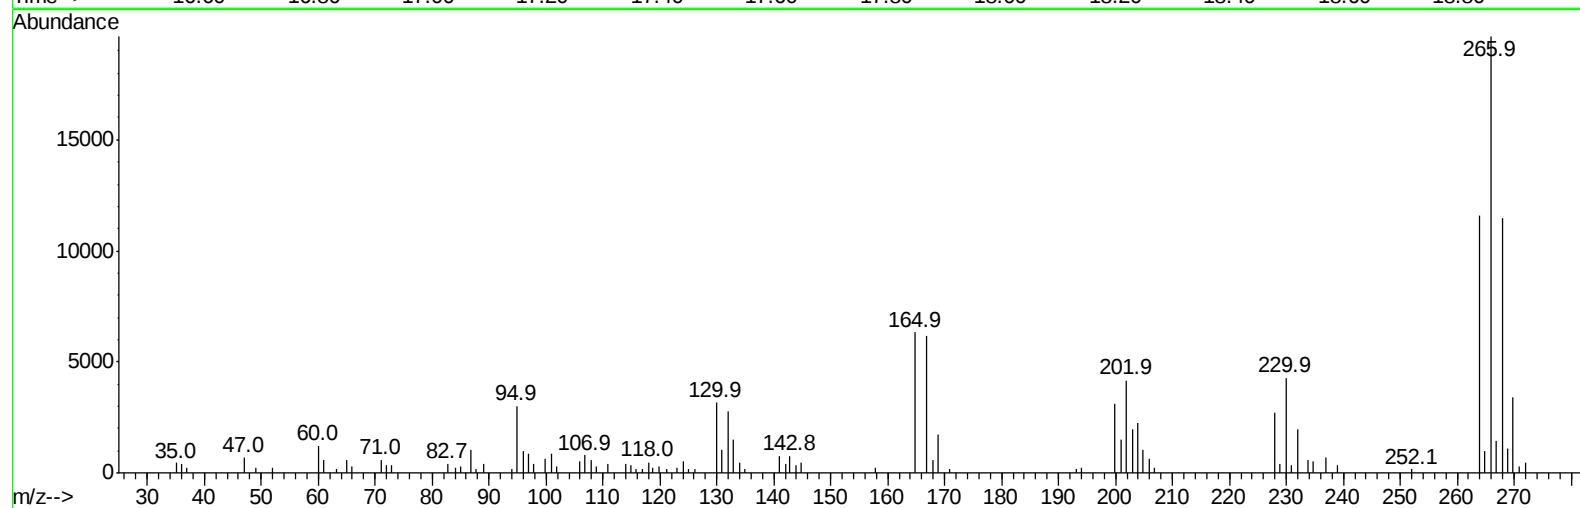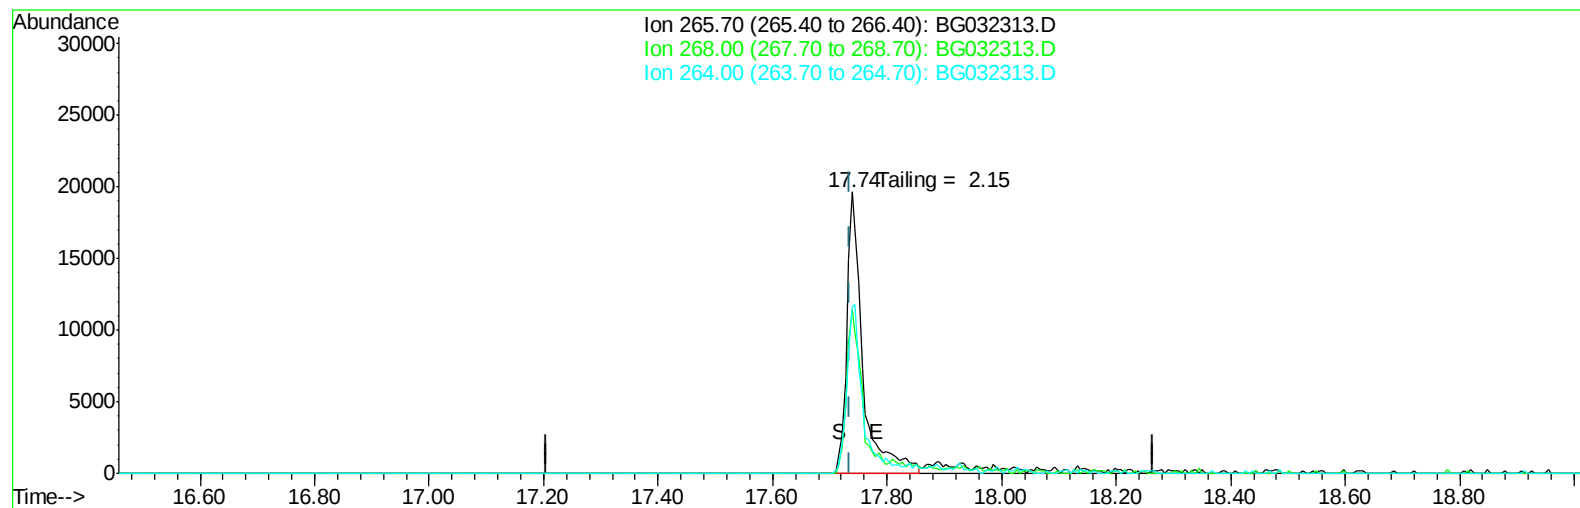

TIC: BG032313.D

(69) Pentachlorophenol (C)

17.739min (+0.002) 12005.04ng

response 38532

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.38
264.00	62.00	58.99
0.00	0.00	0.00