

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
 Data File : BG032298.D
 Acq On : 25 Jan 2018 18:02
 Operator : SJ/JU
 Sample : PB106006BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB106006BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.155	481	488	505	rVB	443325	753216	21.72%	5.539%
2	7.836	765	774	783	rBV	428176	785705	22.66%	5.778%
3	8.235	834	842	854	rBV	467740	847415	24.44%	6.232%
4	8.723	918	925	934	rVB	99776	175658	5.07%	1.292%
5	9.058	973	982	991	rBV	386164	698555	20.15%	5.137%
6	9.916	1120	1128	1139	rBV	255458	488447	14.09%	3.592%
7	11.602	1406	1415	1426	rBV	133152	241909	6.98%	1.779%
8	13.982	1813	1820	1830	rBV	1031976	1658458	47.83%	12.196%
9	15.356	2047	2054	2062	rBV2	262671	421596	12.16%	3.100%
10	16.831	2298	2305	2317	rBV	981759	1590897	45.88%	11.700%
11	18.089	2512	2519	2527	rVB2	404163	651654	18.79%	4.792%
12	20.627	2943	2951	2961	rBV	2625064	3467496	100.00%	25.500%
13	22.419	3247	3256	3267	rBV2	482858	896578	25.86%	6.593%
14	26.097	3867	3882	3895	rBV2	282373	920328	26.54%	6.768%


Sum of corrected areas: 13597912

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032298.D
Acq On : 25 Jan 2018 18:02
Operator : SJ/JU
Sample : PB106006BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106006BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

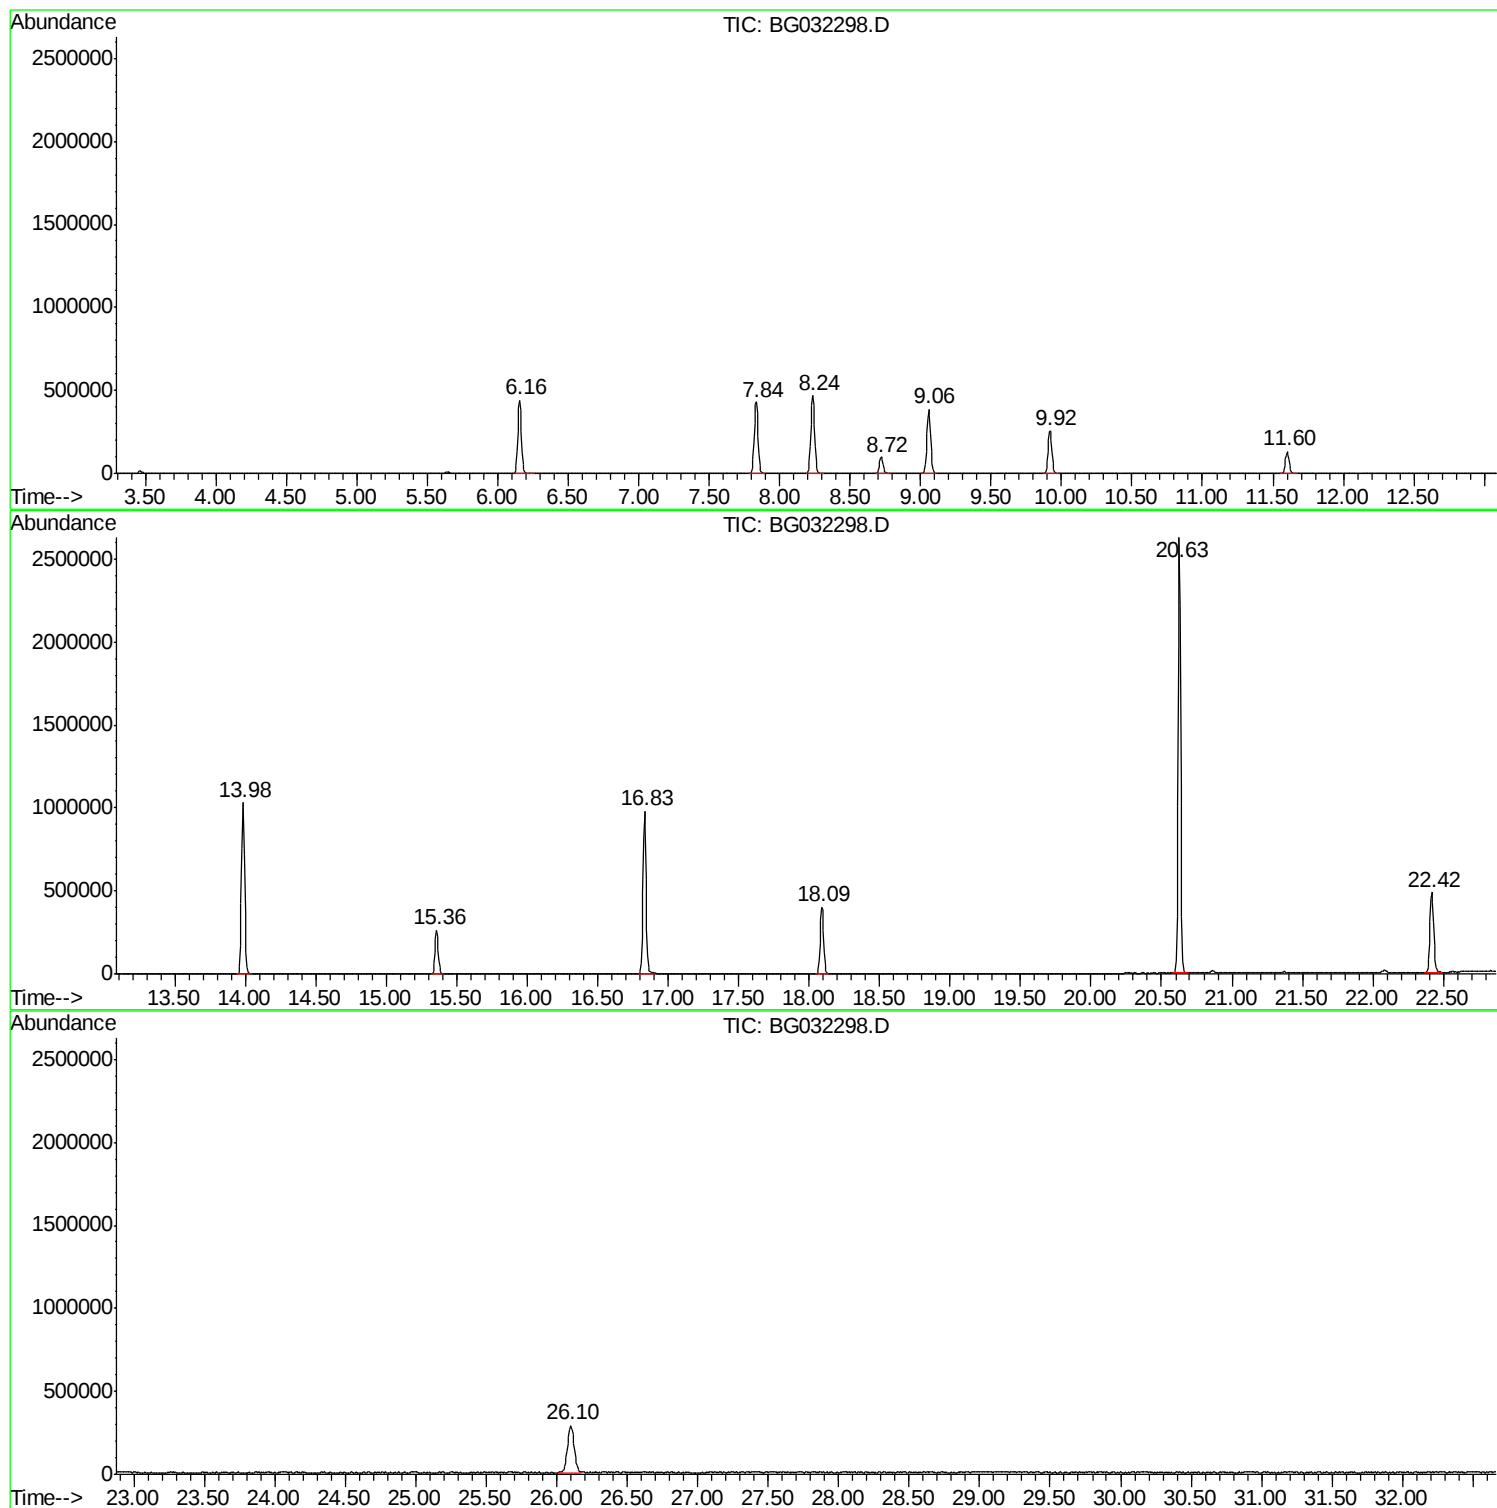

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032298.D
Acq On : 25 Jan 2018 18:02
Operator : SJ/JU
Sample : PB106006BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106006BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.24 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.24	96.48 ng	847415	1,4-Dichlorobenzene-d4	8.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12

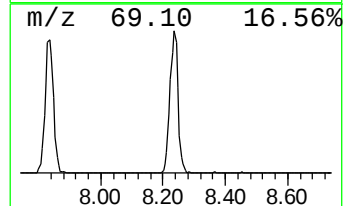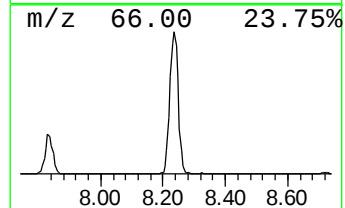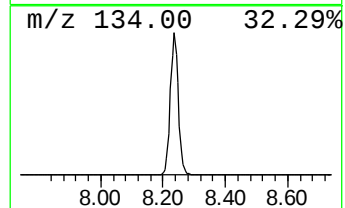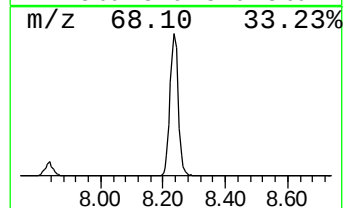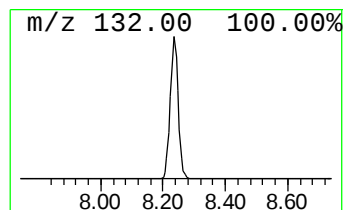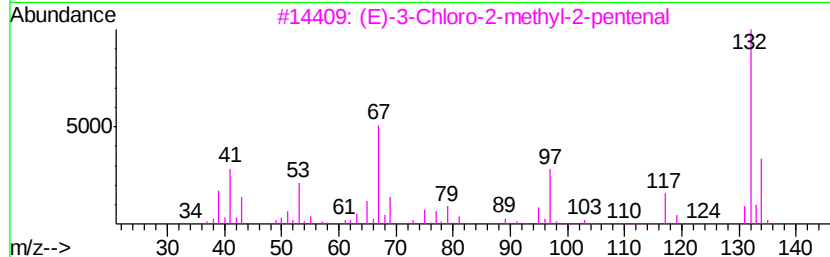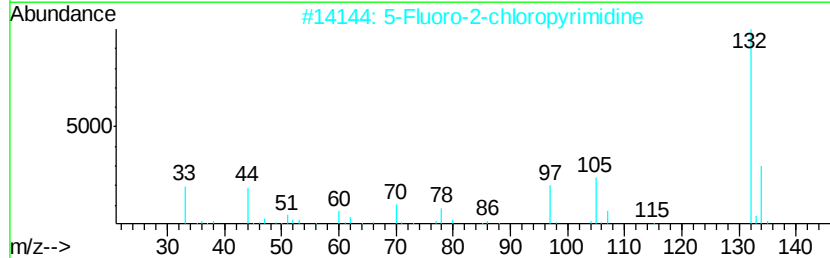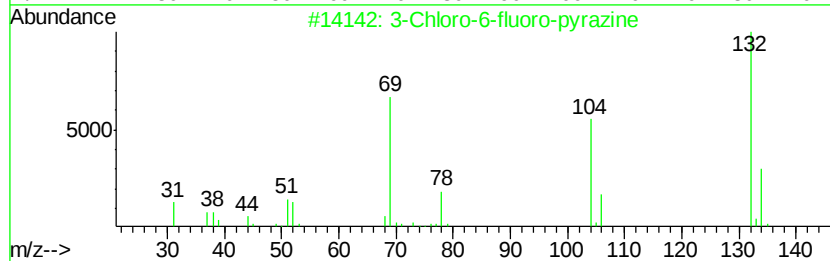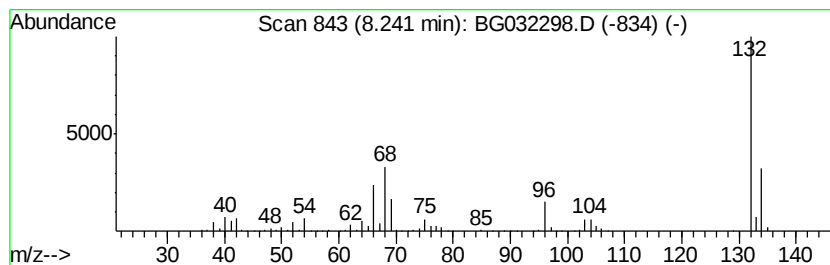

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012518\
Data File : BG032298.D
Acq On : 25 Jan 2018 18:02
Operator : SJ/JU
Sample : PB106006BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106006BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.24	8.24	96.5	ng	847415	1	8.72	175658	20.0