

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
 Data File : BG032311.D
 Acq On : 26 Jan 2018 2:11
 Operator : SJ/JU
 Sample : PB105983BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB105983BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.155	480	488	499	rBV	440528	736458	22.57%	5.716%
2	7.835	766	774	784	rBV	408050	758351	23.24%	5.886%
3	8.235	834	842	853	rBV	455080	824219	25.26%	6.397%
4	8.723	918	925	933	rVB	100801	182010	5.58%	1.413%
5	9.057	974	982	992	rBV	383390	699975	21.45%	5.432%
6	9.915	1120	1128	1140	rBB	250456	475334	14.57%	3.689%
7	11.602	1407	1415	1424	rBV	132116	247957	7.60%	1.924%
8	13.981	1812	1820	1832	rBV	1002732	1576750	48.33%	12.237%
9	15.356	2047	2054	2066	rBV2	253222	414354	12.70%	3.216%
10	16.831	2297	2305	2323	rBV	829175	1321485	40.50%	10.256%
11	18.088	2512	2519	2528	rBV2	407729	632440	19.38%	4.908%
12	20.626	2945	2951	2965	rBV	2429863	3262738	100.00%	25.322%
13	22.418	3248	3256	3267	rBV2	460791	851936	26.11%	6.612%
14	26.096	3868	3882	3900	rBV2	283706	900956	27.61%	6.992%


Sum of corrected areas: 12884963

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032311.D
Acq On : 26 Jan 2018 2:11
Operator : SJ/JU
Sample : PB105983BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105983BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

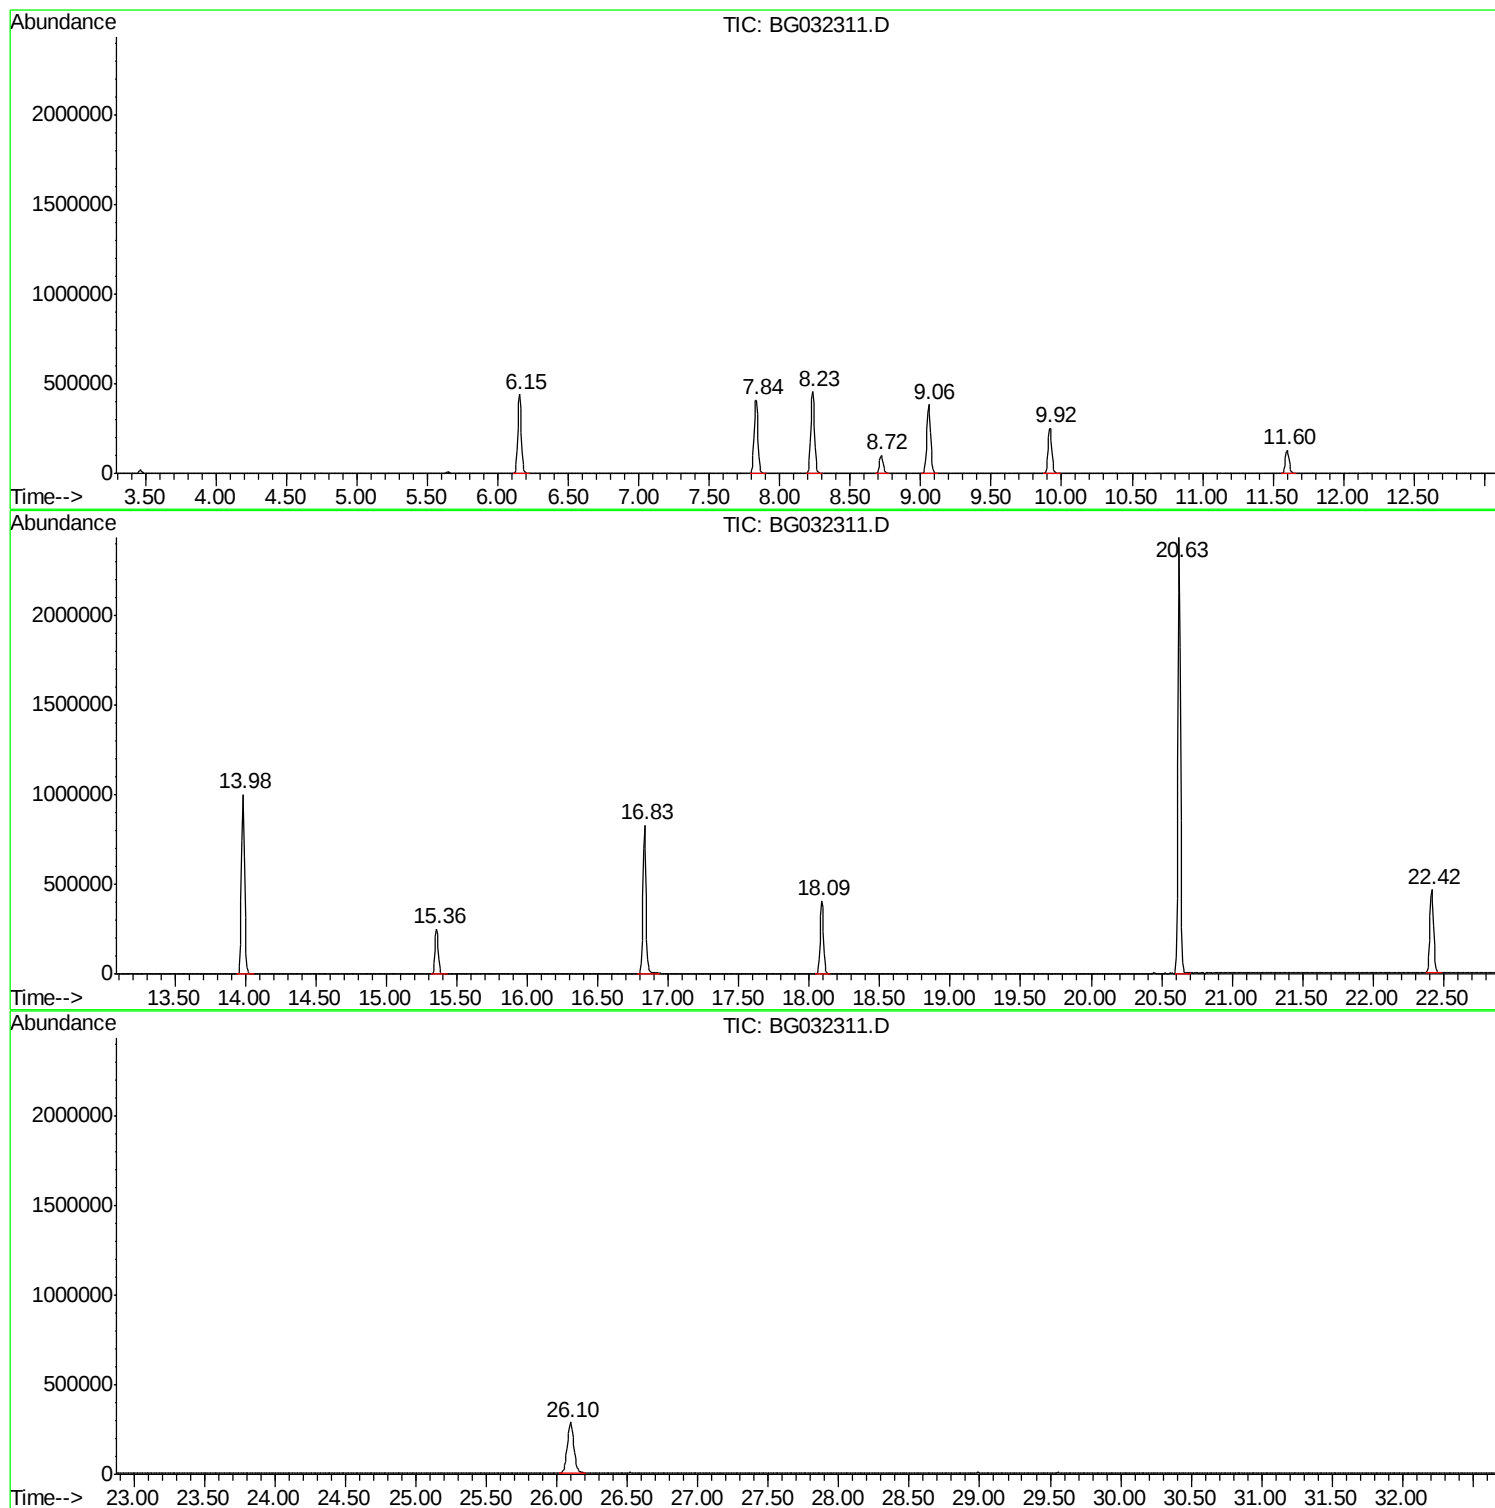

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032311.D
Acq On : 26 Jan 2018 2:11
Operator : SJ/JU
Sample : PB105983BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105983BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.23 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.23	90.57 ng	824219	1,4-Dichlorobenzene-d4	8.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	25
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	12
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12

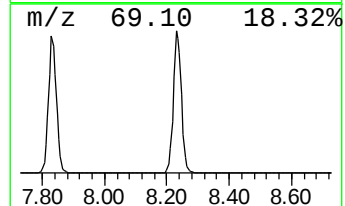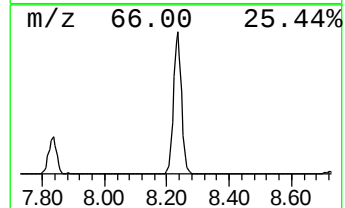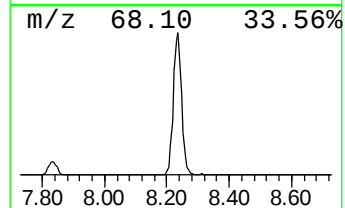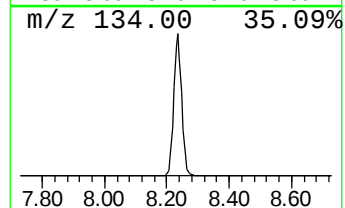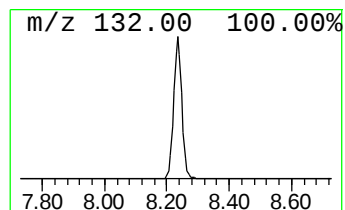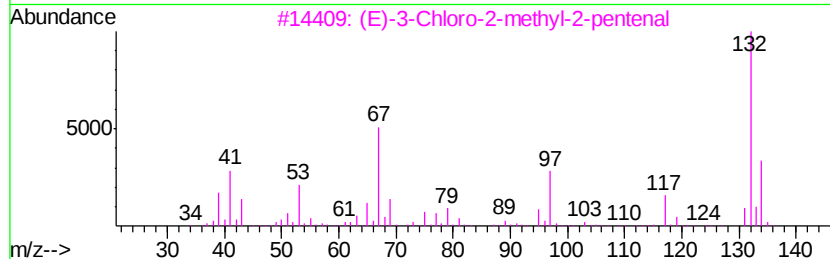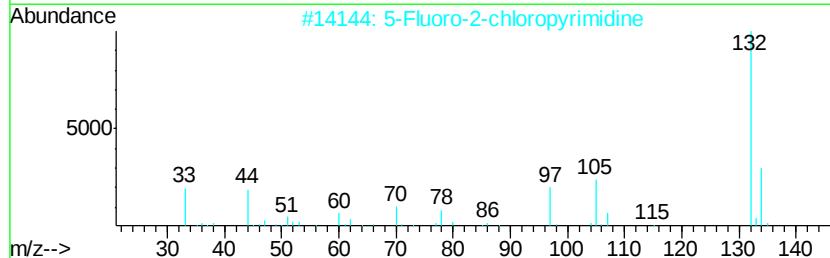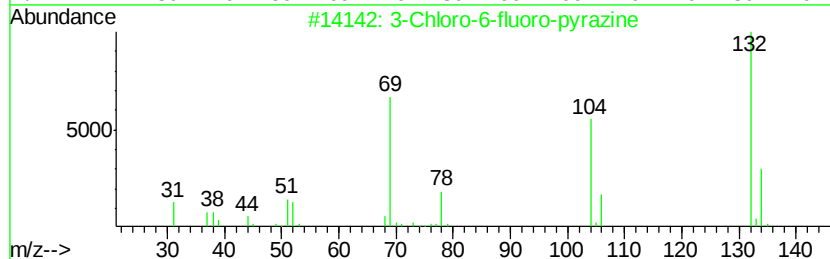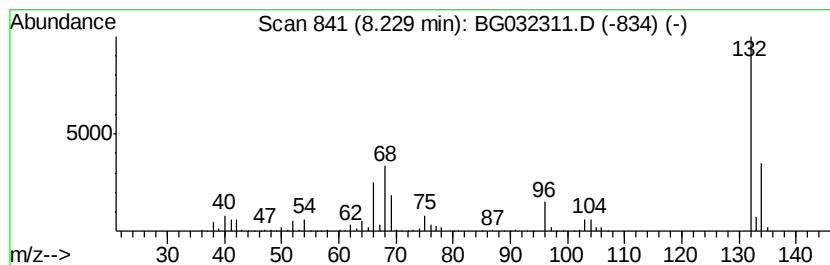

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012518\
Data File : BG032311.D
Acq On : 26 Jan 2018 2:11
Operator : SJ/JU
Sample : PB105983BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105983BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.23	8.23	90.6	ng	824219	1	8.72	182010	20.0