

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032329.D
Acq On : 26 Jan 2018 14:09
Operator : SJ/JU
Sample : PB106006TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106006TB

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.150	480	487	502	rBB	339376	584815	20.10%	5.269%
2	7.831	765	773	786	rBV	345115	622546	21.39%	5.609%
3	8.236	834	842	853	rVB	355590	657646	22.60%	5.925%
4	8.724	917	925	934	rBV	81582	147756	5.08%	1.331%
5	9.053	974	981	991	rBV	289751	549924	18.90%	4.955%
6	9.916	1120	1128	1138	rBV	207141	378720	13.01%	3.412%
7	11.603	1408	1415	1422	rBV	111603	205211	7.05%	1.849%
8	13.982	1813	1820	1833	rBV	846366	1316873	45.25%	11.864%
9	15.357	2045	2054	2064	rBB2	220601	365211	12.55%	3.290%
10	16.832	2298	2305	2320	rBV	703373	1170924	40.24%	10.549%
11	18.089	2512	2519	2528	rBV2	375748	579001	19.90%	5.217%
12	20.622	2944	2950	2963	rBV	2054168	2910083	100.00%	26.218%
13	22.414	3247	3255	3265	rBV2	437526	793273	27.26%	7.147%
14	26.092	3869	3881	3896	rBV2	260302	817371	28.09%	7.364%


Sum of corrected areas: 11099354

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
Data File : BG032329.D
Acq On : 26 Jan 2018 14:09
Operator : SJ/JU
Sample : PB106006TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106006TB

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

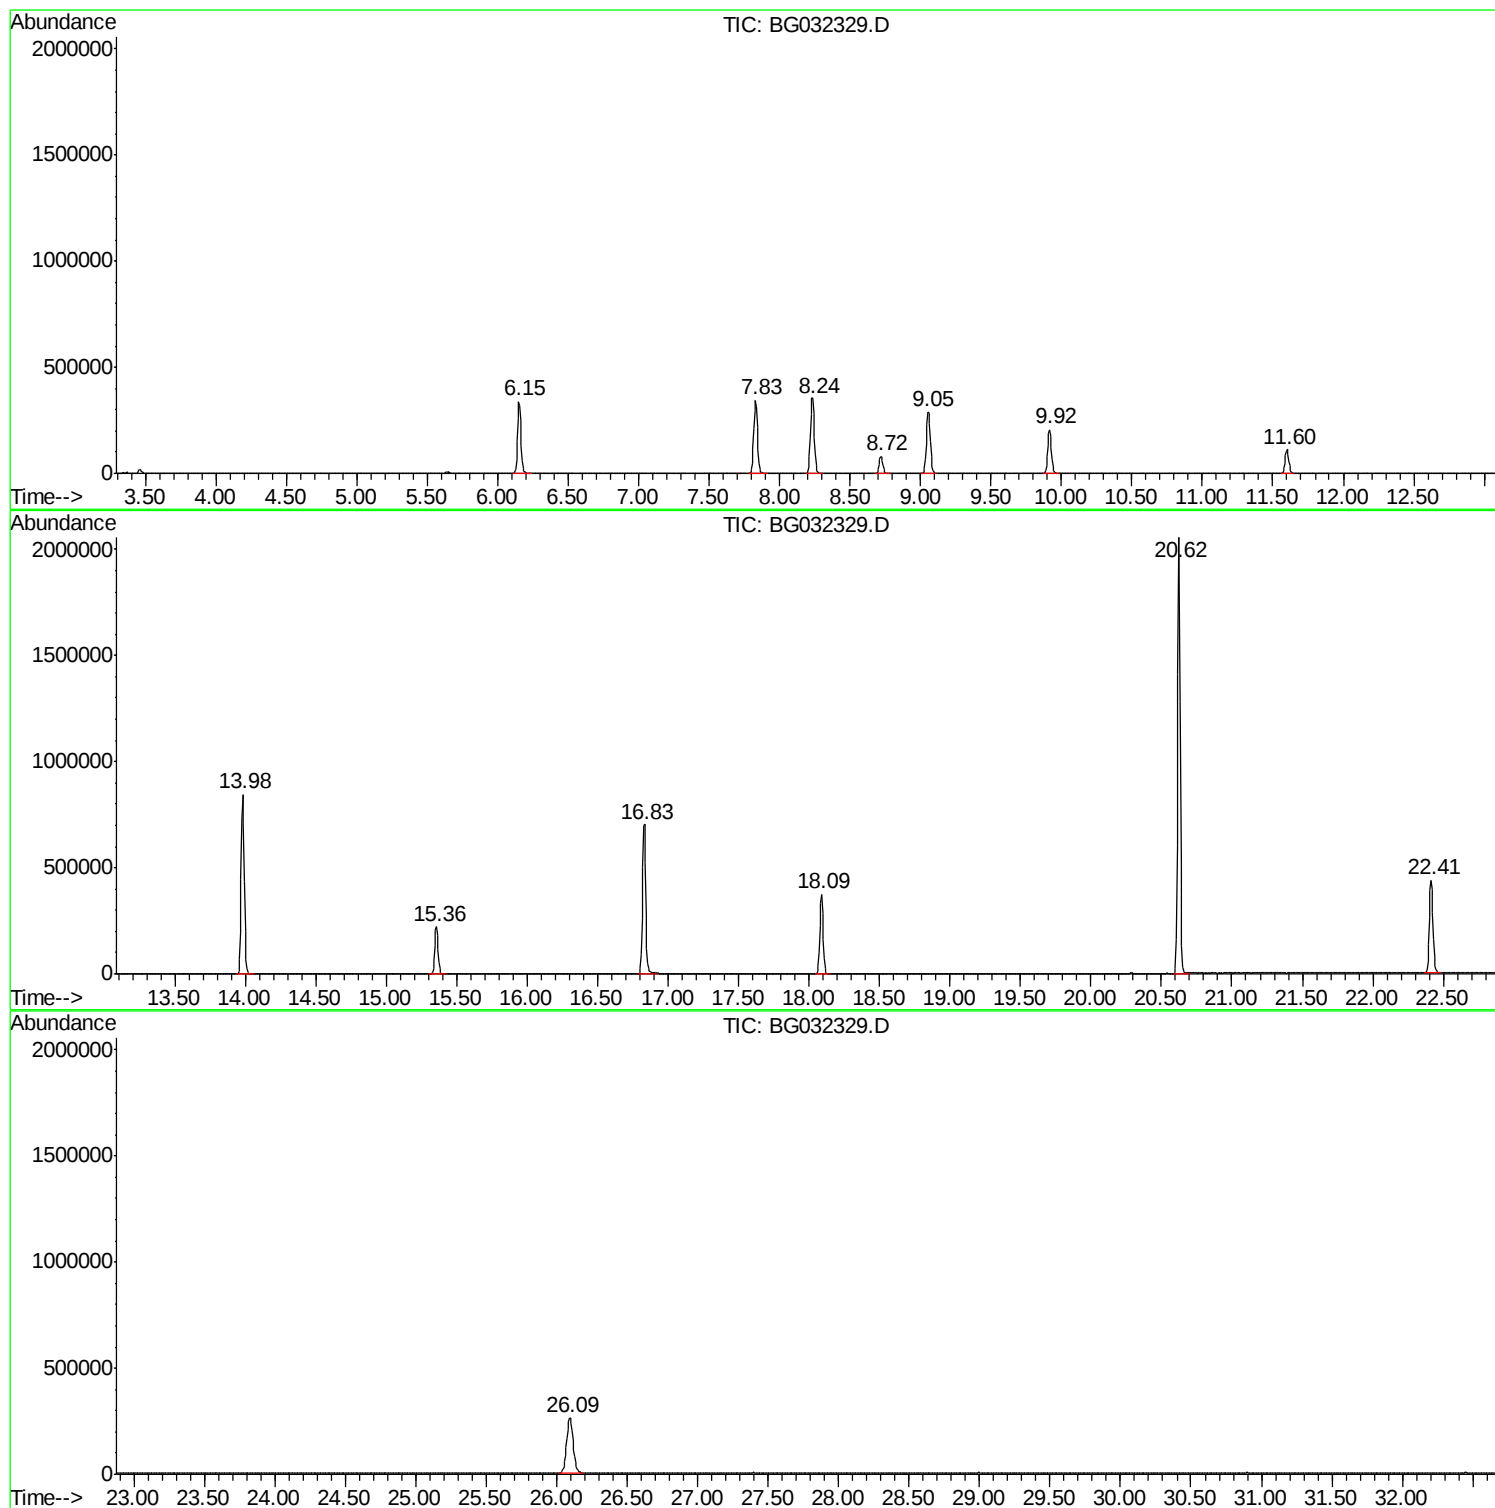

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG012518\
Data_File : BG032329.D
Acq_On : 26 Jan 2018 14:099
Operator : SJ/JUU
Sample : PB106006TBB
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB106006TB

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
