


Data Path : Z:\HPCHEM1\BNA G\DATA\BG012518\
 Data File : BG032295.D
 Acq On : 25 Jan 2018 15:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

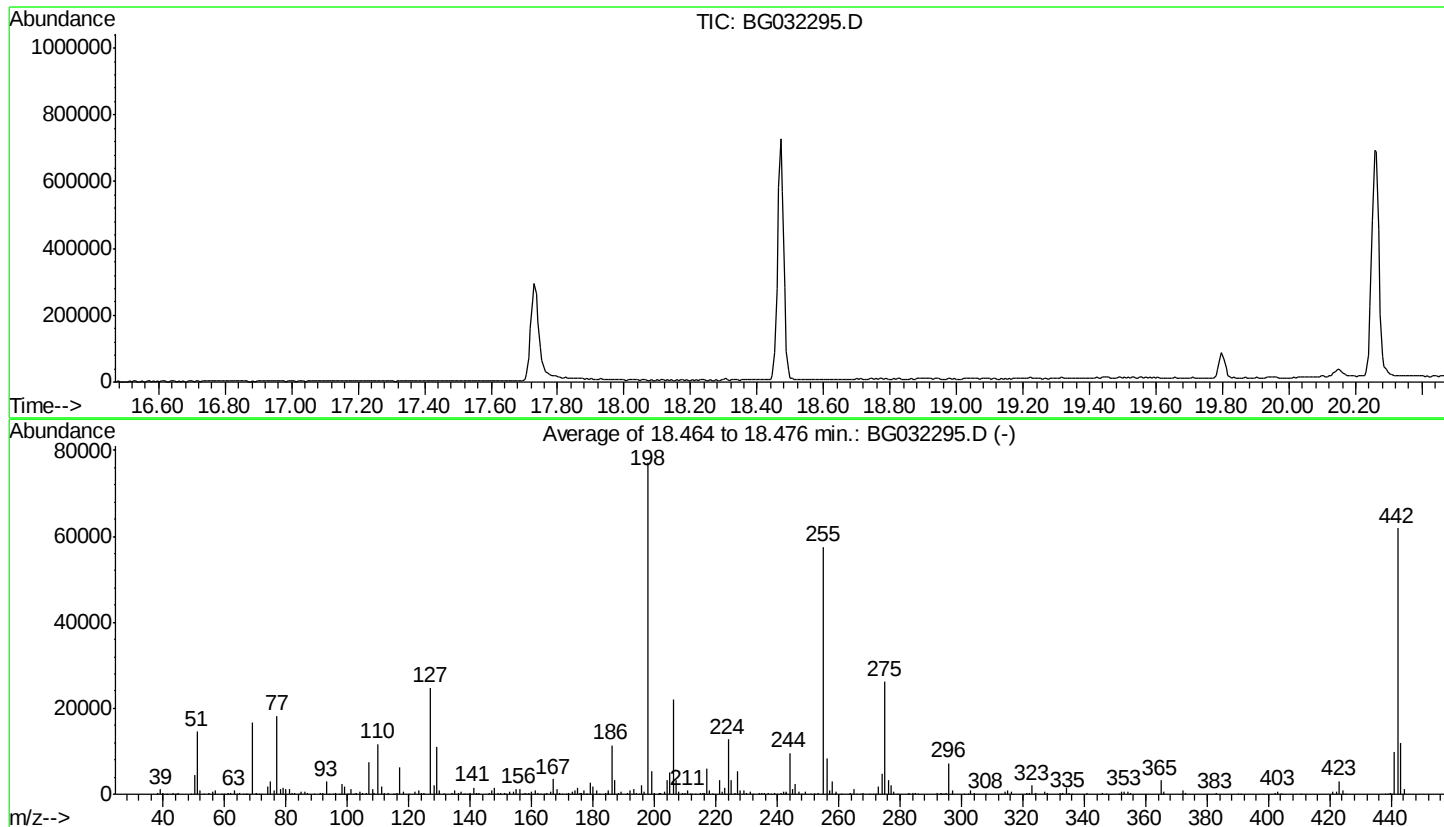

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.9	14575	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.7	16725	PASS
70	69	0.00	2	1.5	256	PASS
127	198	10	80	32.2	24837	PASS
197	198	0.00	2	0.7	536	PASS
198	198	100	100	100.0	77152	PASS
199	198	5	9	7.1	5471	PASS
275	198	10	60	33.8	26080	PASS
365	198	1	100	4.1	3176	PASS
441	442	0.01	24	16.0	9861	PASS
442	198	50	100	80.1	61810	PASS
443	442	15	24	19.5	12069	PASS