
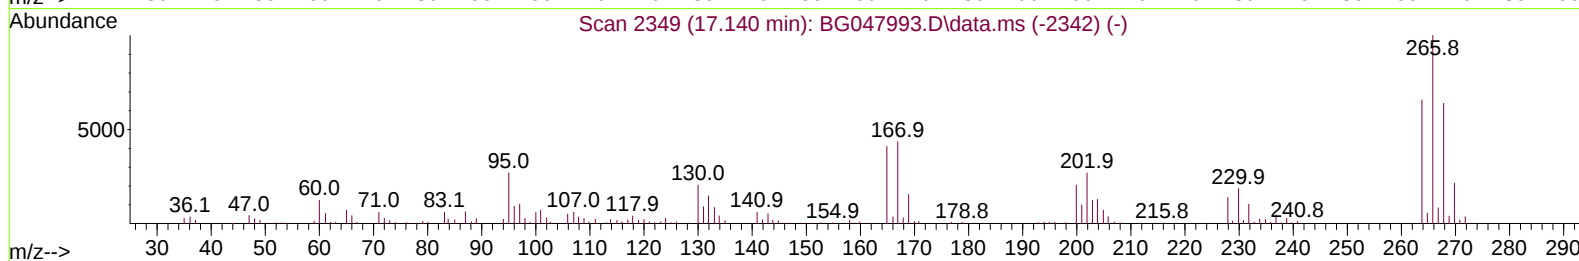
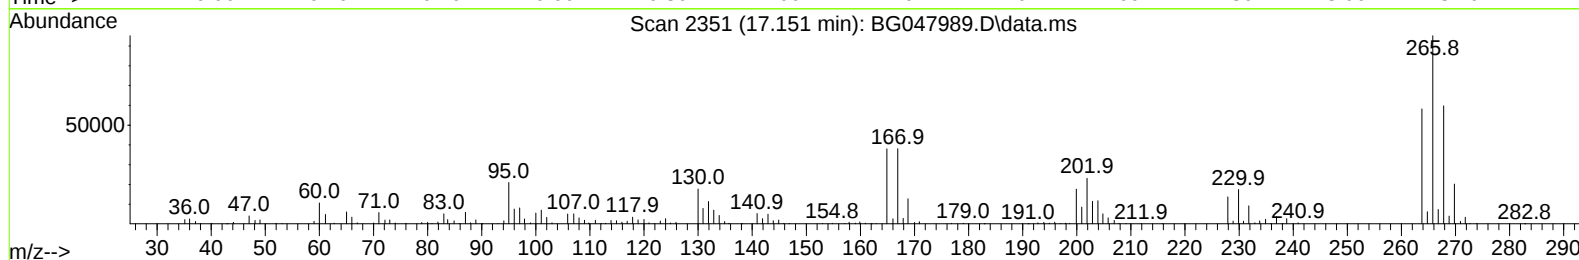


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012521\
Data File : BG047989.D
Acq On : 25 Jan 2021 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 00:45:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

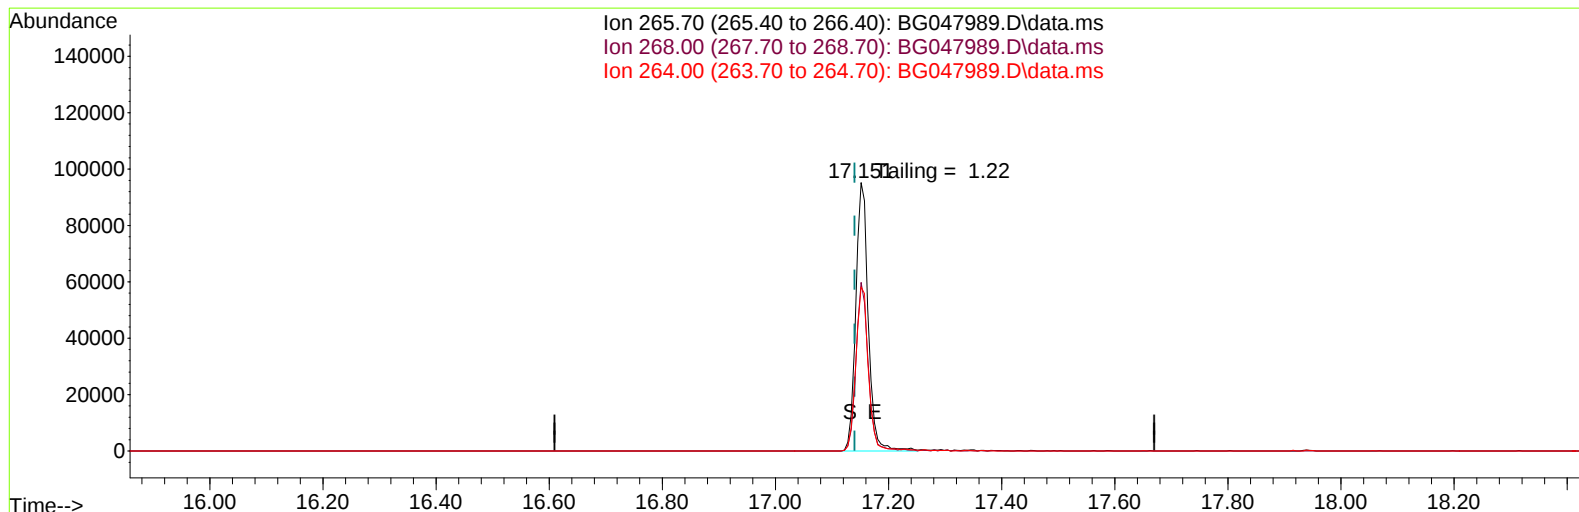

TIC: BG047989.D\data.ms

(70) Pentachlorophenol (C)




17.151min (+ 0.012) 279086.26 ng

response 145293

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.81
264.00	61.60	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012521\
Data File : BG047989.D
Acq On : 25 Jan 2021 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 00:45:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

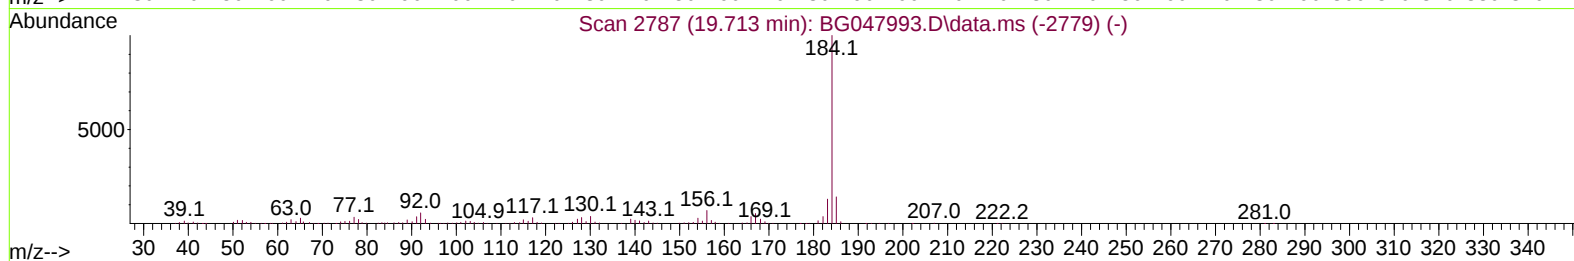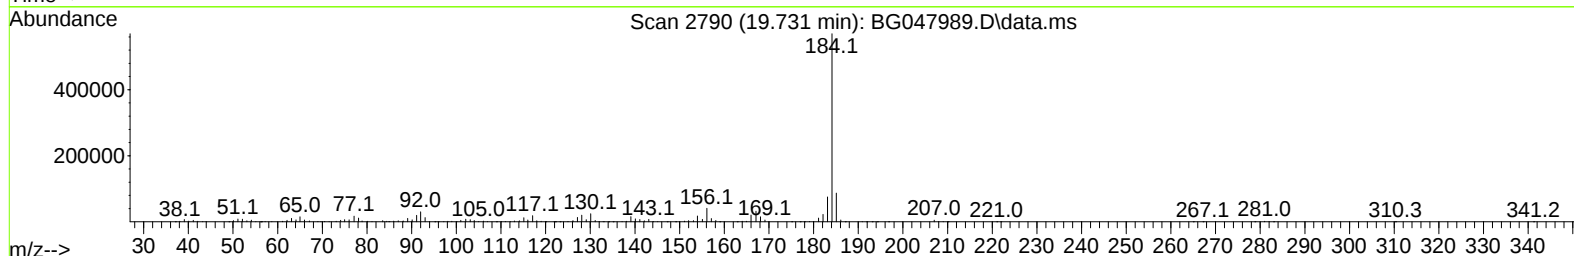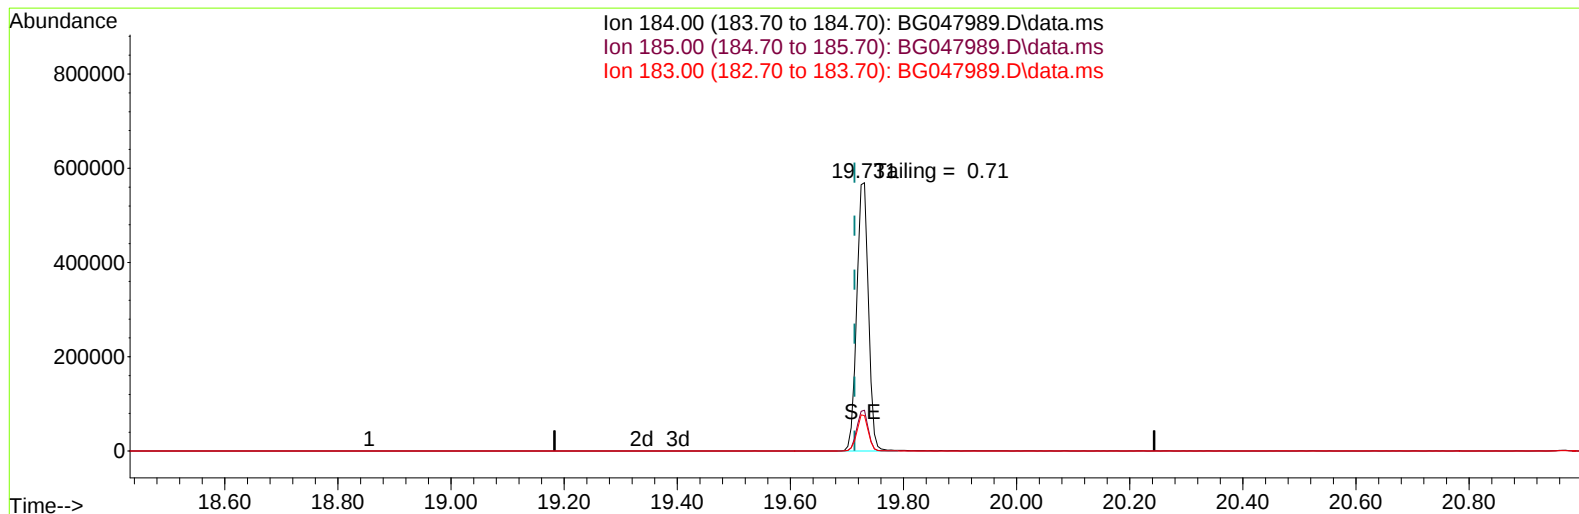

TIC: BG047989.D\data.ms

(77) Benzidine

19.731min (+ 0.018) 4375.46 ng m

response 823481

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.23
183.00	13.20	13.18
0.00	0.00	0.00