
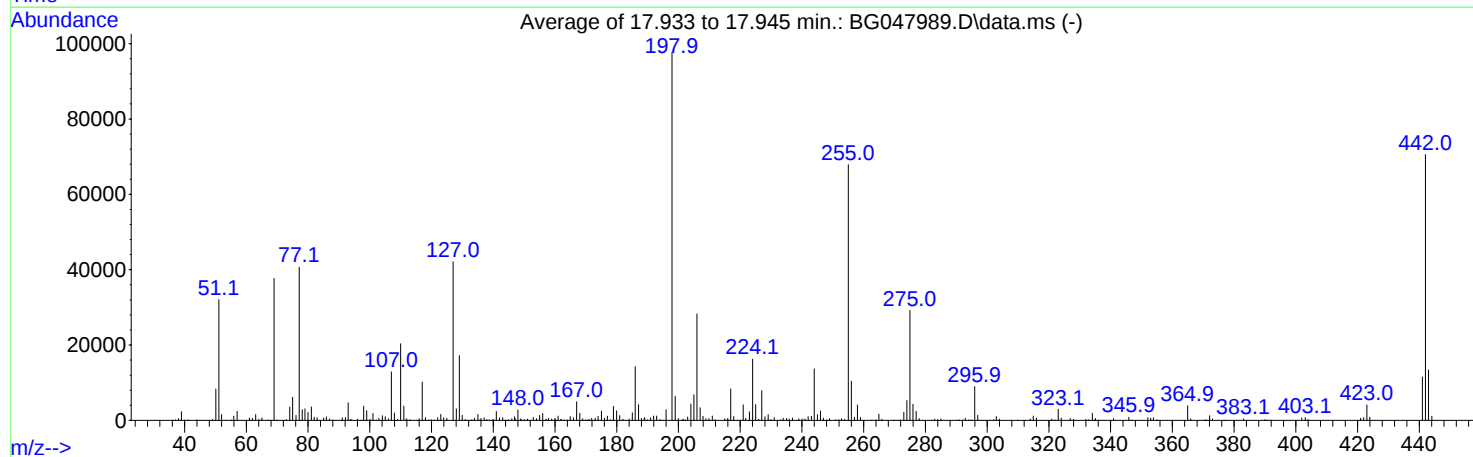


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012521\
 Data File : BG047989.D
 Acq On : 25 Jan 2021 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 19:39:42 2021

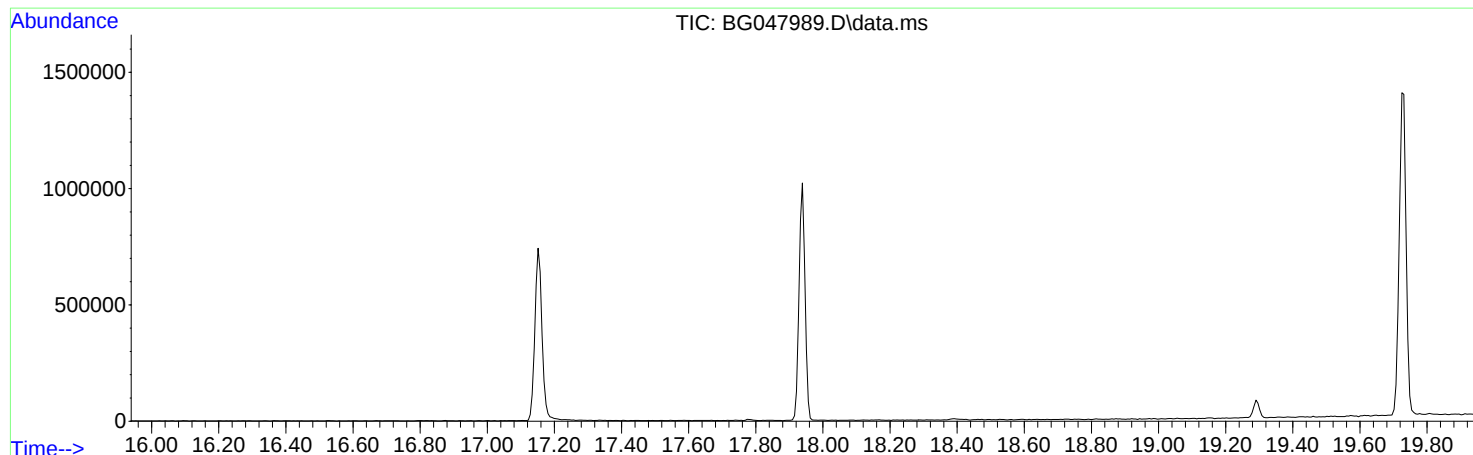

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	32053	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	37675	PASS
70	69	0.00	2	0.4	142	PASS
127	198	10	80	43.1	42072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97651	PASS
199	198	5	9	6.6	6403	PASS
275	198	10	60	29.9	29171	PASS
365	198	1	100	3.9	3852	PASS
441	198	0.01	100	11.8	11518	PASS
442	198	50	100	72.3	70571	PASS
443	442	15	24	19.0	13384	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2021	BNA_G	<u>BG047989.D</u>
Compound Name	Response	Retention Time
DDT	421605	20.965
DDD	7375	20.518
DDE	811	20.019
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8186	429791	1.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012521\
Data File : BG047989.D
Acq On : 25 Jan 2021 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 27 00:45:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

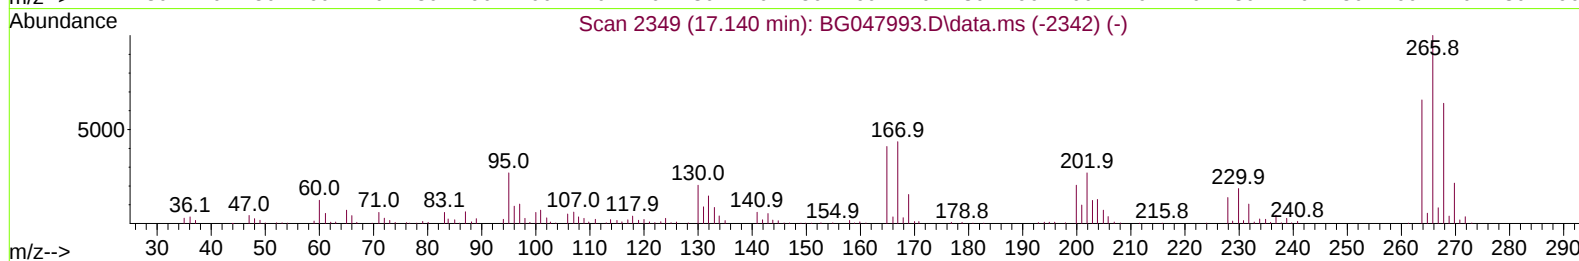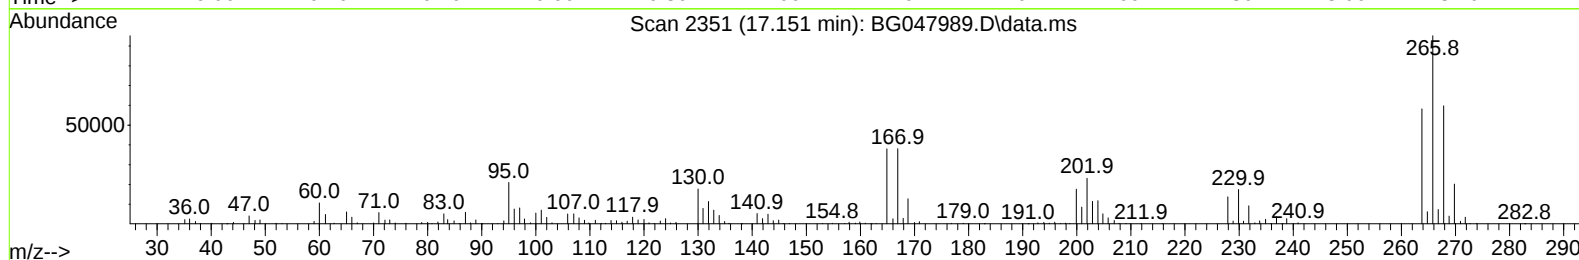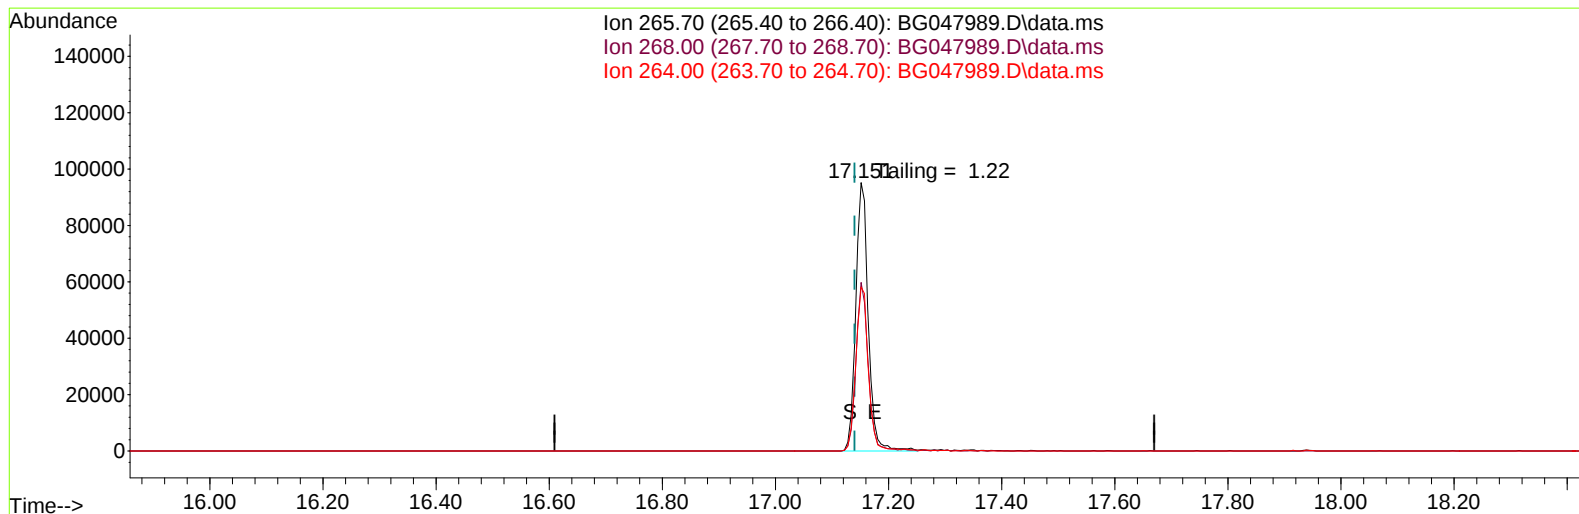

TIC: BG047989.D\data.ms

(70) Pentachlorophenol (C)

17.151min (+ 0.012) 279086.26 ng




response 145293

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.81
264.00	61.60	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012521\
 Data File : BG047989.D
 Acq On : 25 Jan 2021 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 27 00:45:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 25 19:39:42 2021
 Response via : Initial Calibration

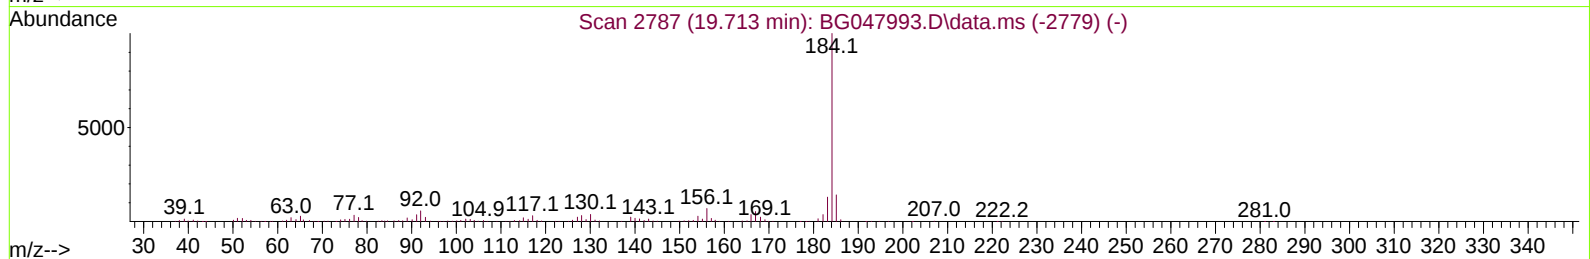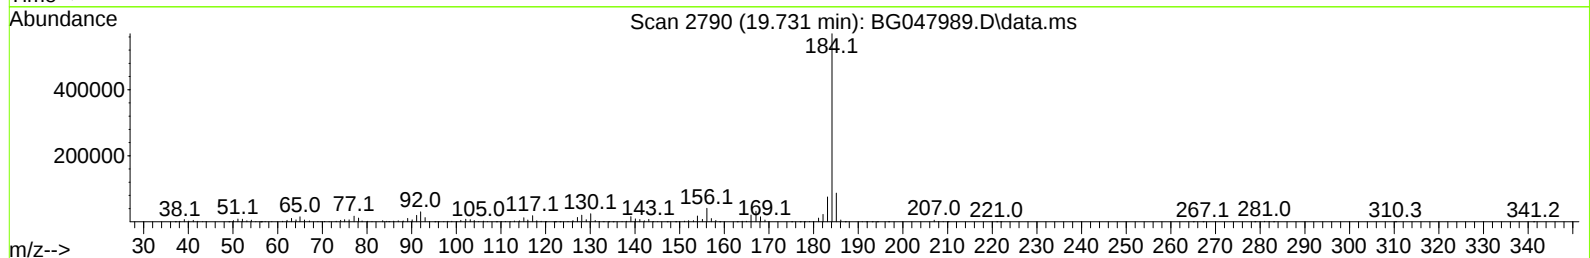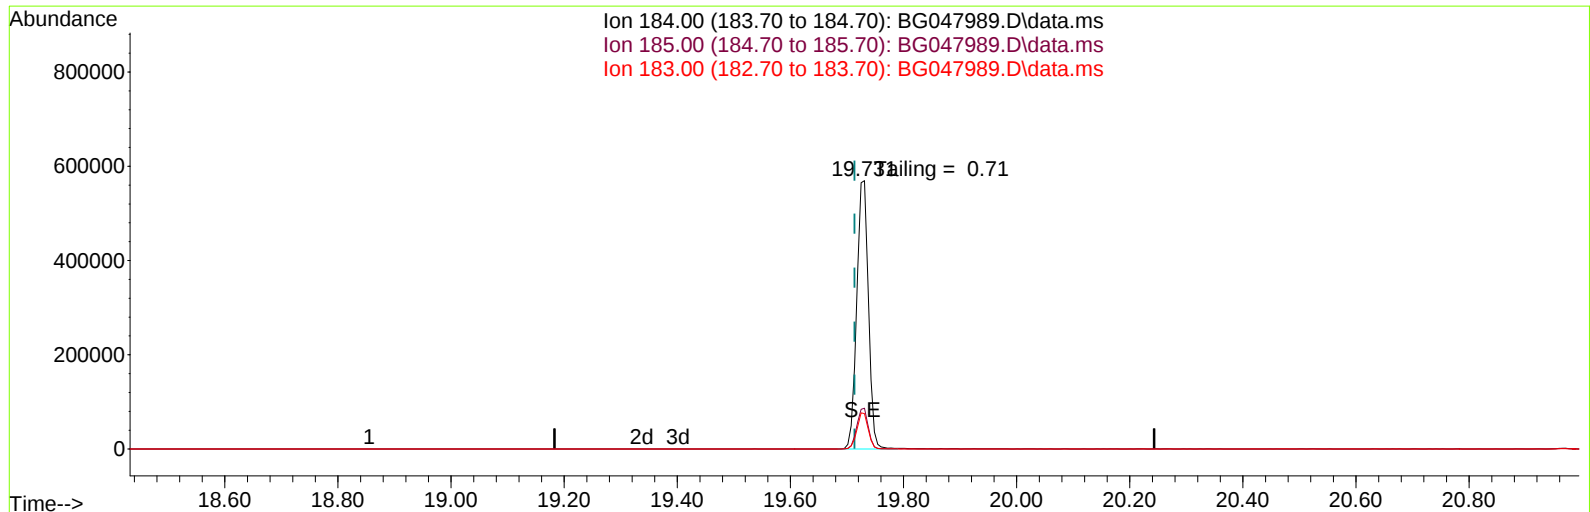

TIC: BG047989.D\data.ms

(77) Benzidine

19.731min (+ 0.018) 4375.46 ng m

response 823481

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.23
183.00	13.20	13.18
0.00	0.00	0.00