

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052139.D
 Acq On : 25 Jan 2022 11:15
 Operator : CG/JU
 Sample : PB142203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.578	10	15	21	rVV2	8301	12226	1.21%	0.121%
2	4.007	83	88	104	rBV	109029	191422	18.88%	1.896%
3	4.359	146	148	155	rBV3	2249	2354	0.23%	0.023%
4	7.402	659	666	674	rBV	157286	270621	26.69%	2.680%
5	7.566	686	694	703	rBV	104086	173050	17.07%	1.714%
6	7.784	725	731	741	rVB	137894	243303	24.00%	2.410%
7	8.260	802	812	818	rBV	94065	156096	15.40%	1.546%
8	8.965	923	932	940	rBV	189600	323005	31.86%	3.199%
9	9.429	1004	1011	1019	rBV	141835	253603	25.01%	2.512%
10	10.163	1129	1136	1142	rBV	125385	222703	21.96%	2.206%
11	10.709	1222	1229	1238	rVV	190849	342294	33.76%	3.390%
12	11.097	1286	1295	1302	rBV	134785	240519	23.72%	2.382%
13	11.220	1309	1316	1325	rBV	174523	329179	32.47%	3.260%
14	12.671	1558	1563	1568	rVB3	2814	4262	0.42%	0.042%
15	14.287	1831	1838	1846	rBV	368790	535156	52.78%	5.301%
16	14.592	1878	1890	1898	rBV	420698	640913	63.21%	6.348%
17	14.898	1935	1942	1948	rBV	236402	364925	35.99%	3.615%
18	15.080	1965	1973	1982	rBV	130926	241047	23.77%	2.388%
19	15.885	2101	2110	2118	rVB	538616	792202	78.13%	7.847%
20	15.990	2122	2128	2140	rBV	115666	177018	17.46%	1.753%
21	16.120	2146	2150	2154	rVB2	2879	3446	0.34%	0.034%
22	17.430	2370	2373	2377	rVB2	2003	2672	0.26%	0.026%
23	17.647	2403	2410	2417	rBV	297531	465961	45.96%	4.615%
24	17.741	2420	2426	2434	rVB2	566281	875347	86.33%	8.670%
25	19.591	2736	2741	2745	rBV3	7120	10297	1.02%	0.102%
26	19.656	2748	2752	2758	rVV	7190	9804	0.97%	0.097%
27	19.932	2796	2799	2802	rBV4	1287	2061	0.20%	0.020%
28	20.020	2807	2814	2821	rVV	753702	1013908	100.00%	10.043%
29	20.091	2823	2826	2829	rVB5	2075	2774	0.27%	0.027%
30	20.332	2864	2867	2870	rVB4	2618	1919	0.19%	0.019%
31	20.719	2931	2933	2935	rVB2	2352	1916	0.19%	0.019%
32	20.743	2935	2937	2940	rBV3	2197	2379	0.23%	0.024%
33	20.937	2968	2970	2972	rBV2	1665	1792	0.18%	0.018%
34	21.224	3017	3019	3023	rBV5	1776	2293	0.23%	0.023%
35	21.377	3041	3045	3049	rBV6	2857	5201	0.51%	0.052%
36	21.471	3057	3061	3062	rVB3	1888	2123	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052139.D
 Acq On : 25 Jan 2022 11:15
 Operator : CG/JU
 Sample : PB142203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	21.718	3100	3103	3104	rBV3	2599	2582	0.25%	0.026%
38	21.771	3111	3112	3117	rVB4	2534	2605	0.26%	0.026%
39	21.894	3131	3133	3134	rBV2	2903	2308	0.23%	0.023%
40	21.959	3138	3144	3153	rVB	289297	496494	48.97%	4.918%
41	22.029	3153	3156	3159	rBV5	1892	2052	0.20%	0.020%
42	22.405	3218	3220	3222	rBV3	1878	1861	0.18%	0.018%
43	22.628	3255	3258	3259	rVB2	2903	2375	0.23%	0.024%
44	22.787	3282	3285	3286	rBV3	3411	3583	0.35%	0.035%
45	22.934	3308	3310	3312	rVB2	2360	1816	0.18%	0.018%
46	23.098	3333	3338	3339	rVB4	2098	3073	0.30%	0.030%
47	23.116	3339	3341	3345	rBV5	1997	2332	0.23%	0.023%
48	23.562	3413	3417	3422	rVB8	7009	13087	1.29%	0.130%
49	23.598	3422	3423	3425	rBV2	2094	1850	0.18%	0.018%
50	23.786	3453	3455	3459	rBV4	2096	2775	0.27%	0.027%
51	24.027	3494	3496	3498	rVB3	2494	2340	0.23%	0.023%
52	24.050	3498	3500	3502	rBV2	1463	1809	0.18%	0.018%
53	24.332	3546	3548	3551	rBV4	1805	2464	0.24%	0.024%
54	24.432	3559	3565	3573	rBV7	9012	22129	2.18%	0.219%
55	24.590	3590	3592	3593	rBV2	2720	2208	0.22%	0.022%
56	24.778	3622	3624	3626	rVB3	2267	1789	0.18%	0.018%
57	24.984	3657	3659	3661	rBV2	2478	1917	0.19%	0.019%
58	25.072	3672	3674	3676	rVB3	3115	1975	0.19%	0.020%
59	25.213	3685	3698	3710	rBV2	314638	967409	95.41%	9.582%
60	25.454	3728	3739	3756	rVB2	149843	508379	50.14%	5.035%
61	25.818	3800	3801	3803	rBV2	2800	1793	0.18%	0.018%
62	26.153	3857	3858	3860	rVV2	2339	1740	0.17%	0.017%
63	26.547	3923	3925	3927	rVB3	2483	2110	0.21%	0.021%
64	26.570	3927	3929	3930	rBV2	2441	1871	0.18%	0.019%
65	26.741	3951	3958	3964	rBV6	8915	23290	2.30%	0.231%
66	26.934	3990	3991	3995	rBV2	2239	2986	0.29%	0.030%
67	27.257	4043	4046	4050	rBV4	2778	4064	0.40%	0.040%
68	27.393	4067	4069	4071	rVB3	3037	2244	0.22%	0.022%
69	27.434	4073	4076	4078	rVV4	2780	2908	0.29%	0.029%
70	27.657	4113	4114	4117	rVB3	2999	2107	0.21%	0.021%
71	27.898	4154	4155	4160	rVV5	2265	2237	0.22%	0.022%
72	27.939	4160	4162	4164	rVV3	2556	2434	0.24%	0.024%
73	27.962	4164	4166	4168	rBV3	2792	1743	0.17%	0.017%
74	28.197	4203	4206	4207	rBV3	2753	2901	0.29%	0.029%
75	28.227	4207	4211	4214	rBV4	7324	12840	1.27%	0.127%
76	28.468	4250	4252	4253	rVB2	2836	1710	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052139.D
 Acq On : 25 Jan 2022 11:15
 Operator : CG/JU
 Sample : PB142203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	28.967	4336	4337	4340	rBV3	2245	1957	0.19%	0.019%
78	29.102	4358	4360	4363	rBV4	2190	3013	0.30%	0.030%
79	29.155	4365	4369	4372	rBV5	3252	3839	0.38%	0.038%
80	29.243	4381	4384	4386	rBV3	2056	2138	0.21%	0.021%
81	29.343	4398	4401	4402	rBV3	3448	2631	0.26%	0.026%
82	29.578	4438	4441	4442	rVB3	2693	2326	0.23%	0.023%
83	29.789	4475	4477	4478	rVB2	3031	1870	0.18%	0.019%
84	29.813	4478	4481	4483	rBV4	2411	3174	0.31%	0.031%
85	29.860	4486	4489	4491	rVB4	2035	1778	0.18%	0.018%
86	29.960	4505	4506	4510	rBV4	2528	2407	0.24%	0.024%
87	30.024	4515	4517	4518	rBV2	2593	1888	0.19%	0.019%
88	30.042	4518	4520	4522	rVV3	3389	2832	0.28%	0.028%
89	30.271	4557	4559	4565	rVB6	3280	3342	0.33%	0.033%
90	30.424	4583	4585	4588	rVB4	2751	2152	0.21%	0.021%
91	30.524	4600	4602	4606	rBV4	1645	2373	0.23%	0.024%
92	30.588	4611	4613	4616	rVV3	2626	2235	0.22%	0.022%
93	30.635	4619	4621	4623	rVB3	2207	1753	0.17%	0.017%
94	30.811	4648	4651	4653	rVV4	2056	1893	0.19%	0.019%
95	30.999	4682	4683	4686	rBV3	2117	1944	0.19%	0.019%
96	31.088	4695	4698	4699	rVB3	2766	2204	0.22%	0.022%
97	31.375	4745	4747	4751	rVB4	2260	2132	0.21%	0.021%
98	32.045	4859	4861	4863	rBV3	1711	1819	0.18%	0.018%
99	32.180	4882	4884	4885	rBV2	2477	1736	0.17%	0.017%
100	32.562	4947	4949	4952	rVV4	2218	2714	0.27%	0.027%




Sum of corrected areas: 10096131

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052139.D
Acq On : 25 Jan 2022 11:15
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

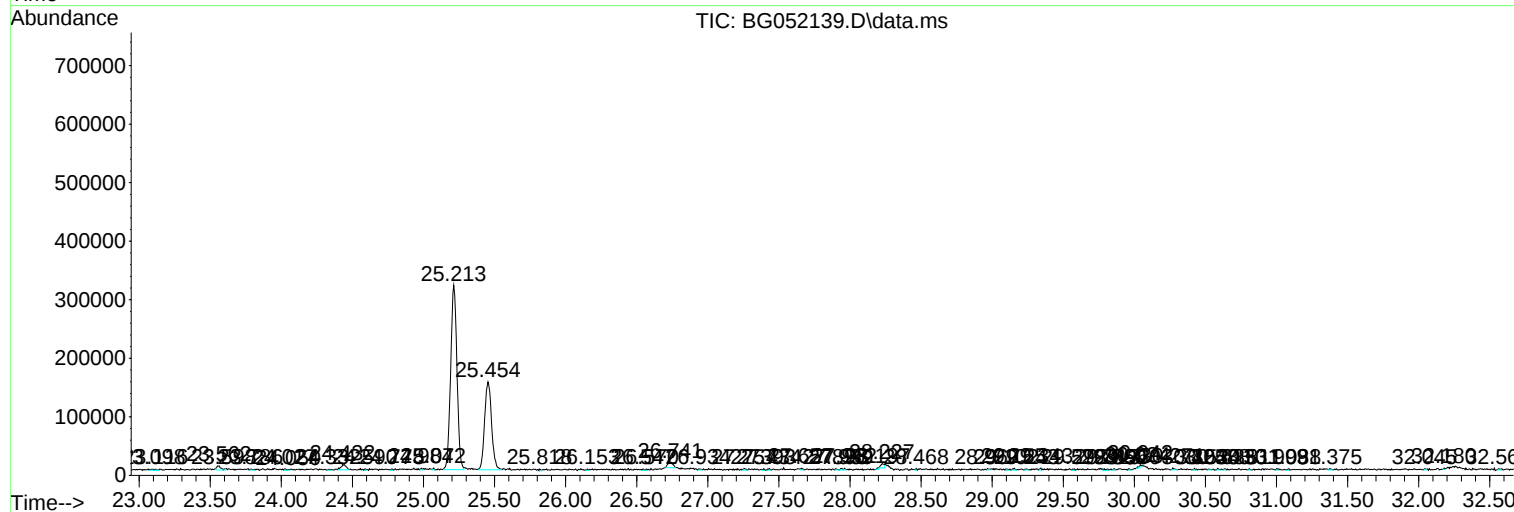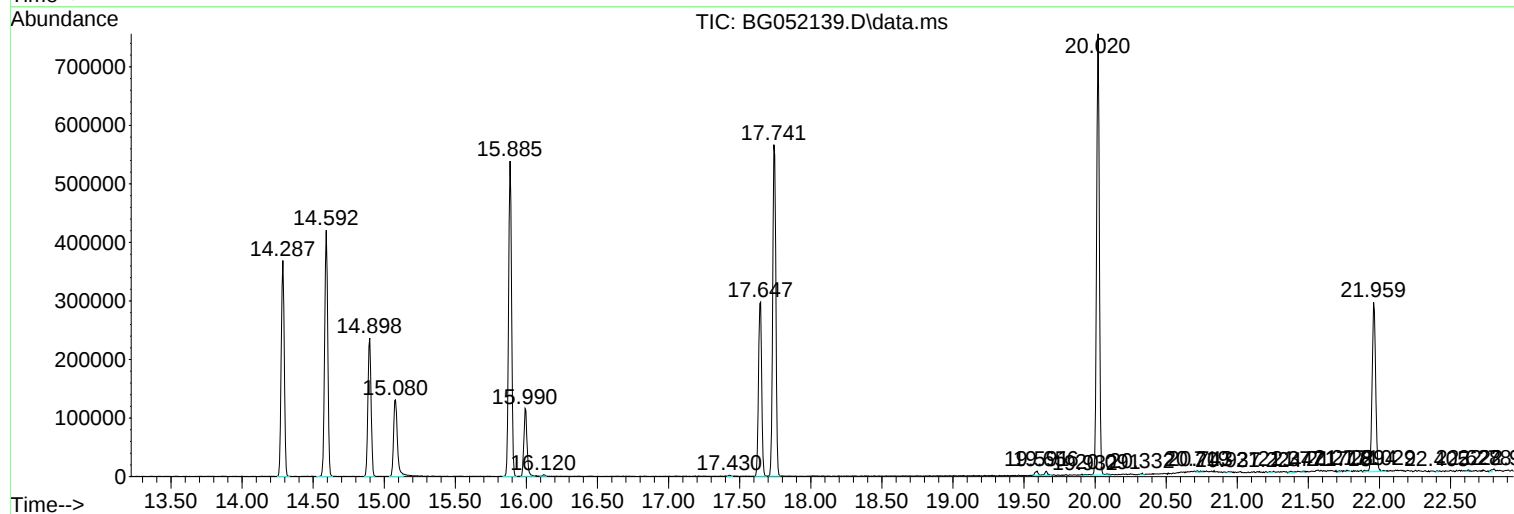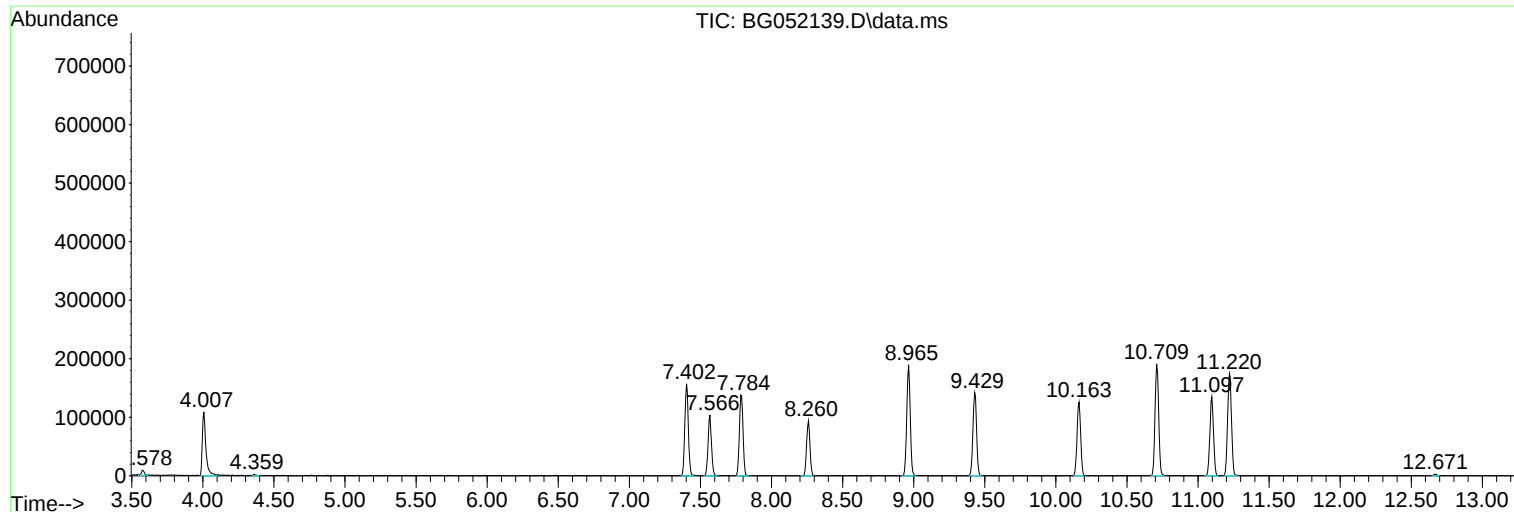

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052139.D
Acq On : 25 Jan 2022 11:15
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052139.D
Acq On : 25 Jan 2022 11:15
Operator : CG/JU
Sample : PB142203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK203

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc