

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052141.D
 Acq On : 25 Jan 2022 12:30
 Operator : CG/JU
 Sample : N1199-18DL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.769	46	48	49	rVB	1341	731	0.13%	0.021%
2	3.886	65	68	69	rVB2	1272	992	0.17%	0.028%
3	3.945	76	78	81	rVB	901	722	0.12%	0.020%
4	4.074	99	100	103	rVB	956	771	0.13%	0.022%
5	4.098	103	104	106	rBV	1060	780	0.13%	0.022%
6	4.198	119	121	124	rVB	1029	1136	0.20%	0.032%
7	4.233	124	127	128	rBV	756	898	0.16%	0.025%
8	4.350	143	147	148	rBV2	1697	1964	0.34%	0.055%
9	4.503	171	173	176	rVB	790	908	0.16%	0.026%
10	4.603	186	190	191	rVB	684	791	0.14%	0.022%
11	5.637	363	366	368	rBV	622	753	0.13%	0.021%
12	5.713	376	379	382	rBV2	944	1209	0.21%	0.034%
13	5.801	391	394	398	rBV	541	830	0.14%	0.023%
14	6.224	462	466	470	rVB3	1373	1669	0.29%	0.047%
15	6.959	588	591	595	rBB	644	751	0.13%	0.021%
16	7.399	664	666	670	rVB	1254	1098	0.19%	0.031%
17	7.552	687	692	696	rBV3	3244	5344	0.92%	0.151%
18	7.634	701	706	709	rBB	838	1075	0.19%	0.030%
19	7.775	725	730	736	rVB3	3376	4997	0.86%	0.141%
20	7.834	737	740	744	rBV	510	906	0.16%	0.026%
21	8.245	803	810	820	rVB	111116	184652	31.90%	5.205%
22	8.357	826	829	835	rVB2	1188	2057	0.36%	0.058%
23	8.621	872	874	881	rVB2	1305	1930	0.33%	0.054%
24	8.715	887	890	894	rBB2	576	945	0.16%	0.027%
25	8.950	925	930	935	rVB	1990	3395	0.59%	0.096%
26	9.050	943	947	950	rVB	762	1090	0.19%	0.031%
27	9.414	1004	1009	1014	rBV3	3869	6718	1.16%	0.189%
28	9.919	1092	1095	1098	rVB	598	798	0.14%	0.022%
29	10.013	1108	1111	1117	rBB	402	736	0.13%	0.021%
30	10.154	1128	1135	1138	rBV6	3146	5618	0.97%	0.158%
31	10.401	1174	1177	1181	rBB	585	735	0.13%	0.021%
32	10.466	1184	1188	1189	rBV	998	789	0.14%	0.022%
33	10.542	1198	1201	1205	rVB	746	724	0.13%	0.020%
34	10.624	1212	1215	1217	rBV	964	814	0.14%	0.023%
35	10.695	1222	1227	1240	rBV3	4675	9373	1.62%	0.264%
36	11.083	1286	1293	1300	rVB	168136	292512	50.53%	8.246%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052141.D
 Acq On : 25 Jan 2022 12:30
 Operator : CG/JU
 Sample : N1199-18DL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	11.206	1311	1314	1315	rBV	2674	2288	0.40%	0.064%
38	12.622	1552	1555	1558	rVB2	561	857	0.15%	0.024%
39	12.939	1603	1609	1615	rVB4	2203	4365	0.75%	0.123%
40	13.209	1652	1655	1658	rBV2	628	782	0.14%	0.022%
41	13.409	1681	1689	1695	rBV4	8645	15380	2.66%	0.434%
42	13.591	1715	1720	1728	rBV3	14837	23010	3.97%	0.649%
43	13.720	1738	1742	1749	rVB	3847	4300	0.74%	0.121%
44	13.908	1771	1774	1775	rVB2	979	822	0.14%	0.023%
45	13.943	1778	1780	1785	rVB3	1168	1214	0.21%	0.034%
46	14.272	1831	1836	1843	rVB	13687	18527	3.20%	0.522%
47	14.431	1859	1863	1864	rBV	901	987	0.17%	0.028%
48	14.578	1883	1888	1897	rVB	14291	23933	4.13%	0.675%
49	14.672	1901	1904	1907	rBV	869	910	0.16%	0.026%
50	14.889	1934	1941	1950	rVB	285663	449351	77.62%	12.667%
51	14.960	1950	1953	1954	rBV	1025	1134	0.20%	0.032%
52	15.283	2004	2008	2013	rVB	1415	1837	0.32%	0.052%
53	15.506	2041	2046	2055	rVB3	11142	17178	2.97%	0.484%
54	15.576	2055	2058	2062	rBV	600	943	0.16%	0.027%
55	15.876	2103	2109	2115	rBV	20815	28160	4.86%	0.794%
56	15.929	2115	2118	2123	rVV3	2300	3788	0.65%	0.107%
57	15.999	2125	2130	2138	rVV2	29960	48069	8.30%	1.355%
58	16.064	2138	2141	2143	rVB	1033	1018	0.18%	0.029%
59	16.651	2236	2241	2242	rBV2	657	1111	0.19%	0.031%
60	16.834	2271	2272	2277	rVB	620	1001	0.17%	0.028%
61	16.910	2282	2285	2291	rVB	950	2204	0.38%	0.062%
62	16.986	2297	2298	2301	rVB2	1363	897	0.15%	0.025%
63	17.010	2301	2302	2308	rBV	807	1006	0.17%	0.028%
64	17.227	2335	2339	2343	rBV	643	1036	0.18%	0.029%
65	17.286	2343	2349	2361	rBV	359064	559911	96.72%	15.784%
66	17.415	2369	2371	2377	rVB3	2017	2492	0.43%	0.070%
67	17.638	2402	2409	2420	rVB	338856	525044	90.70%	14.801%
68	17.732	2420	2425	2433	rVB2	21598	30665	5.30%	0.864%
69	17.832	2439	2442	2445	rBV	691	856	0.15%	0.024%
70	18.014	2469	2473	2475	rBV3	1221	1237	0.21%	0.035%
71	18.196	2501	2504	2507	rVB3	620	922	0.16%	0.026%
72	18.243	2507	2512	2514	rBV2	850	1520	0.26%	0.043%
73	18.396	2535	2538	2540	rBV2	944	988	0.17%	0.028%
74	18.984	2637	2638	2642	rVB2	1188	940	0.16%	0.026%
75	19.036	2645	2647	2649	rBV	875	757	0.13%	0.021%
76	19.177	2668	2671	2673	rBV2	1116	1230	0.21%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052141.D
 Acq On : 25 Jan 2022 12:30
 Operator : CG/JU
 Sample : N1199-18DL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q13DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	19.277	2687	2688	2691	rBV2	841	773	0.13%	0.022%
78	19.412	2709	2711	2714	rBV3	854	822	0.14%	0.023%
79	19.606	2742	2744	2747	rBV3	1181	1266	0.22%	0.036%
80	19.671	2752	2755	2756	rBV2	1587	1175	0.20%	0.033%
81	19.712	2760	2762	2763	rBV2	1537	1322	0.23%	0.037%
82	19.847	2783	2785	2786	rBV2	1409	1109	0.19%	0.031%
83	19.906	2793	2795	2798	rVB3	4794	4706	0.81%	0.133%
84	19.935	2798	2800	2801	rVB2	1360	804	0.14%	0.023%
85	19.947	2801	2802	2806	rBV3	1257	1708	0.30%	0.048%
86	20.012	2808	2813	2822	rVB2	24409	37745	6.52%	1.064%
87	20.135	2832	2834	2835	rBV2	1374	760	0.13%	0.021%
88	20.182	2840	2842	2845	rBV3	1749	2067	0.36%	0.058%
89	20.211	2845	2847	2849	rVV	1789	1104	0.19%	0.031%
90	20.305	2862	2863	2866	rBV2	1647	1291	0.22%	0.036%
91	20.517	2896	2899	2900	rBV3	2258	1937	0.33%	0.055%
92	20.852	2954	2956	2958	rBV3	2116	1196	0.21%	0.034%
93	20.928	2967	2969	2970	rBV2	2488	1650	0.29%	0.047%
94	21.057	2989	2991	2995	rBV3	2313	3187	0.55%	0.090%
95	21.956	3137	3144	3154	rVB2	319946	546995	94.49%	15.420%
96	22.385	3215	3217	3218	rVB2	3379	1964	0.34%	0.055%
97	24.423	3562	3564	3572	rVB7	11647	19076	3.30%	0.538%
98	25.440	3727	3737	3753	rVB2	175492	578877	100.00%	16.319%
99	26.708	3950	3953	3954	rBV3	9234	9901	1.71%	0.279%
100	26.797	3966	3968	3969	rBV	3129	2038	0.35%	0.057%




Sum of corrected areas: 3547354

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052141.D
Acq On : 25 Jan 2022 12:30
Operator : CG/JU
Sample : N1199-18DL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q13DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

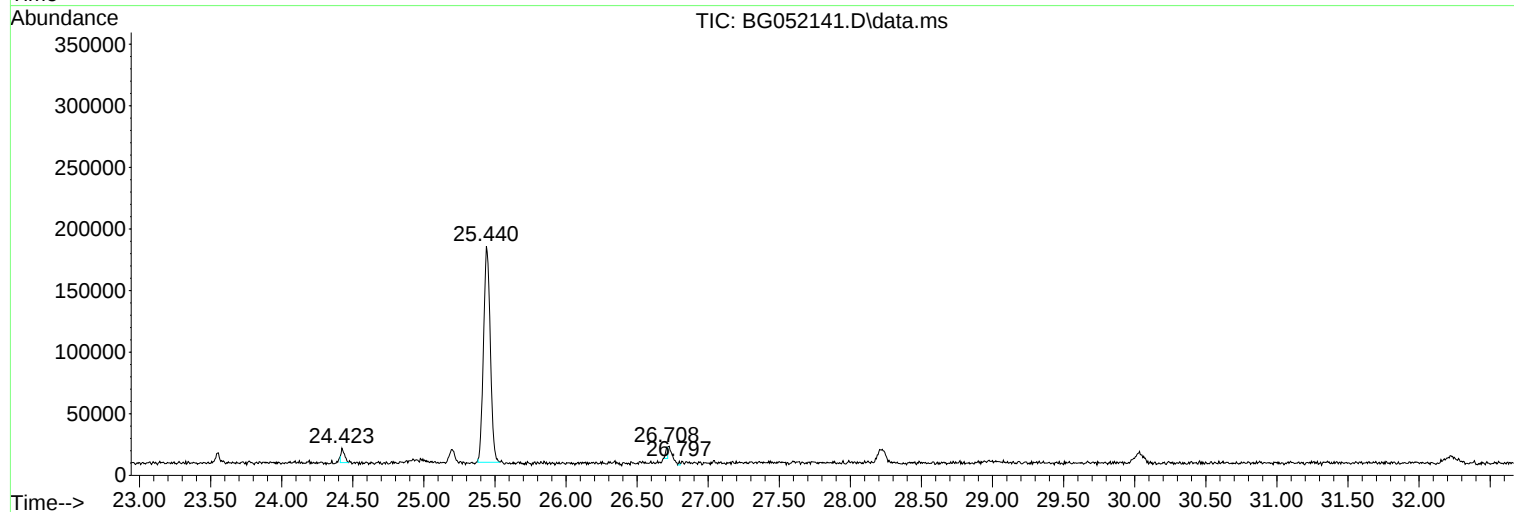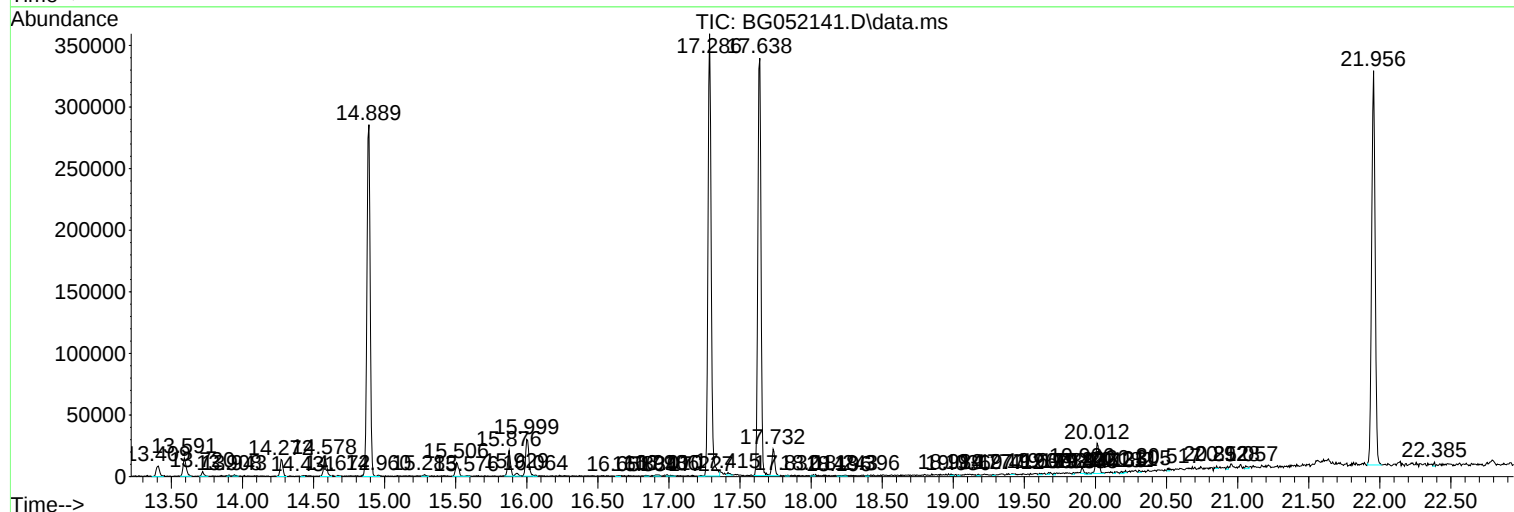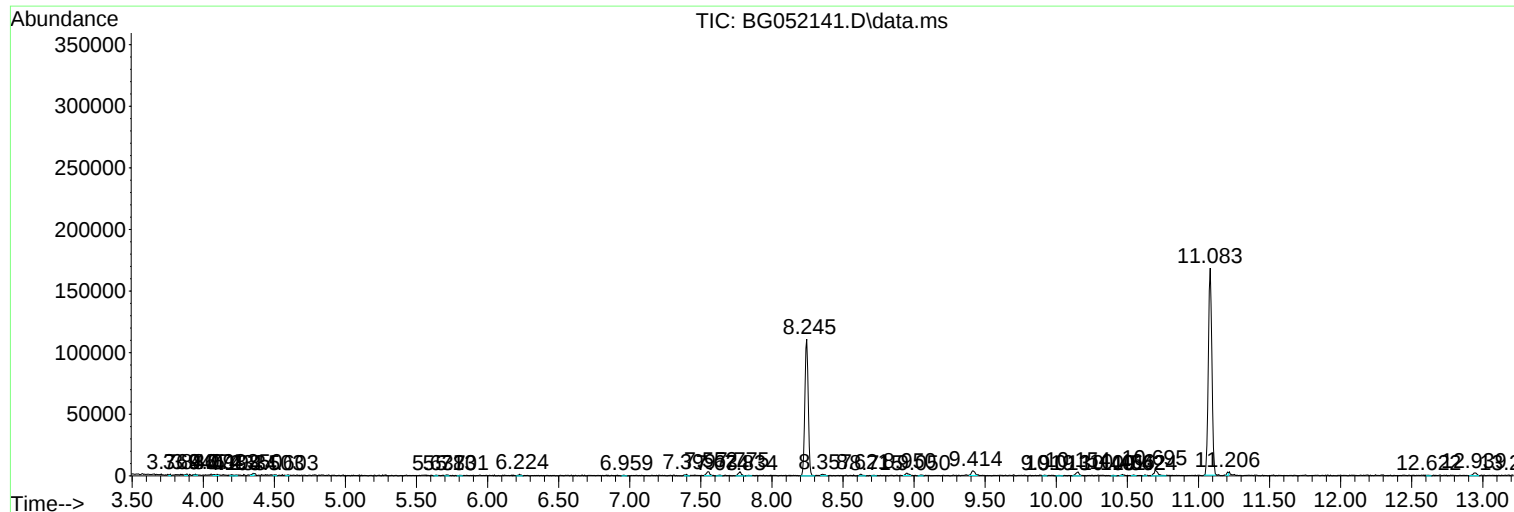

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052141.D
Acq On : 25 Jan 2022 12:30
Operator : CG/JU
Sample : N1199-18DL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q13DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052141.D
Acq On : 25 Jan 2022 12:30
Operator : CG/JU
Sample : N1199-18DL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q13DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc