

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052142.D
 Acq On : 25 Jan 2022 13:08
 Operator : CG/JU
 Sample : N1199-19DL2 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q14DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.311	139	140	143	rVB	1445	1159	0.14%	0.031%
2	4.358	143	148	152	rBV3	2280	4187	0.50%	0.111%
3	7.377	660	662	667	rVB	896	1080	0.13%	0.029%
4	7.548	687	691	697	rBV2	2290	3438	0.41%	0.091%
5	7.624	701	704	710	rVB2	1523	2244	0.27%	0.059%
6	7.765	726	728	735	rVB2	1619	2834	0.34%	0.075%
7	8.247	803	810	817	rBB	107429	182241	21.55%	4.826%
8	8.364	825	830	835	rBV	2091	3345	0.40%	0.089%
9	8.629	871	875	879	rBV2	1936	2519	0.30%	0.067%
10	9.363	997	1000	1003	rBV	1150	1070	0.13%	0.028%
11	9.416	1005	1009	1016	rBV3	2245	4368	0.52%	0.116%
12	9.945	1095	1099	1102	rBV2	876	1237	0.15%	0.033%
13	10.156	1130	1135	1138	rBV	1539	2646	0.31%	0.070%
14	10.321	1161	1163	1168	rVB2	779	1244	0.15%	0.033%
15	10.473	1183	1189	1194	rVB2	1608	2844	0.34%	0.075%
16	10.696	1221	1227	1228	rBV	1920	1770	0.21%	0.047%
17	10.714	1228	1230	1235	rVB2	2028	1709	0.20%	0.045%
18	11.084	1283	1293	1300	rBV	160482	289280	34.21%	7.660%
19	11.208	1312	1314	1318	rVV2	1014	1379	0.16%	0.037%
20	11.255	1320	1322	1327	rVB2	1117	1634	0.19%	0.043%
21	12.629	1553	1556	1562	rVB2	789	1191	0.14%	0.032%
22	12.941	1601	1609	1617	rVB2	8316	14455	1.71%	0.383%
23	13.328	1671	1675	1679	rBV2	1269	1938	0.23%	0.051%
24	13.410	1684	1689	1693	rVB3	2375	3841	0.45%	0.102%
25	13.716	1737	1741	1742	rBV2	1887	2263	0.27%	0.060%
26	13.857	1763	1765	1769	rVB	1364	1292	0.15%	0.034%
27	13.945	1777	1780	1783	rBV3	1045	1073	0.13%	0.028%
28	14.209	1821	1825	1829	rBV2	2409	3420	0.40%	0.091%
29	14.274	1832	1836	1842	rBV	6689	9482	1.12%	0.251%
30	14.450	1861	1866	1868	rBV3	1295	1779	0.21%	0.047%
31	14.579	1882	1888	1896	rBV3	7239	12831	1.52%	0.340%
32	14.885	1932	1940	1947	rVB	280073	440506	52.09%	11.665%
33	14.950	1949	1951	1954	rBV	1111	1330	0.16%	0.035%
34	15.273	2004	2006	2008	rBV	1012	1049	0.12%	0.028%
35	15.349	2015	2019	2021	rVB	1195	1093	0.13%	0.029%
36	15.431	2026	2033	2037	rVB2	4405	6188	0.73%	0.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
 Data File : BG052142.D
 Acq On : 25 Jan 2022 13:08
 Operator : CG/JU
 Sample : N1199-19DL2 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0Q14DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.508	2039	2046	2053	rBV3	41546	63250	7.48%	1.675%
38	15.872	2104	2108	2115	rBV2	10855	15269	1.81%	0.404%
39	15.931	2115	2118	2126	rVB	3256	4163	0.49%	0.110%
40	16.007	2126	2131	2137	rBV2	11005	15601	1.84%	0.413%
41	16.800	2264	2266	2271	rVB	925	1191	0.14%	0.032%
42	16.906	2280	2284	2287	rBV2	1393	1898	0.22%	0.050%
43	17.288	2342	2349	2364	rBV	529416	845665	100.00%	22.394%
44	17.405	2366	2369	2379	rVB7	5313	10656	1.26%	0.282%
45	17.634	2402	2408	2415	rBV	357766	539337	63.78%	14.282%
46	17.734	2420	2425	2431	rVB2	12210	18158	2.15%	0.481%
47	17.834	2437	2442	2447	rVB3	1851	3098	0.37%	0.082%
48	17.910	2451	2455	2457	rBV	1130	1128	0.13%	0.030%
49	18.210	2502	2506	2508	rBV	1188	1666	0.20%	0.044%
50	18.263	2513	2515	2517	rBV	1725	1225	0.14%	0.032%
51	18.304	2519	2522	2523	rVB2	1157	1138	0.13%	0.030%
52	18.327	2523	2526	2530	rBV	1104	1446	0.17%	0.038%
53	18.562	2561	2566	2570	rBV2	1210	2064	0.24%	0.055%
54	18.627	2574	2577	2578	rBV	1273	1208	0.14%	0.032%
55	18.921	2625	2627	2628	rBV2	1806	1078	0.13%	0.029%
56	19.162	2665	2668	2671	rBV3	847	1366	0.16%	0.036%
57	19.667	2750	2754	2756	rVB4	2015	2432	0.29%	0.064%
58	19.908	2792	2795	2800	rVB3	5233	6156	0.73%	0.163%
59	20.013	2806	2813	2818	rBV2	16313	22747	2.69%	0.602%
60	20.131	2831	2833	2835	rBV2	1372	1374	0.16%	0.036%
61	20.266	2855	2856	2858	rBV2	1554	1050	0.12%	0.028%
62	20.430	2882	2884	2885	rBV2	1799	1241	0.15%	0.033%
63	20.448	2885	2887	2888	rVB	2802	1444	0.17%	0.038%
64	20.466	2888	2890	2892	rBV2	1852	2245	0.27%	0.059%
65	20.519	2897	2899	2900	rBV2	1726	1115	0.13%	0.030%
66	20.742	2936	2937	2940	rBV3	3044	2820	0.33%	0.075%
67	20.947	2970	2972	2977	rVB4	4311	5413	0.64%	0.143%
68	21.958	3137	3144	3153	rVB	332176	572253	67.67%	15.154%
69	22.134	3172	3174	3178	rBV4	4081	5530	0.65%	0.146%
70	25.441	3727	3737	3752	rVB2	185172	603922	71.41%	15.992%




Sum of corrected areas: 3776306

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052142.D
Acq On : 25 Jan 2022 13:08
Operator : CG/JU
Sample : N1199-19DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q14DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

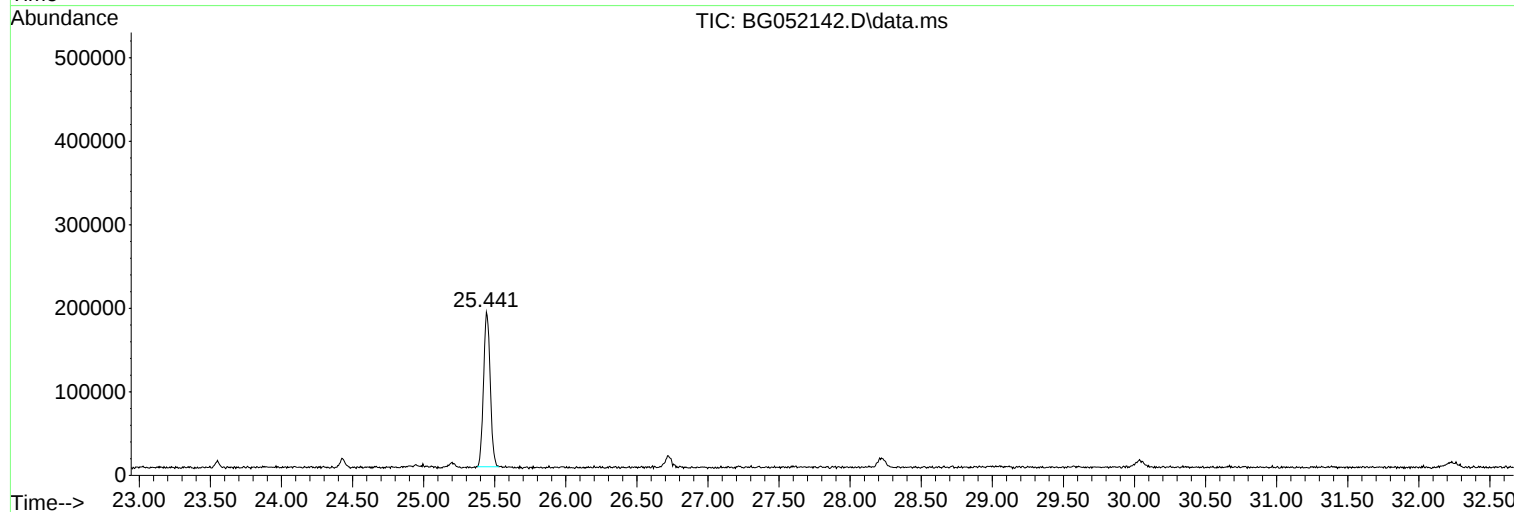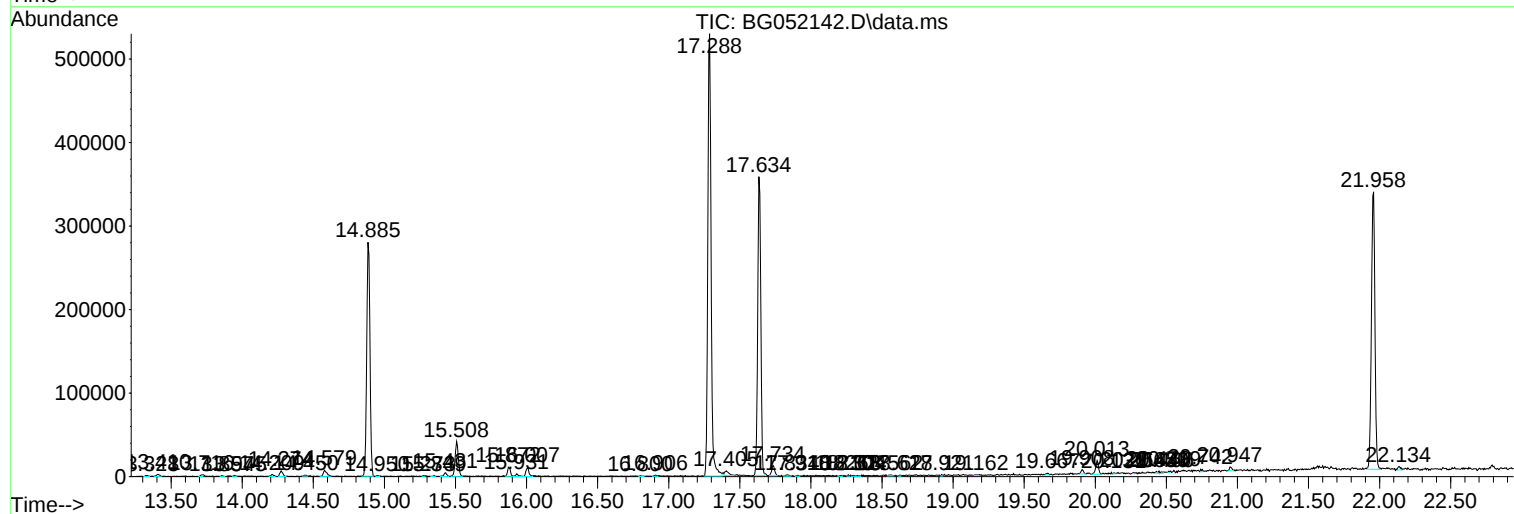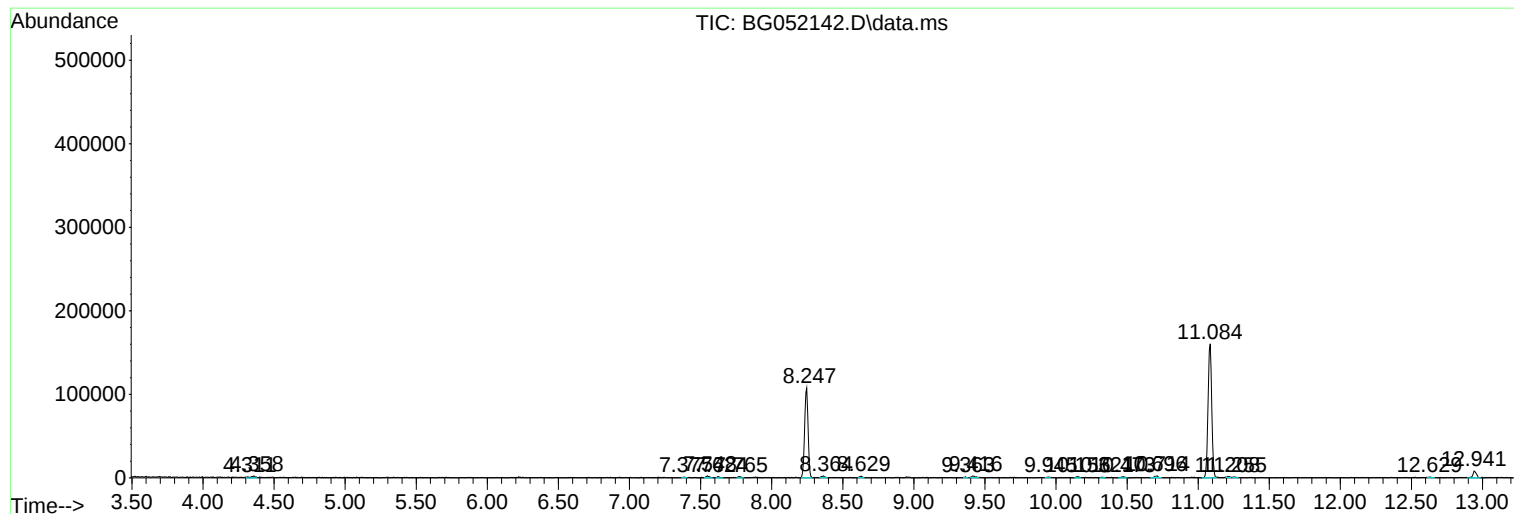

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052142.D
Acq On : 25 Jan 2022 13:08
Operator : CG/JU
Sample : N1199-19DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q14DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012522\
Data File : BG052142.D
Acq On : 25 Jan 2022 13:08
Operator : CG/JU
Sample : N1199-19DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0Q14DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------