
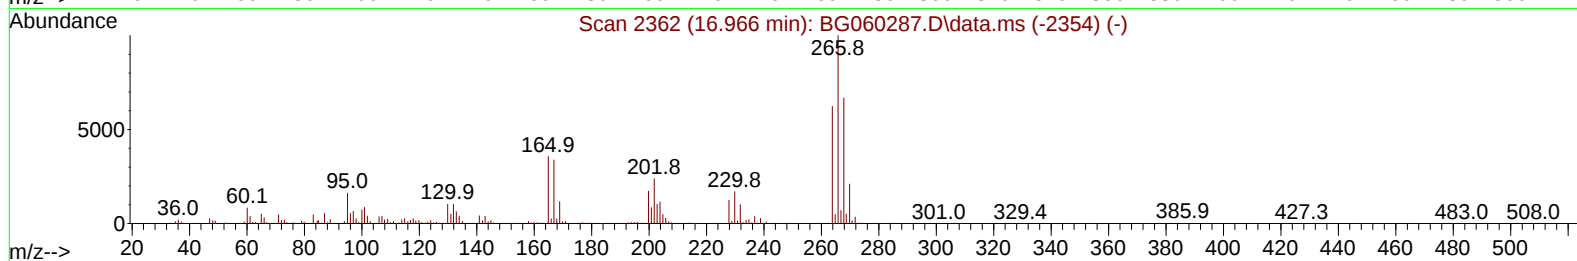
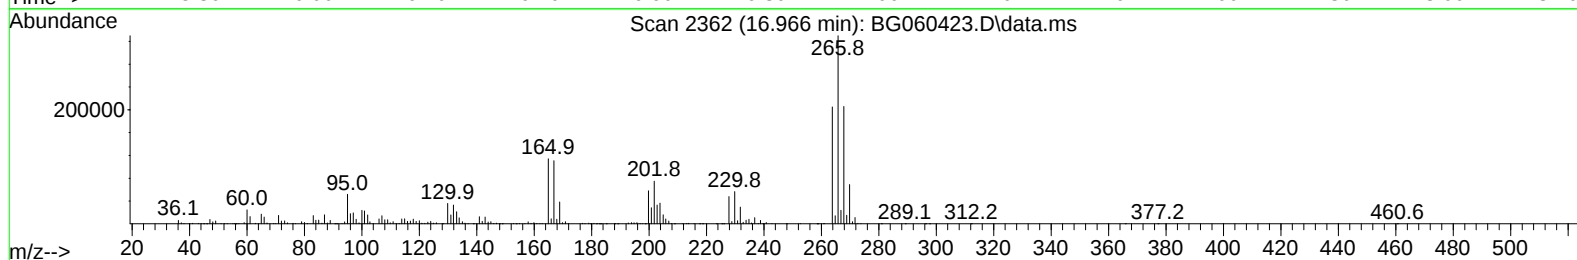


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012524\
Data File : BG060423.D
Acq On : 25 Jan 2024 11:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 13:20:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

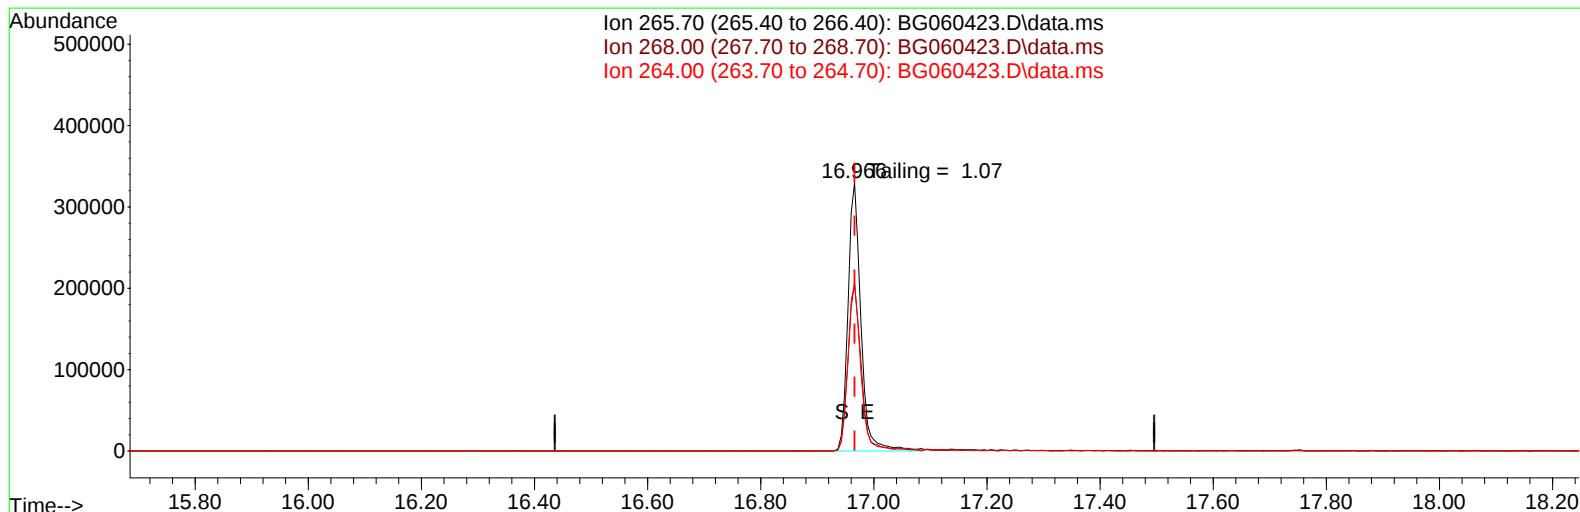




TIC: BG060423.D\data.ms

(70) Pentachlorophenol (C)**16.966min (-0.000) 1338178.83 ng****response 525378**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	62.39
264.00	62.30	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012524\
Data File : BG060423.D
Acq On : 25 Jan 2024 11:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 13:20:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

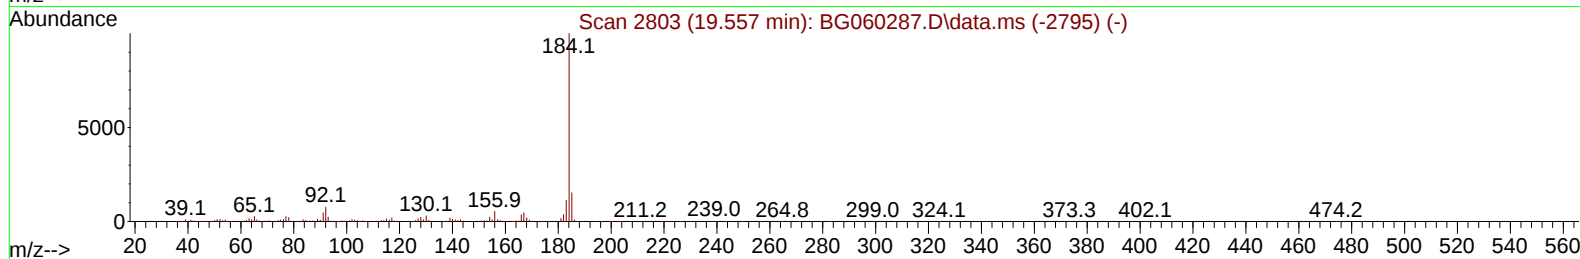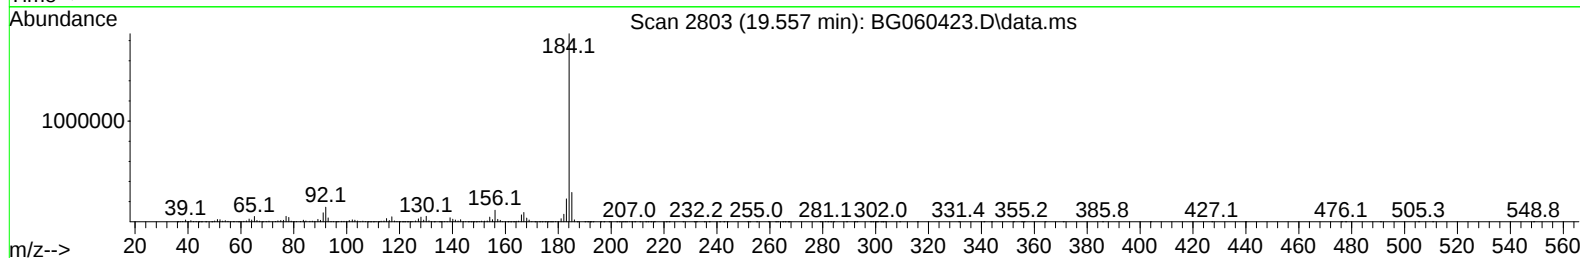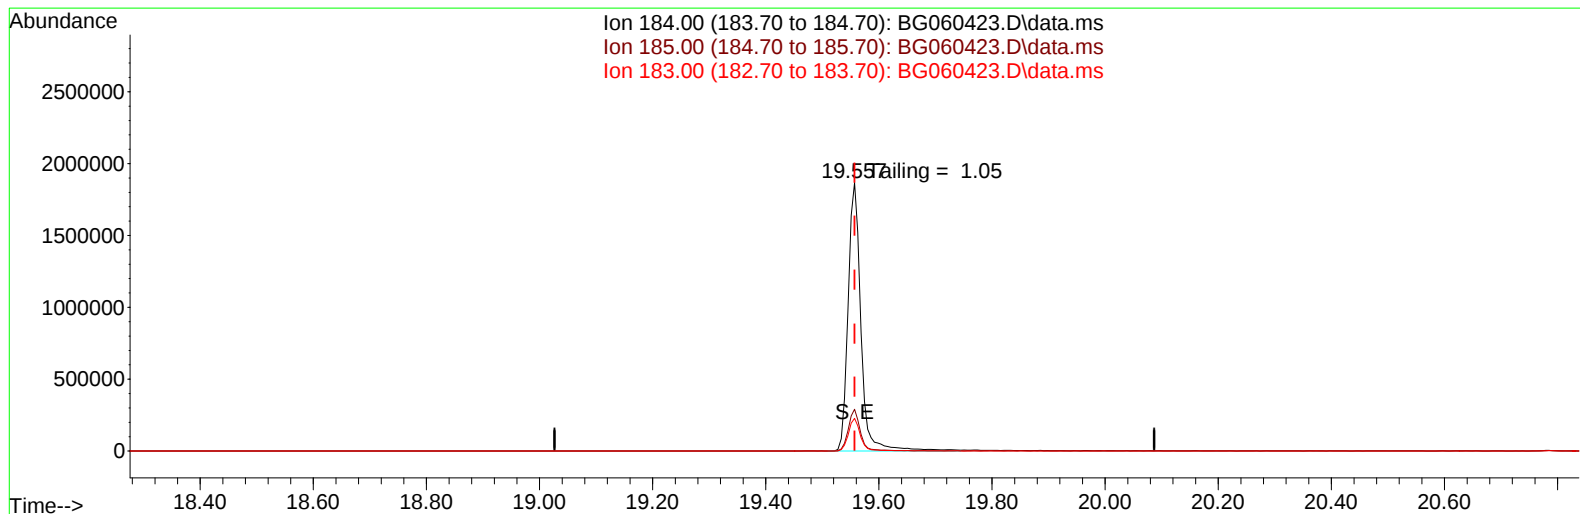

TIC: BG060423.D\data.ms

(77) Benzidine**19.557min (-0.000) 300835.19 ng****response 2934532**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.60
183.00	11.20	12.19
0.00	0.00	0.00