


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012524\
Data File : BG060423.D
Acq On : 25 Jan 2024 11:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

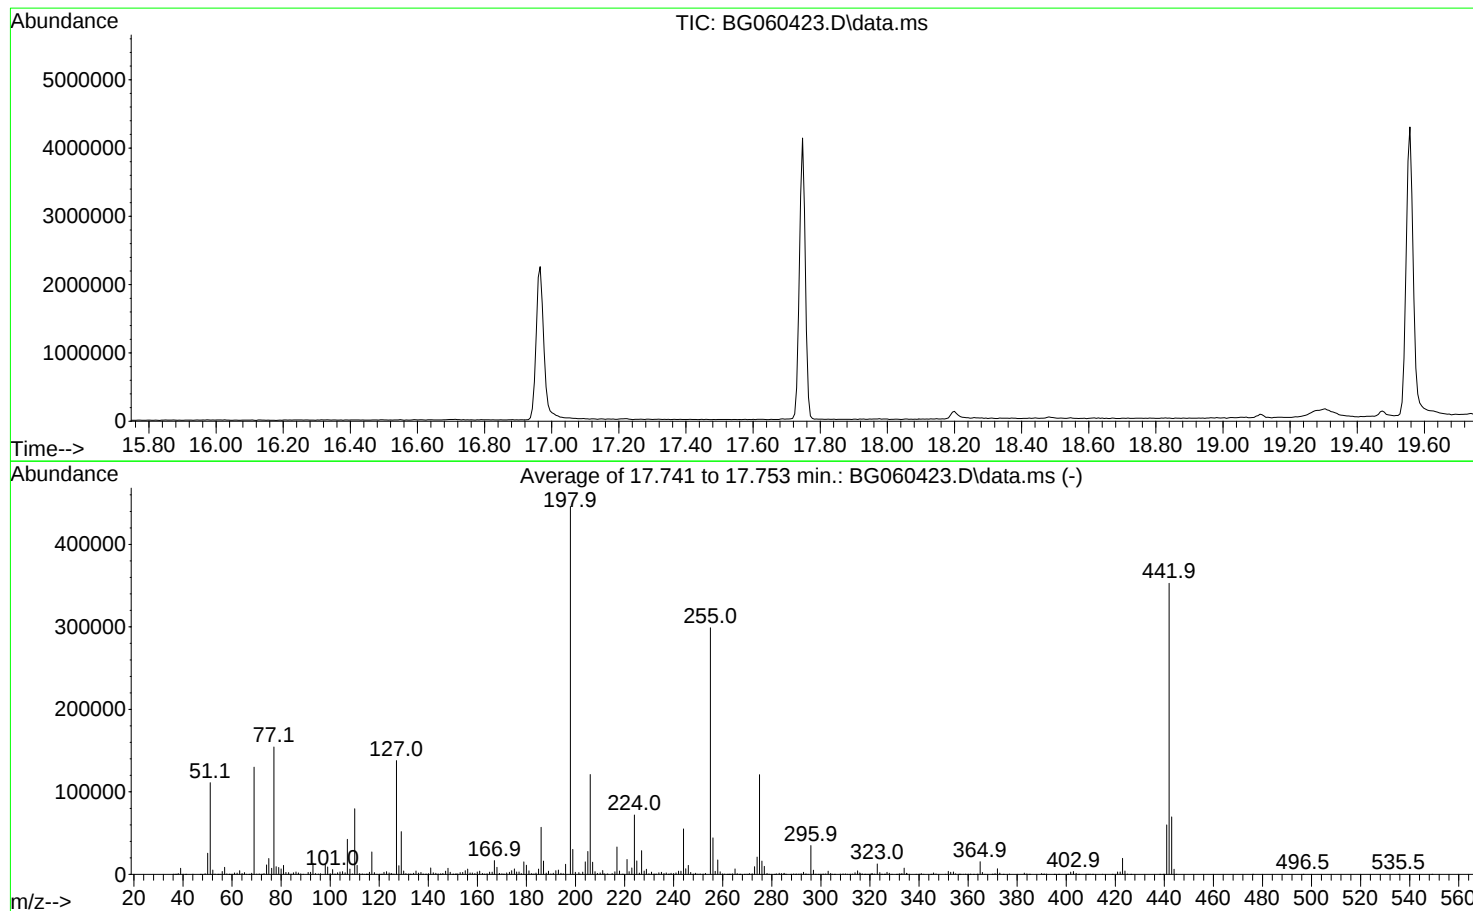




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	111160	PASS
68	69	0.00	2	1.1	1403	PASS
69	198	0.00	100	29.1	129978	PASS
70	69	0.00	2	0.3	385	PASS
127	198	10	80	30.9	137843	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	445931	PASS
199	198	5	9	6.8	30349	PASS
275	198	10	60	27.1	120845	PASS
365	198	1	100	3.4	15355	PASS
441	198	0.01	100	13.4	59888	PASS
442	442	50	100	100.0	352832	PASS
443	442	15	24	19.8	69736	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012524\
Data File : BG060423.D
Acq On : 25 Jan 2024 11:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 13:20:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

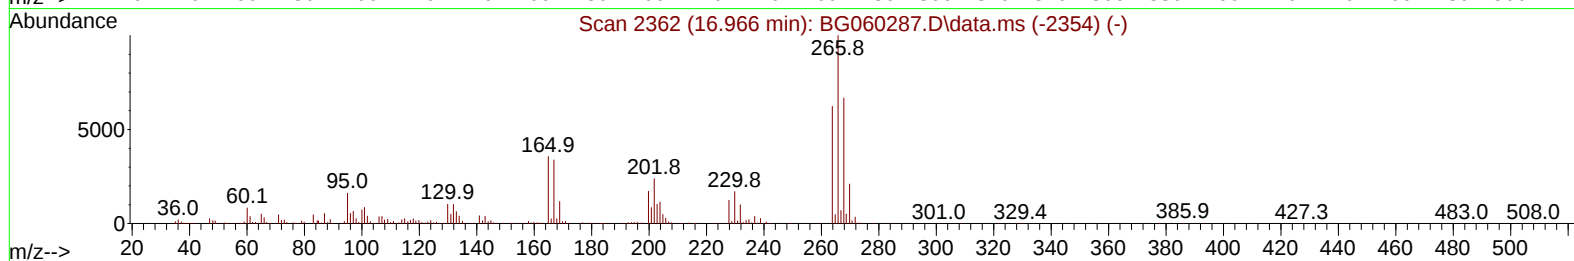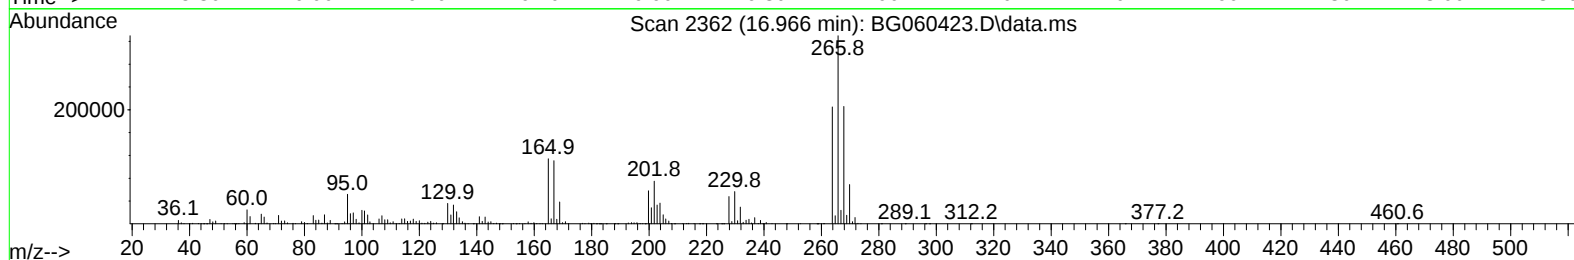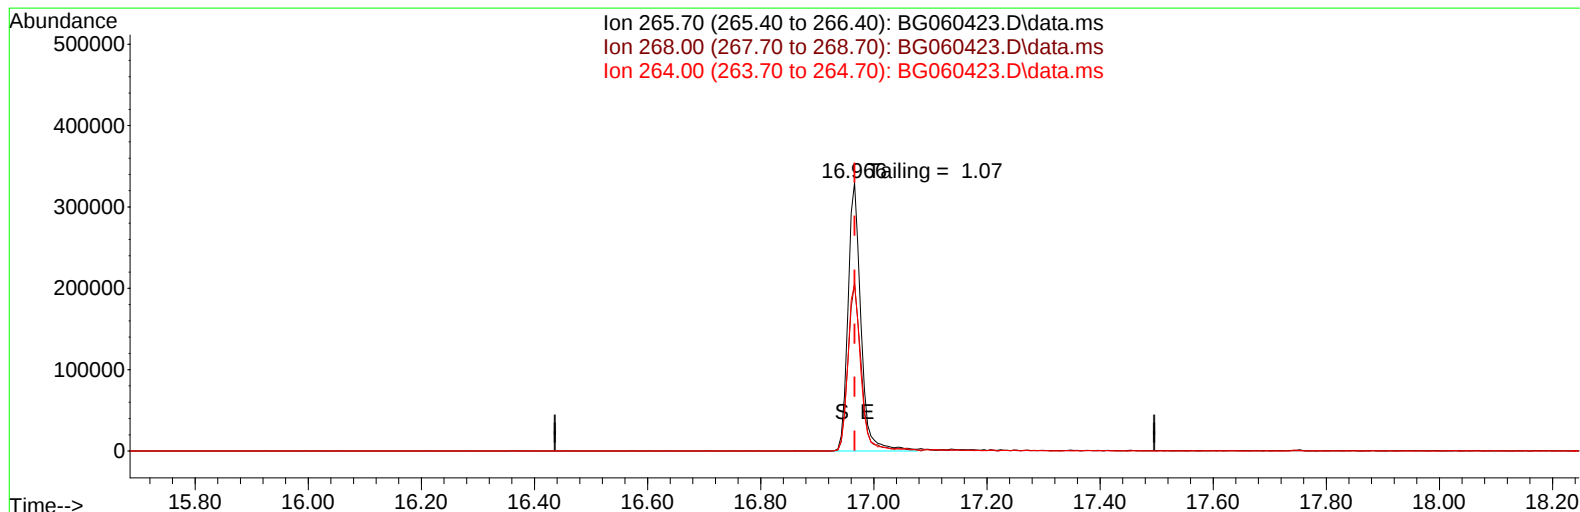

TIC: BG060423.D\data.ms

(70) Pentachlorophenol (C)

16.966min (-0.000) 1338178.83 ng




response 525378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	62.39
264.00	62.30	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012524\
Data File : BG060423.D
Acq On : 25 Jan 2024 11:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 13:20:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

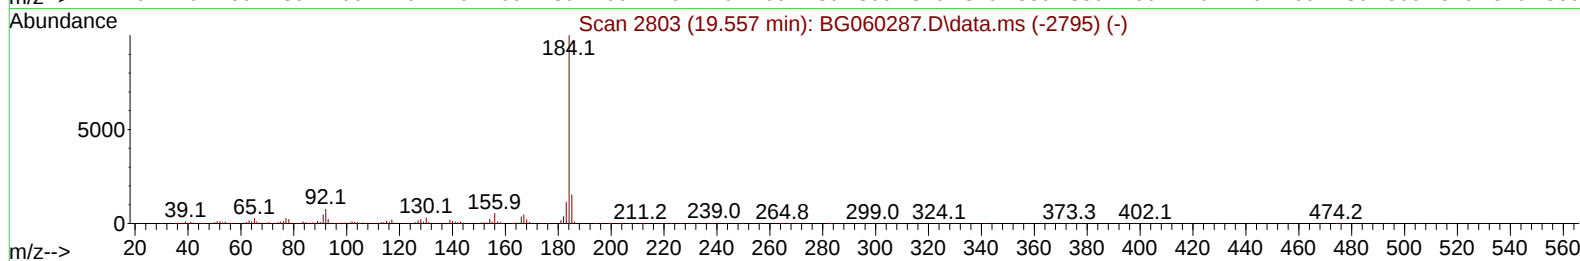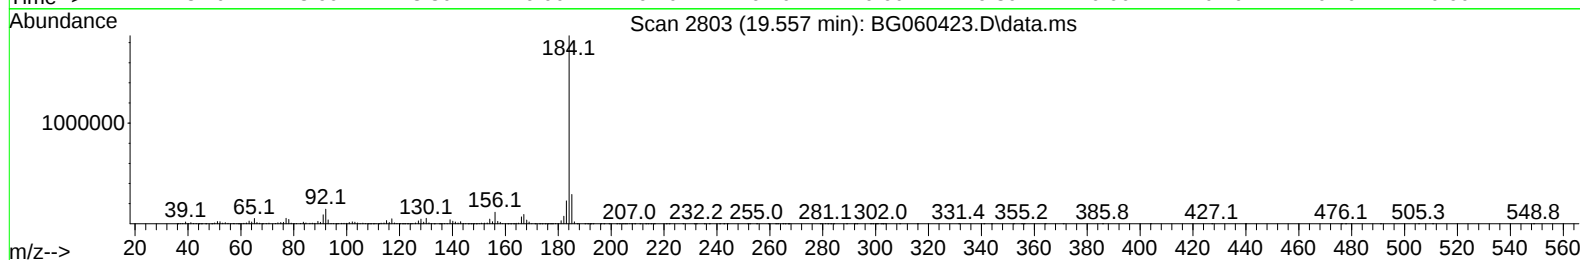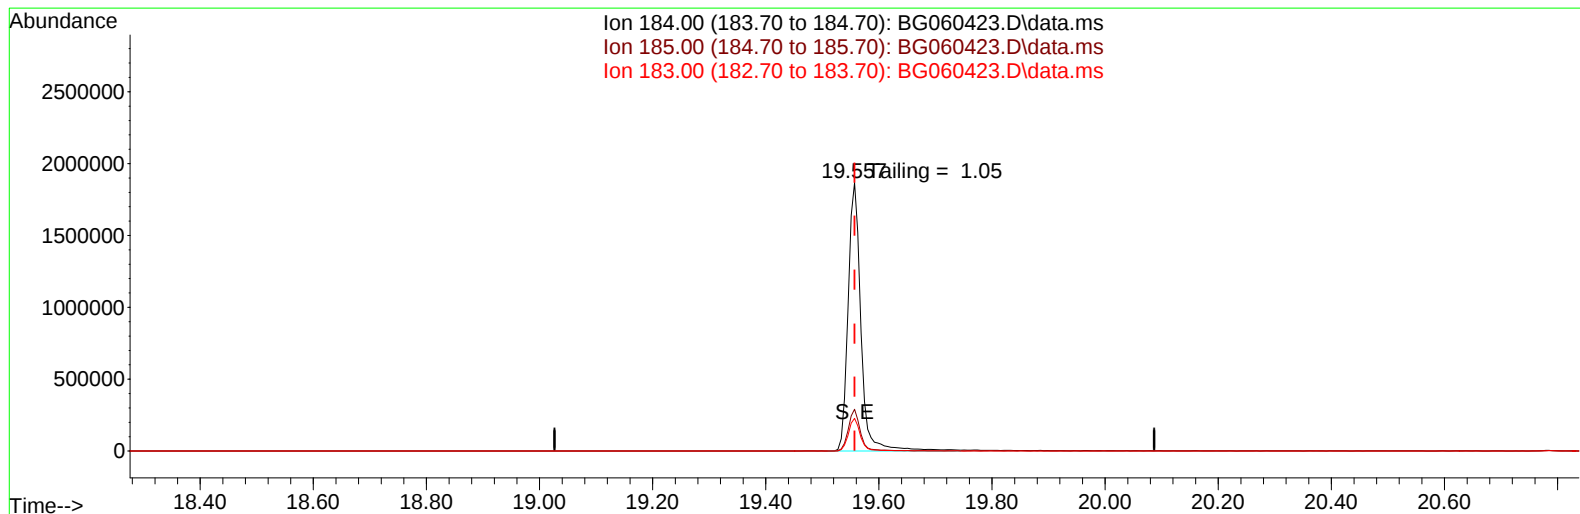

TIC: BG060423.D\data.ms

(77) Benzidine

19.557min (-0.000) 300835.19 ng

response 2934532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.60
183.00	11.20	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2024	BNA_G	<u>BG060423.D</u>
Compound Name	Response	Retention Time
DDT	1475674	20.785
DDD	27772	20.397
DDE	2862	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30634	1506308	2.03

Instrument :
BNA_G
ClientSampleId :
DFTPP