


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012615\
Data File : BG015915.D
Acq On : 26 Jan 2015 15:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 20 17:47:40 2015

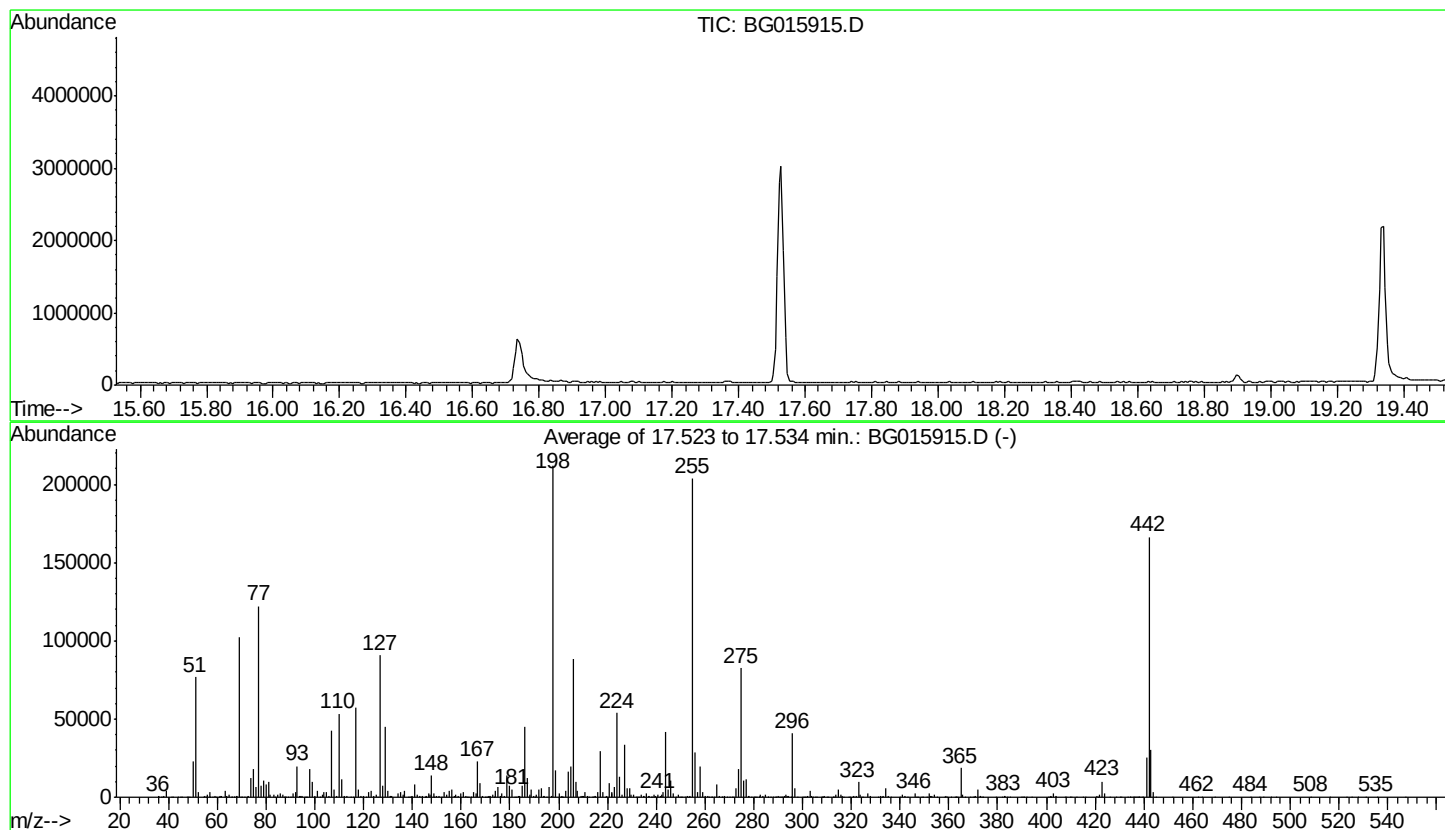

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	76738	PASS
68	69	0.00	2	0.9	964	PASS
69	198	0.00	100	48.2	102108	PASS
70	69	0.00	2	0.2	229	PASS
127	198	10	80	42.8	90653	PASS
197	198	0.00	2	0.5	962	PASS
198	198	100	100	100.0	212032	PASS
199	198	5	9	8.1	17223	PASS
275	198	10	60	38.9	82426	PASS
365	198	1	100	8.8	18607	PASS
441	442	0.01	24	15.1	25066	PASS
442	198	50	100	78.4	166186	PASS
443	442	15	24	18.1	30058	PASS