


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012615\
 Data File : BG015932.D
 Acq On : 27 Jan 2015 4:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 20 17:47:40 2015

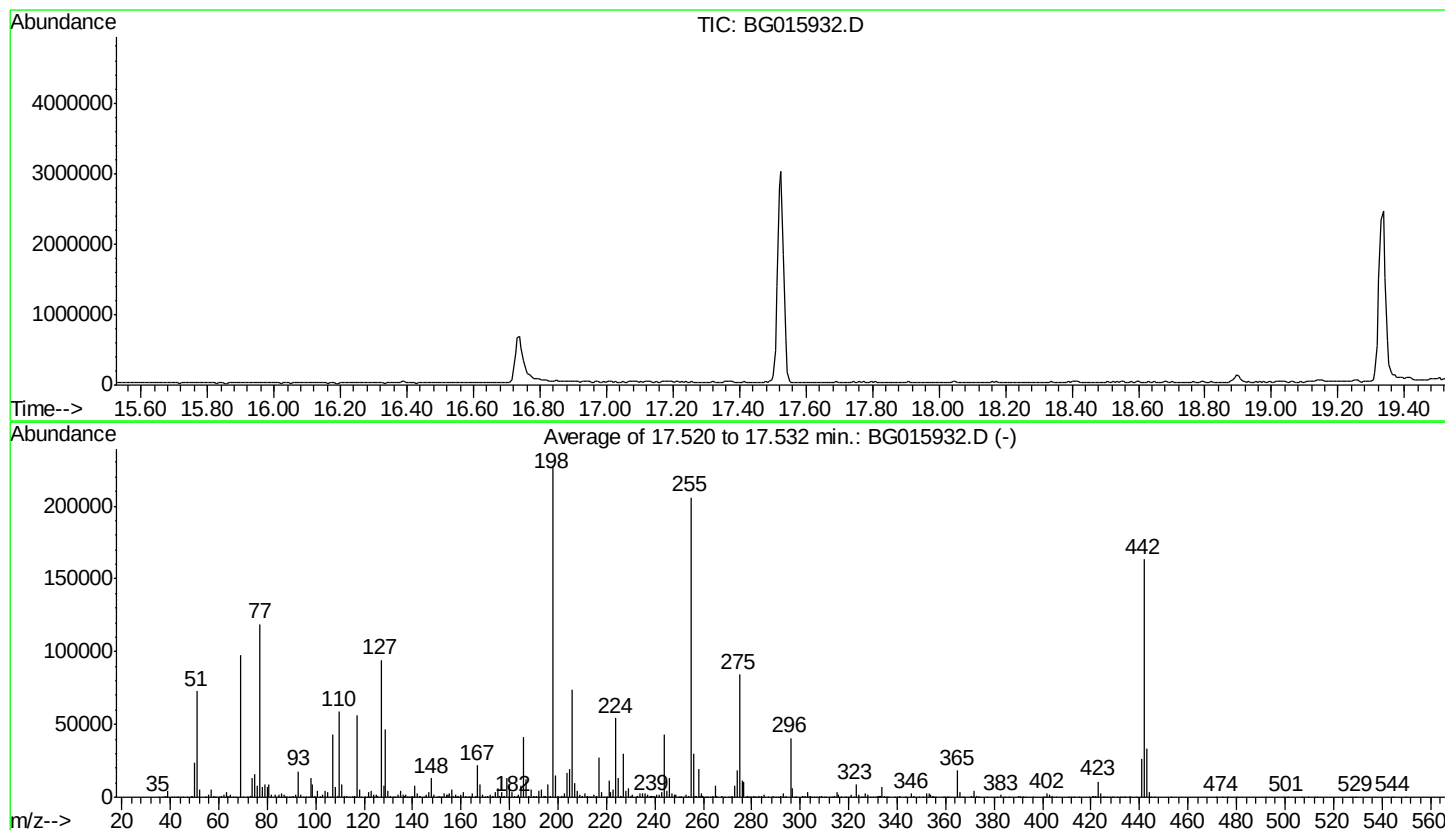

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	72723	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.8	97464	PASS
70	69	0.00	2	0.4	422	PASS
127	198	10	80	41.5	94512	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	227797	PASS
199	198	5	9	6.6	15026	PASS
275	198	10	60	37.0	84205	PASS
365	198	1	100	7.9	18085	PASS
441	442	0.01	24	16.4	26709	PASS
442	198	50	100	71.6	163200	PASS
443	442	15	24	20.7	33813	PASS