


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG012615\  
Data File : BG015915.D  
Acq On : 26 Jan 2015 15:15  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG012015.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jan 20 17:47:40 2015

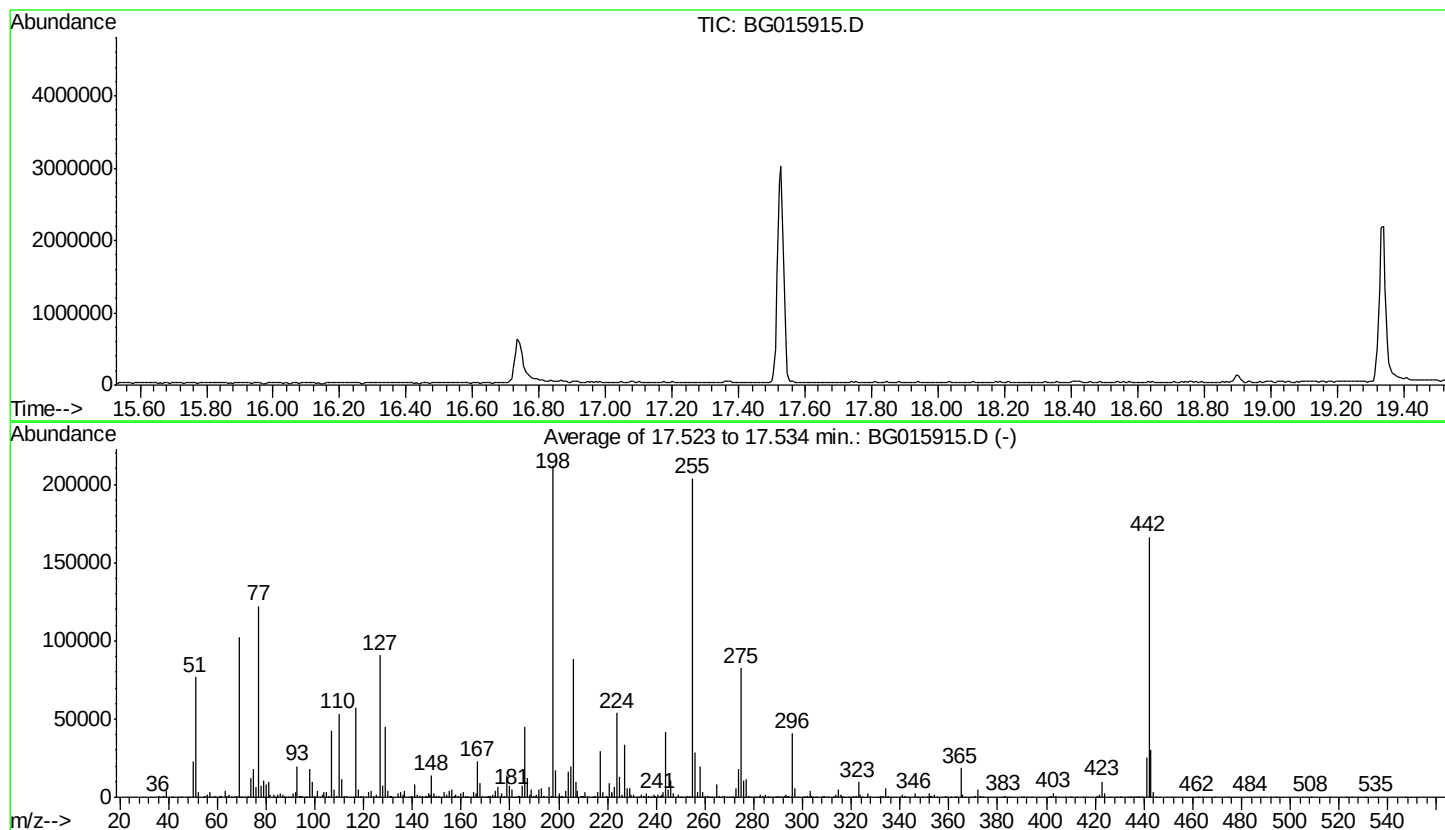

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2517

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.2         | 76738      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.9          | 964        | PASS                |
| 69             | 198             | 0.00            | 100             | 48.2         | 102108     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 229        | PASS                |
| 127            | 198             | 10              | 80              | 42.8         | 90653      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 962        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 212032     | PASS                |
| 199            | 198             | 5               | 9               | 8.1          | 17223      | PASS                |
| 275            | 198             | 10              | 60              | 38.9         | 82426      | PASS                |
| 365            | 198             | 1               | 100             | 8.8          | 18607      | PASS                |
| 441            | 442             | 0.01            | 24              | 15.1         | 25066      | PASS                |
| 442            | 198             | 50              | 100             | 78.4         | 166186     | PASS                |
| 443            | 442             | 15              | 24              | 18.1         | 30058      | PASS                |