


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012615\
 Data File : BG015951.D
 Acq On : 27 Jan 2015 17:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc : W
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 20 17:47:40 2015

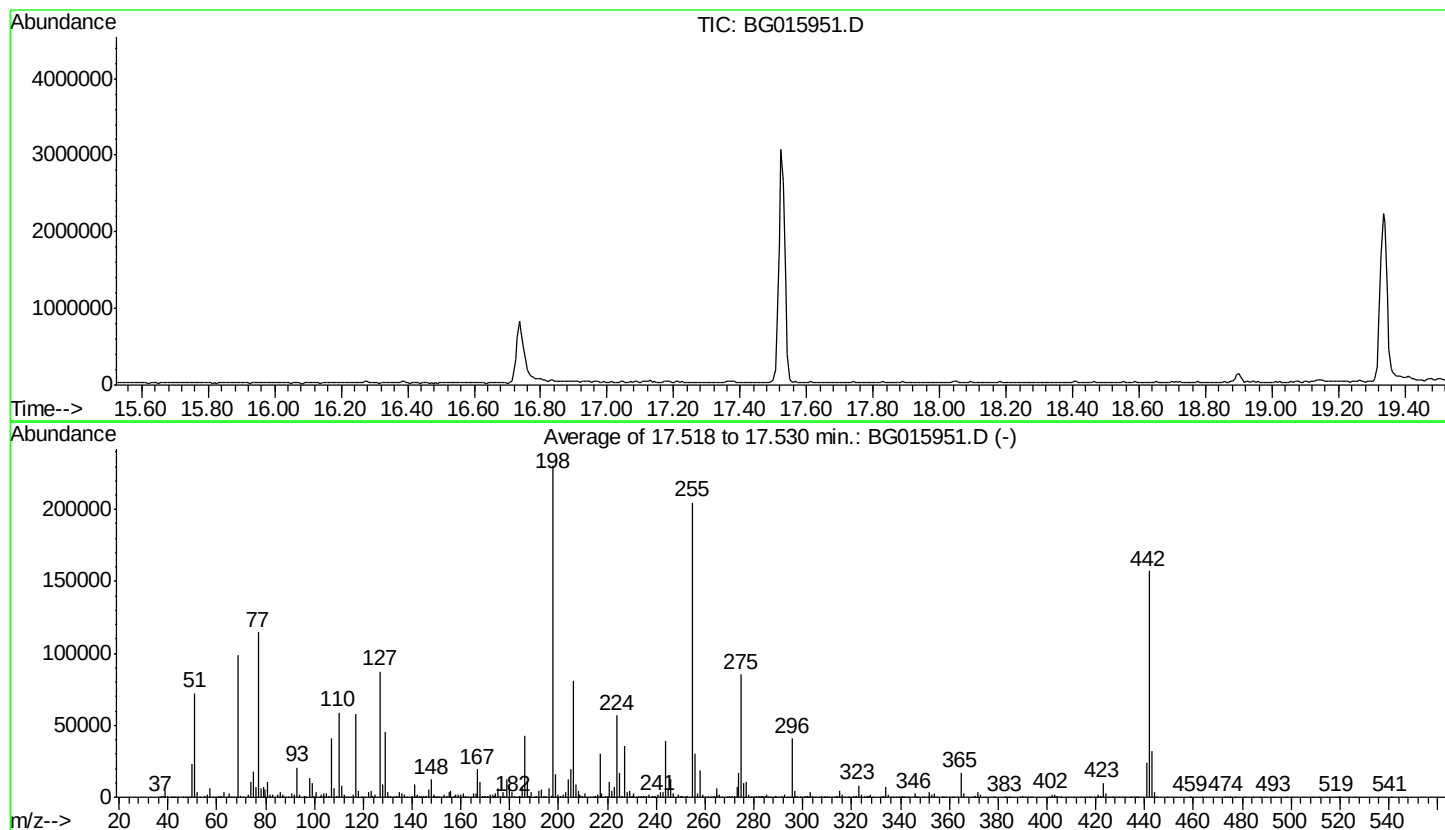

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	72394	PASS
68	69	0.00	2	0.4	442	PASS
69	198	0.00	100	42.7	98384	PASS
70	69	0.00	2	0.6	580	PASS
127	198	10	80	38.0	87584	PASS
197	198	0.00	2	0.5	1265	PASS
198	198	100	100	100.0	230464	PASS
199	198	5	9	7.1	16331	PASS
275	198	10	60	36.9	85101	PASS
365	198	1	100	7.4	17146	PASS
441	442	0.01	24	15.5	24439	PASS
442	198	50	100	68.3	157322	PASS
443	442	15	24	20.3	31864	PASS