
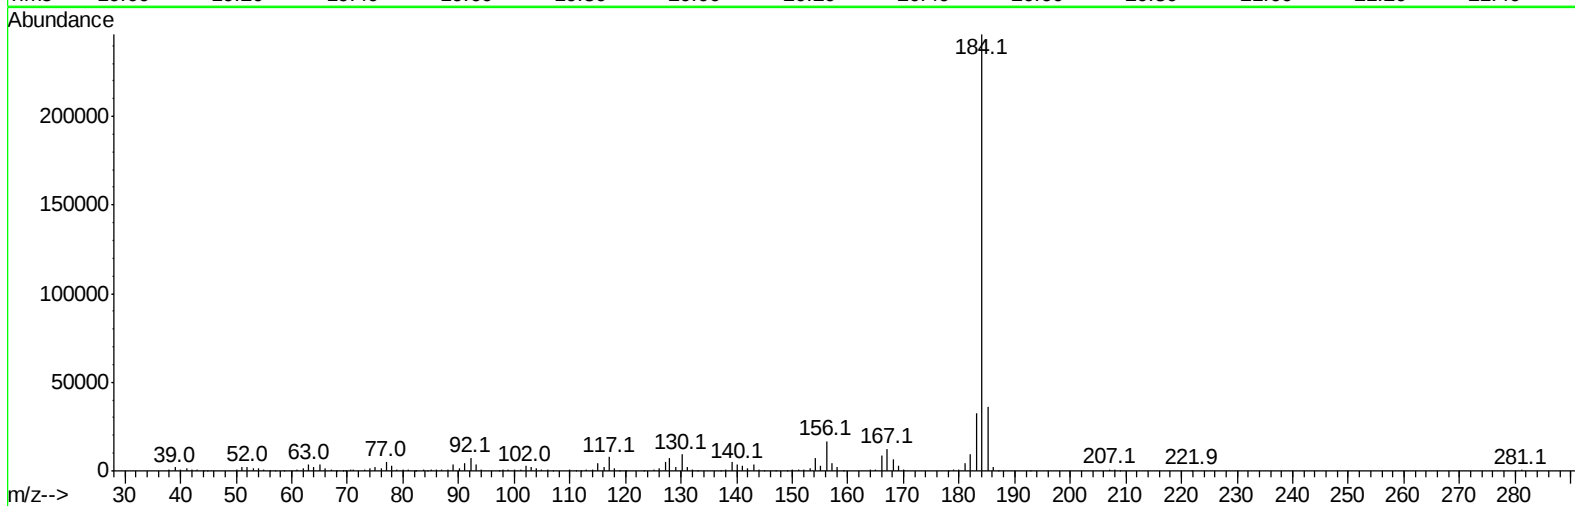


Data Path : U:\HPCHEM1\BNA G\DATA\BG012618\
Data File : BG032330.D
Acq On : 26 Jan 2018 15:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 03:20:12 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

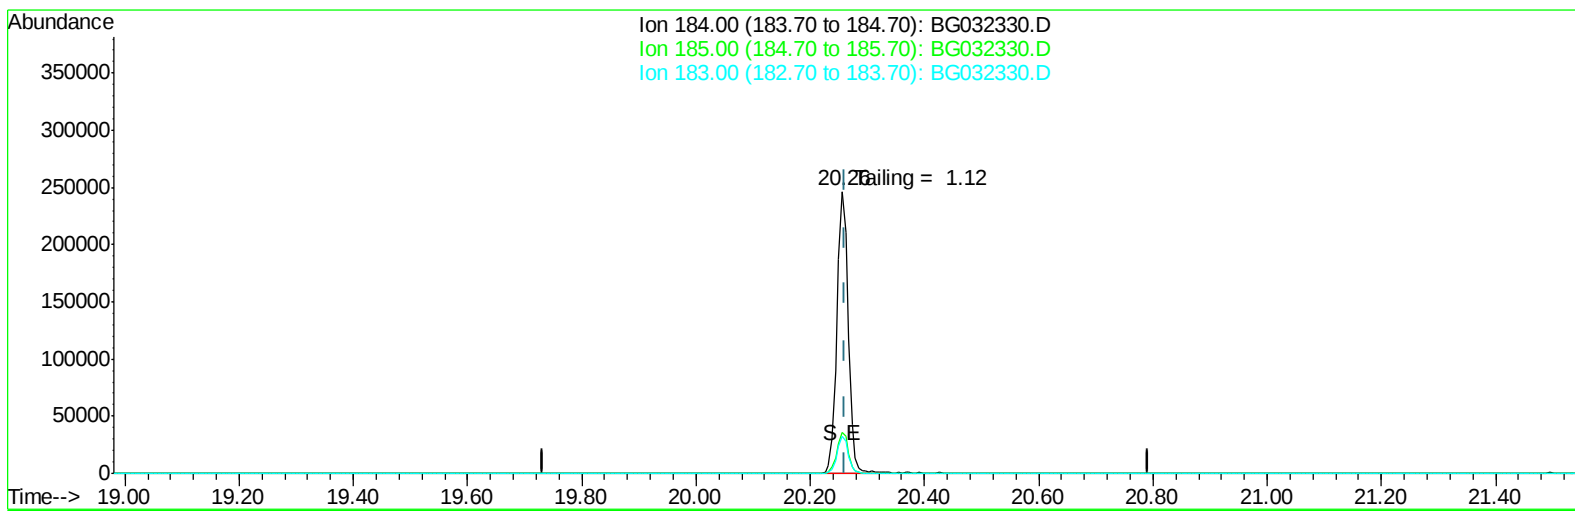

TIC: BG032330.D

(76) Benzidine



20.256min (-0.007) 0.00ng

response 339215

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.60
183.00	13.30	13.16
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012618\
Data File : BG032330.D
Acq On : 26 Jan 2018 15:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 03:20:12 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

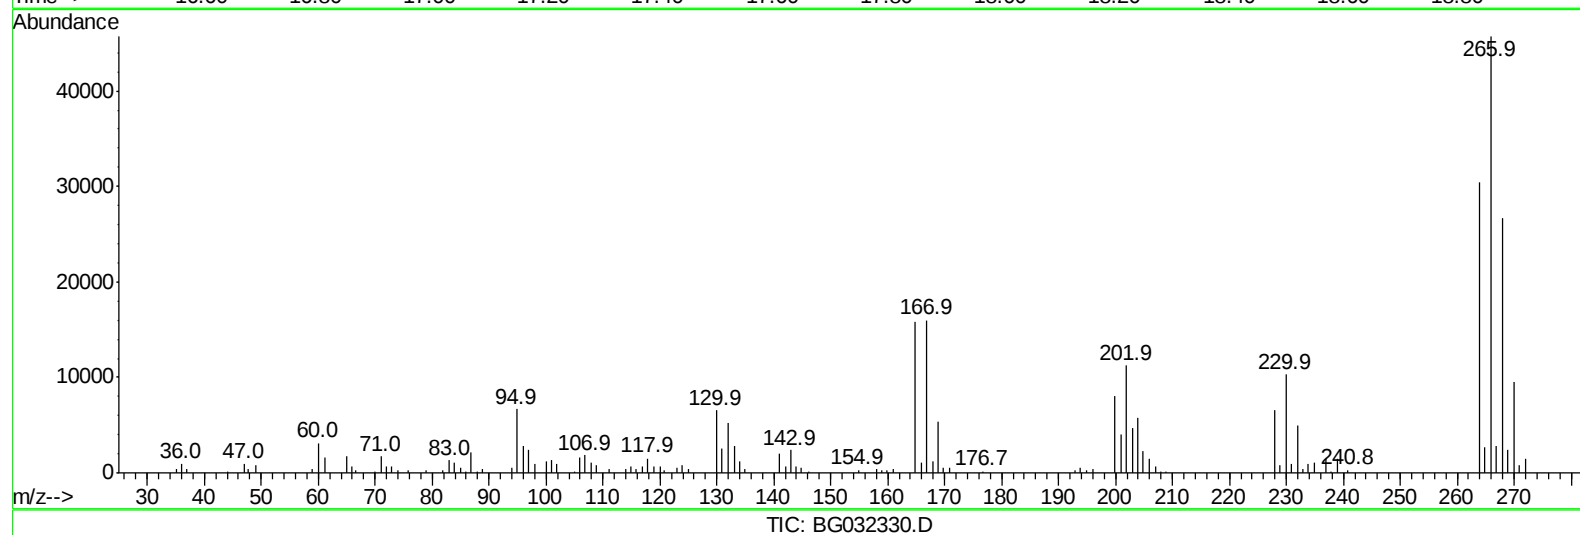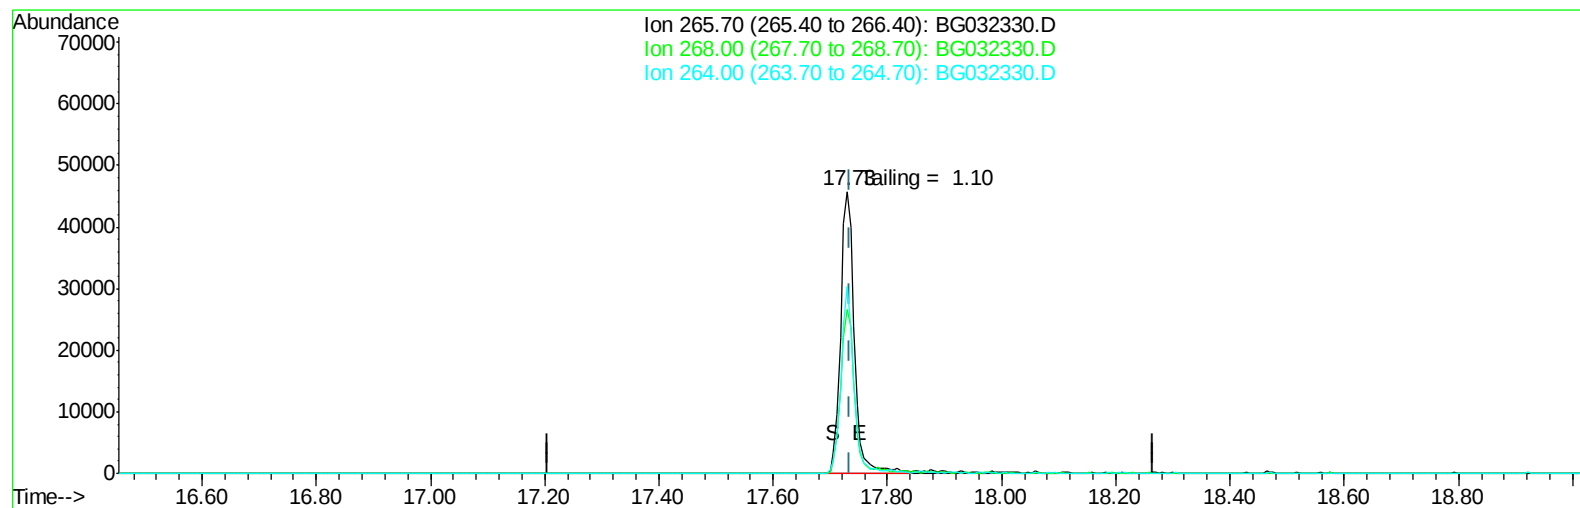

(69) Pentachlorophenol (C)

17.729min (-0.007) 20989.03ng

response 76026

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.38
264.00	62.00	66.59
0.00	0.00	0.00