


Data Path : U:\HPCHEM1\BNA G\Data\BG012618\
 Data File : BG032330.D
 Acq On : 26 Jan 2018 15:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

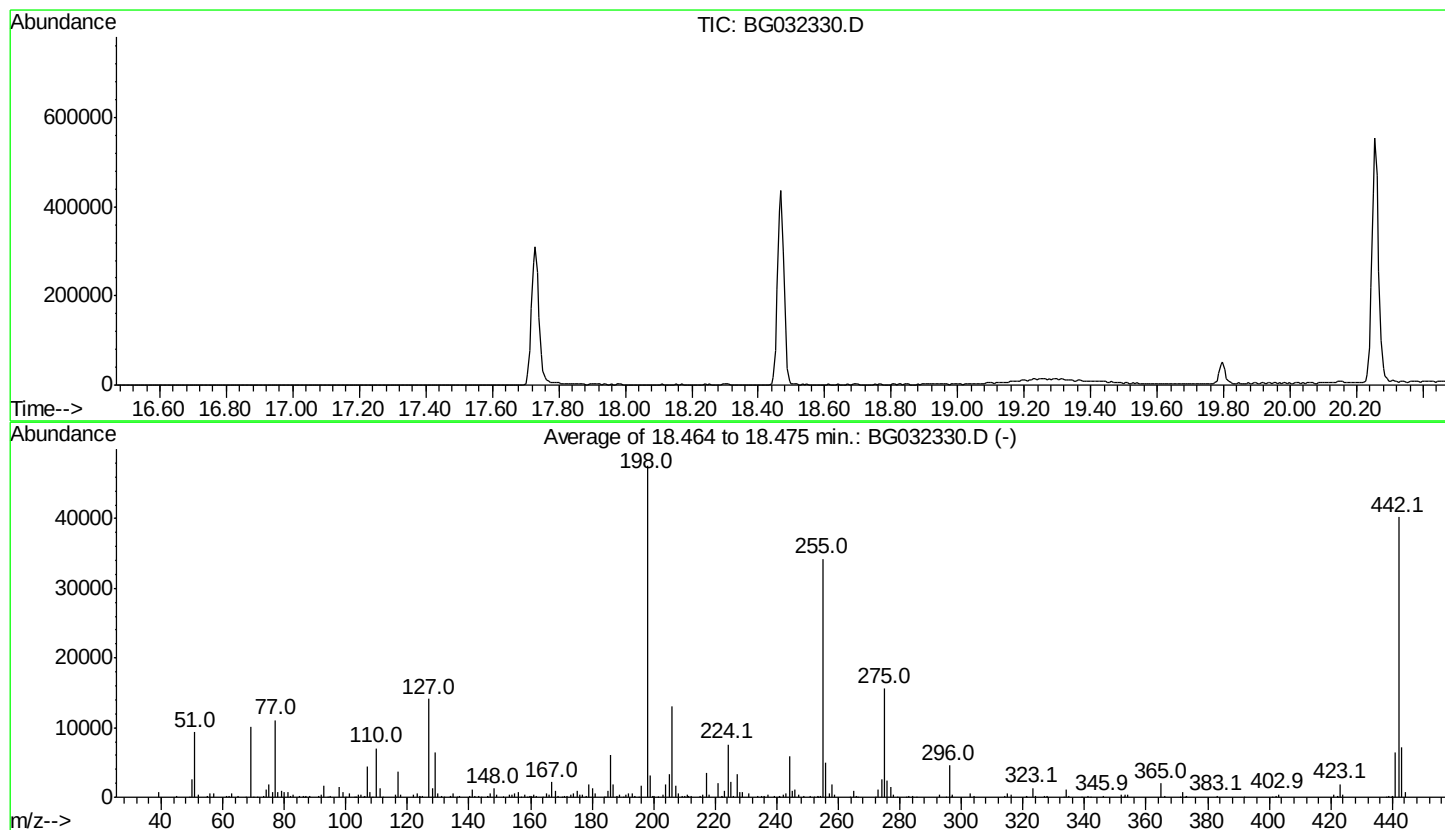

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	9335	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.3	10150	PASS
70	69	0.00	2	0.5	55	PASS
127	198	10	80	29.6	14114	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47618	PASS
199	198	5	9	6.6	3160	PASS
275	198	10	60	32.8	15605	PASS
365	198	1	100	4.2	2000	PASS
441	442	0.01	24	16.1	6492	PASS
442	198	50	100	84.4	40208	PASS
443	442	15	24	17.9	7213	PASS