
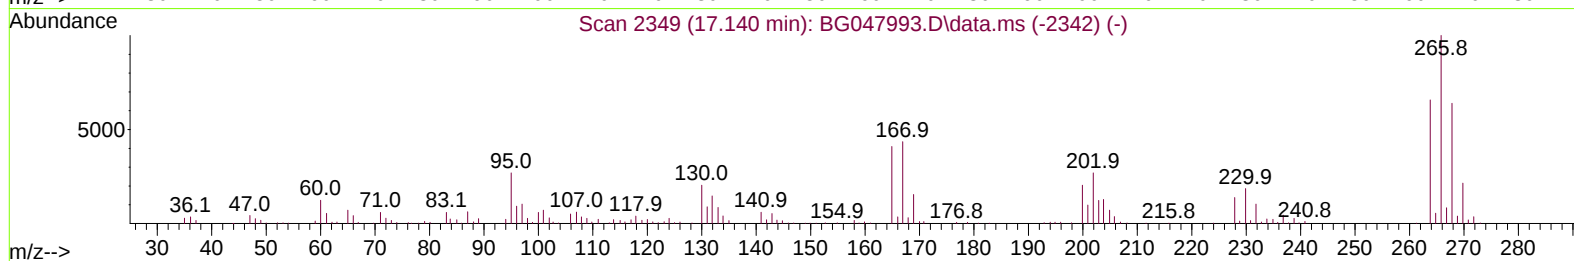
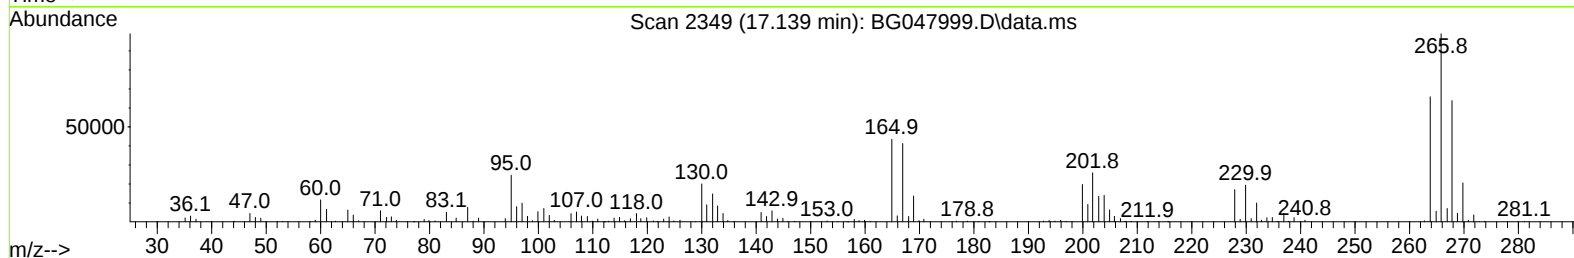


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012621\
Data File : BG047999.D
Acq On : 26 Jan 2021 8:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 00:37:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

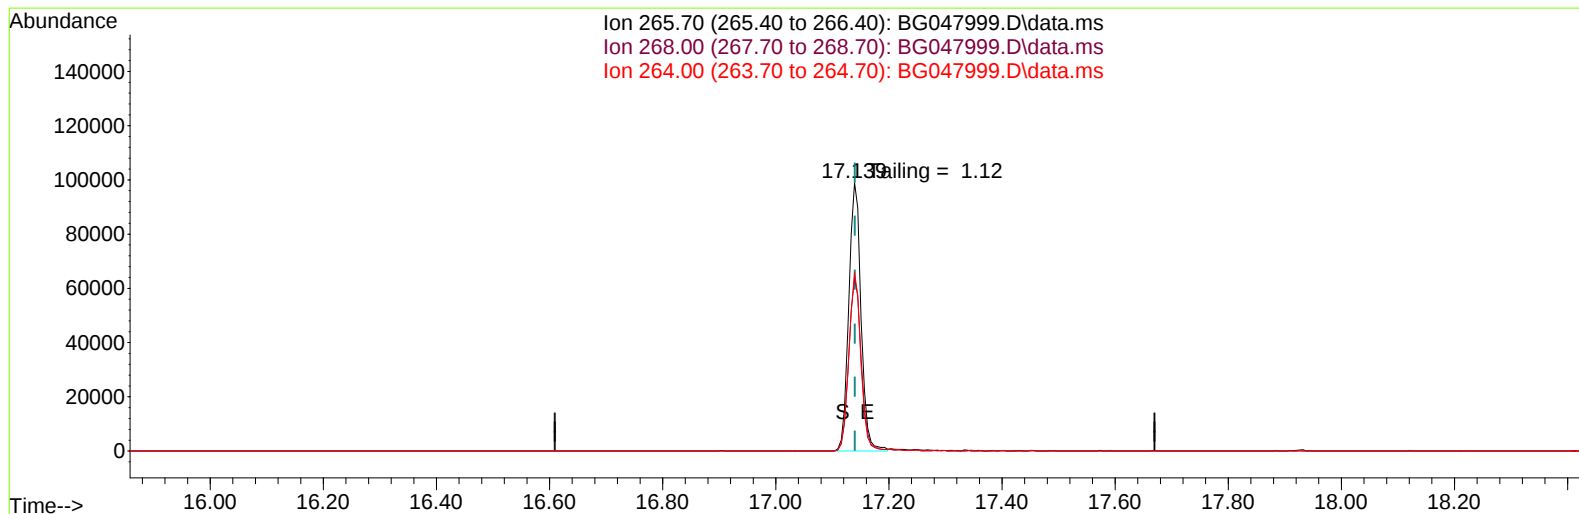

TIC: BG047999.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.000) 243737.71 ng

response 150548

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	66.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012621\
Data File : BG047999.D
Acq On : 26 Jan 2021 8:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 00:37:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

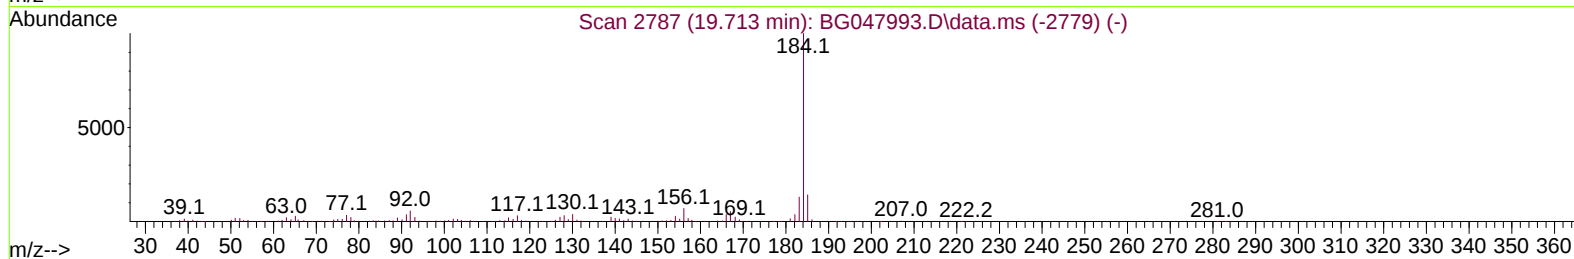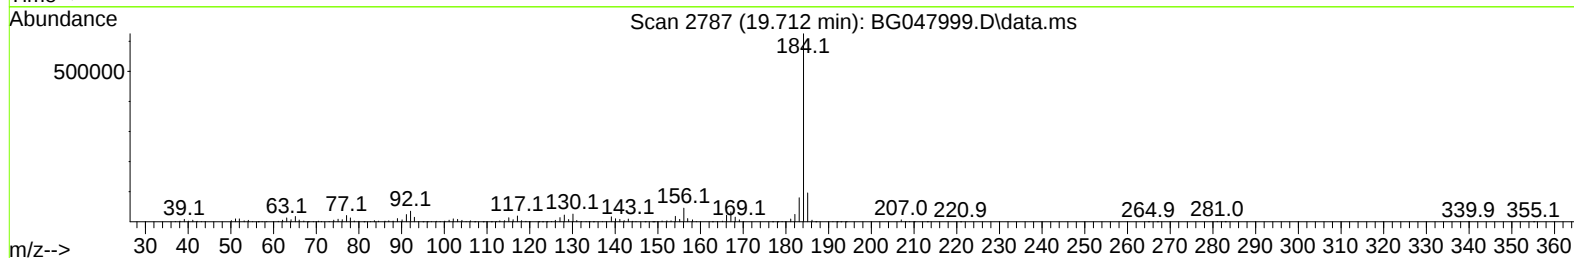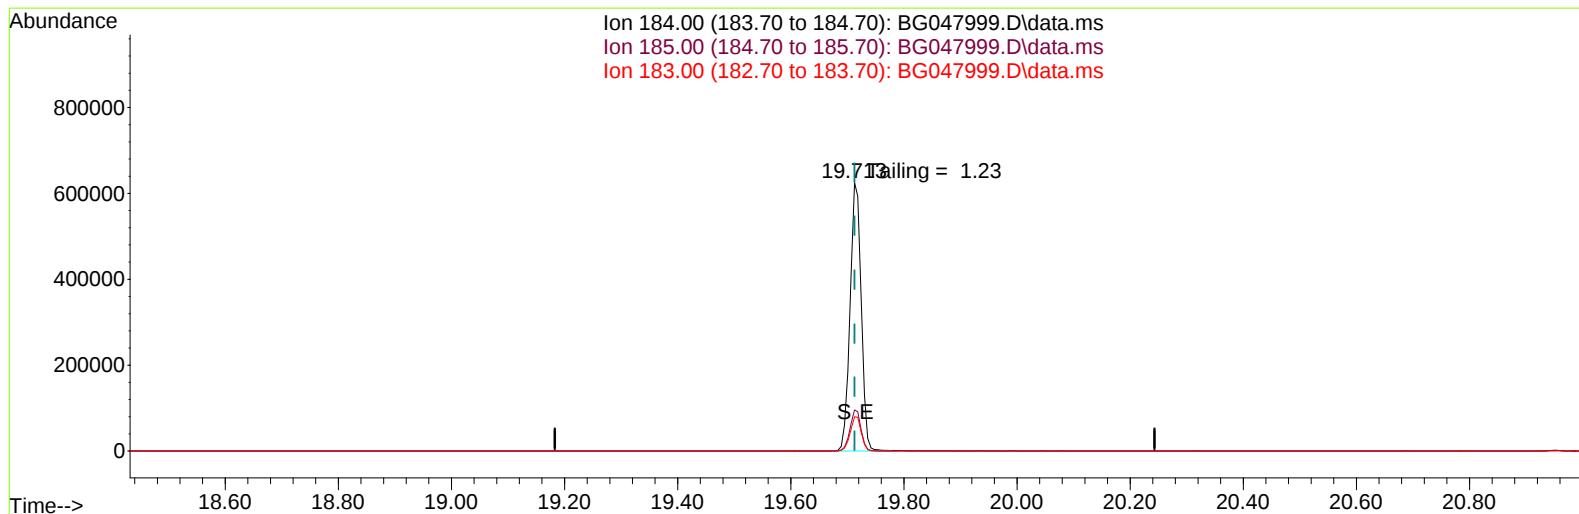

TIC: BG047999.D\data.ms

(77) Benzidine**19.712min (-0.000) 12338.67 ng****response 858541**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.36
183.00	13.20	12.80
0.00	0.00	0.00