
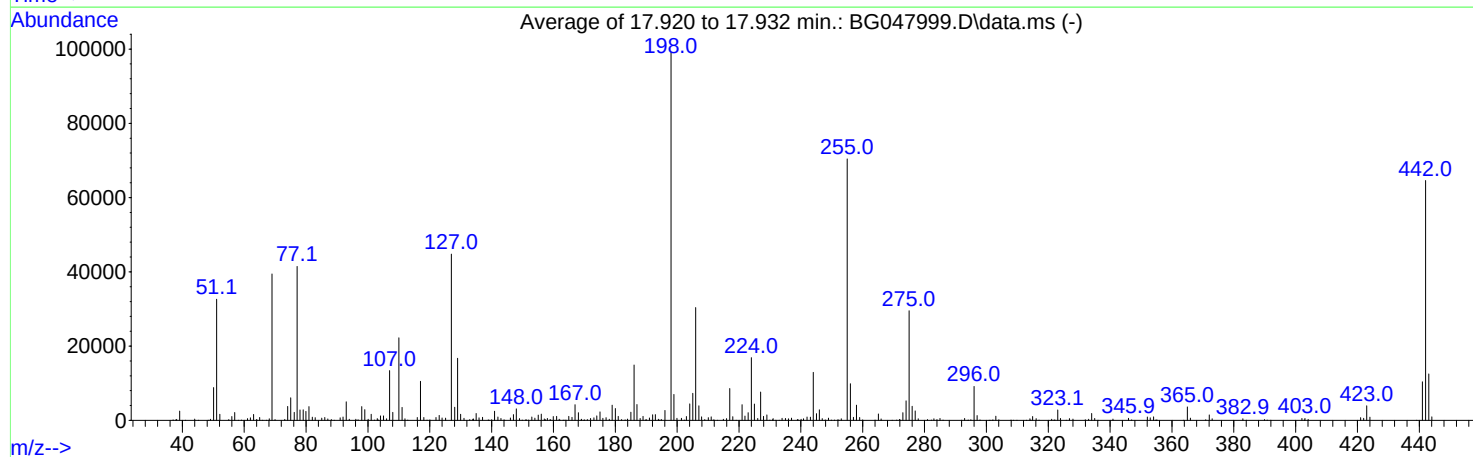


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012621\
 Data File : BG047999.D
 Acq On : 26 Jan 2021 8:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 19:39:42 2021

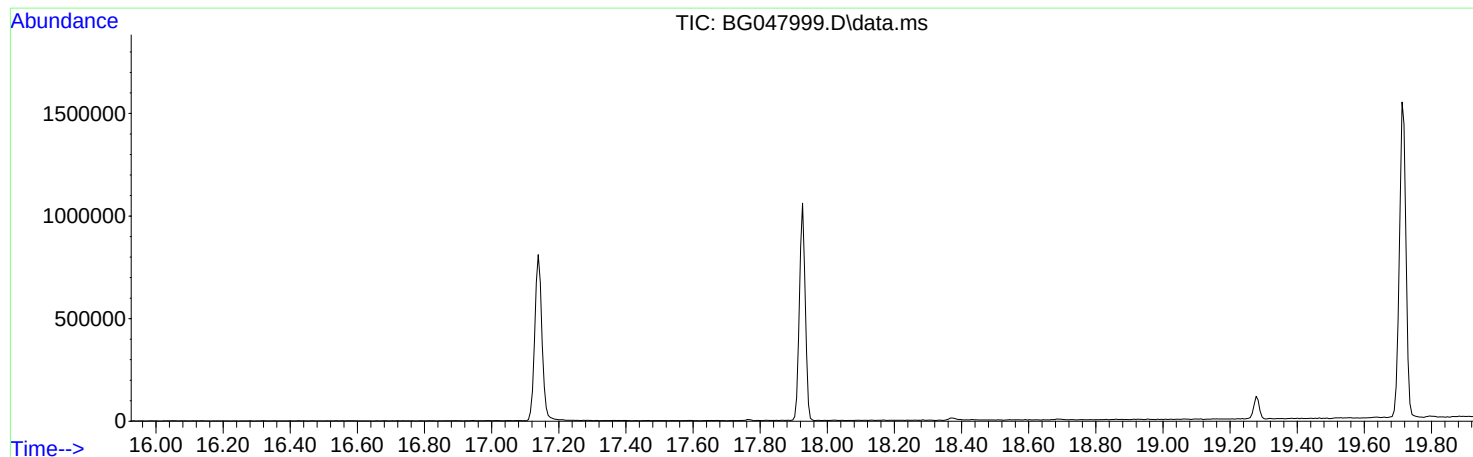

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	32621	PASS
68	69	0.00	2	1.1	447	PASS
69	198	0.00	100	39.8	39448	PASS
70	69	0.00	2	0.5	210	PASS
127	198	10	80	45.2	44776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99083	PASS
199	198	5	9	7.1	6987	PASS
275	198	10	60	29.8	29528	PASS
365	198	1	100	3.7	3636	PASS
441	198	0.01	100	10.5	10390	PASS
442	198	50	100	65.2	64613	PASS
443	442	15	24	19.4	12503	PASS