
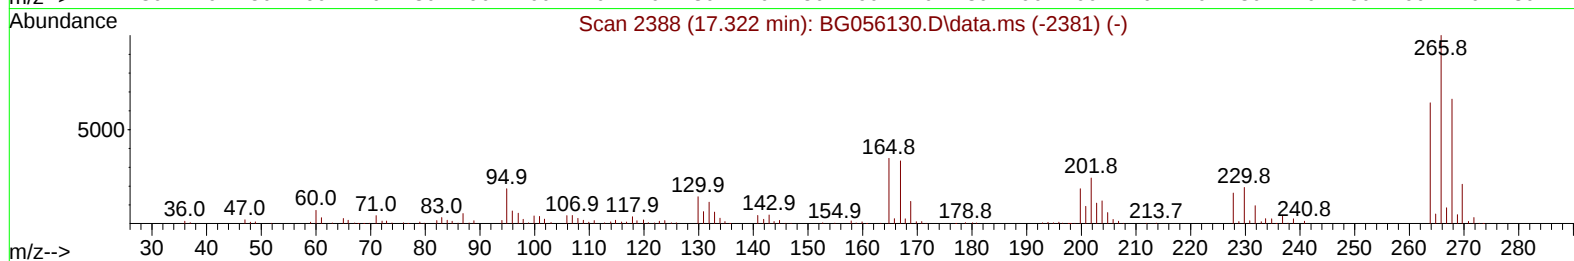
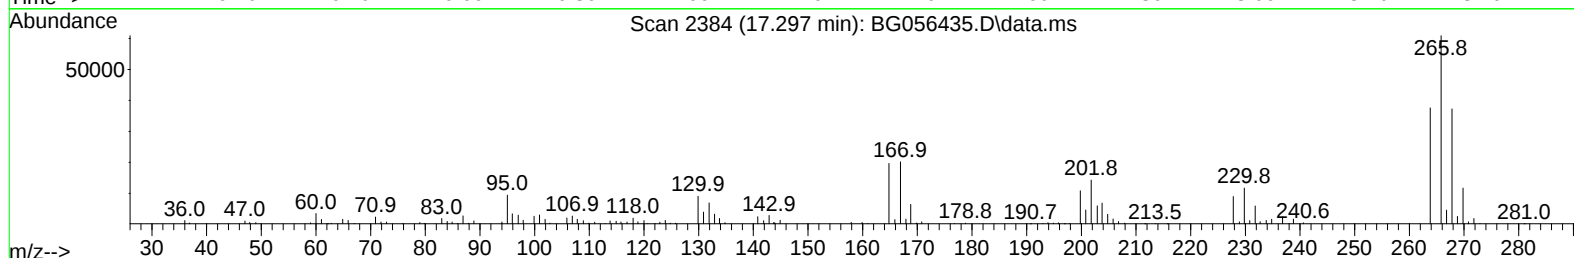


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012623\
Data File : BG056435.D
Acq On : 26 Jan 2023 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 01:55:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

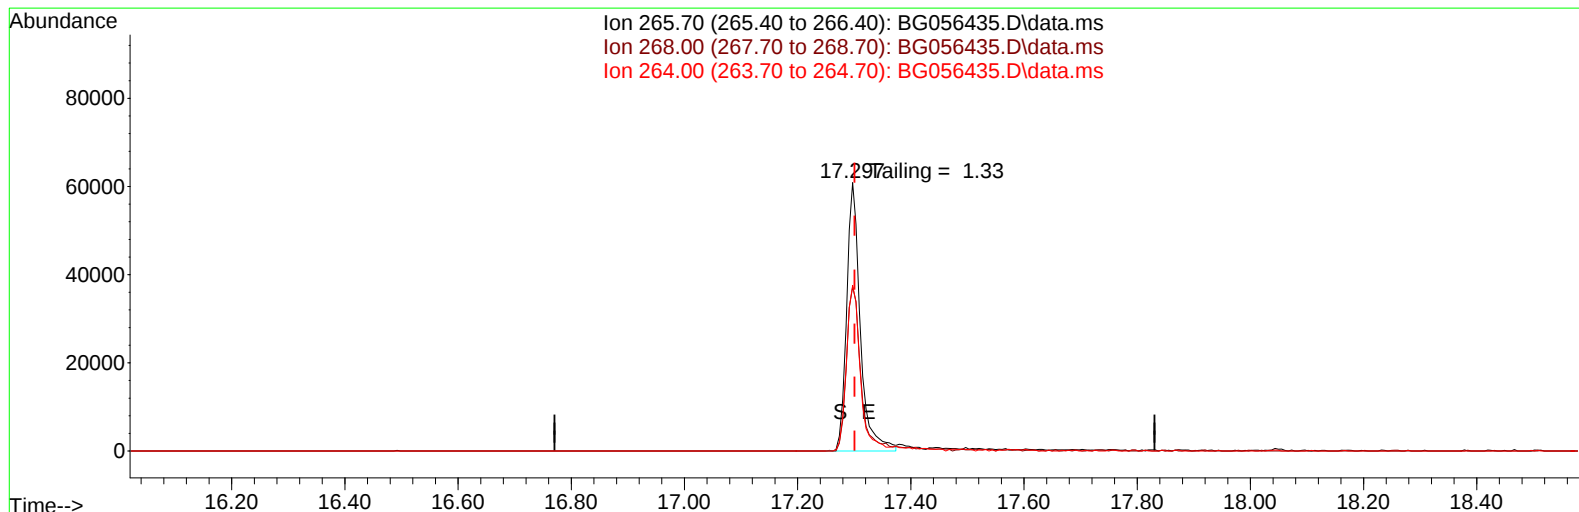

TIC: BG056435.D\data.ms

(70) Pentachlorophenol (C)




17.297min (-0.003) 27152.26 ng

response 102093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	61.20
264.00	64.30	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012623\
Data File : BG056435.D
Acq On : 26 Jan 2023 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 01:55:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

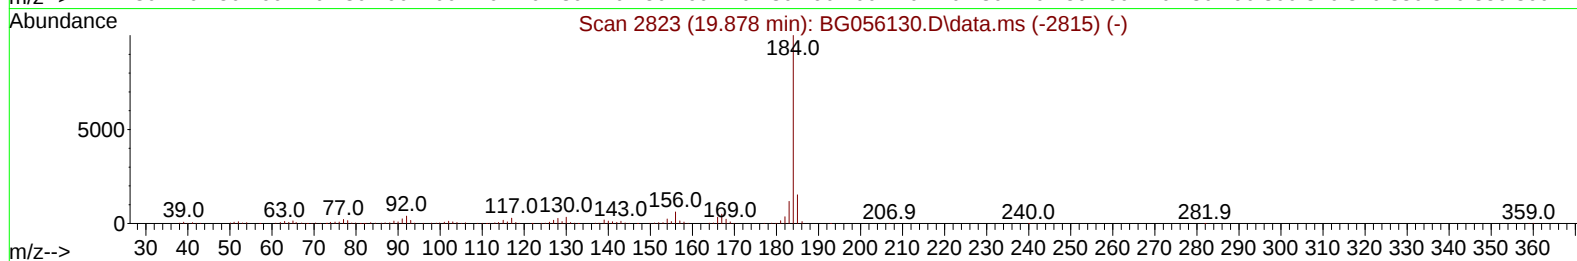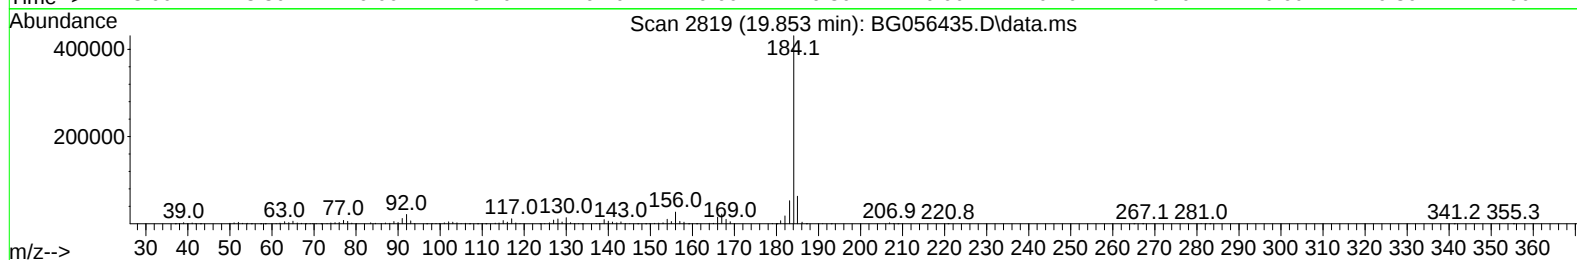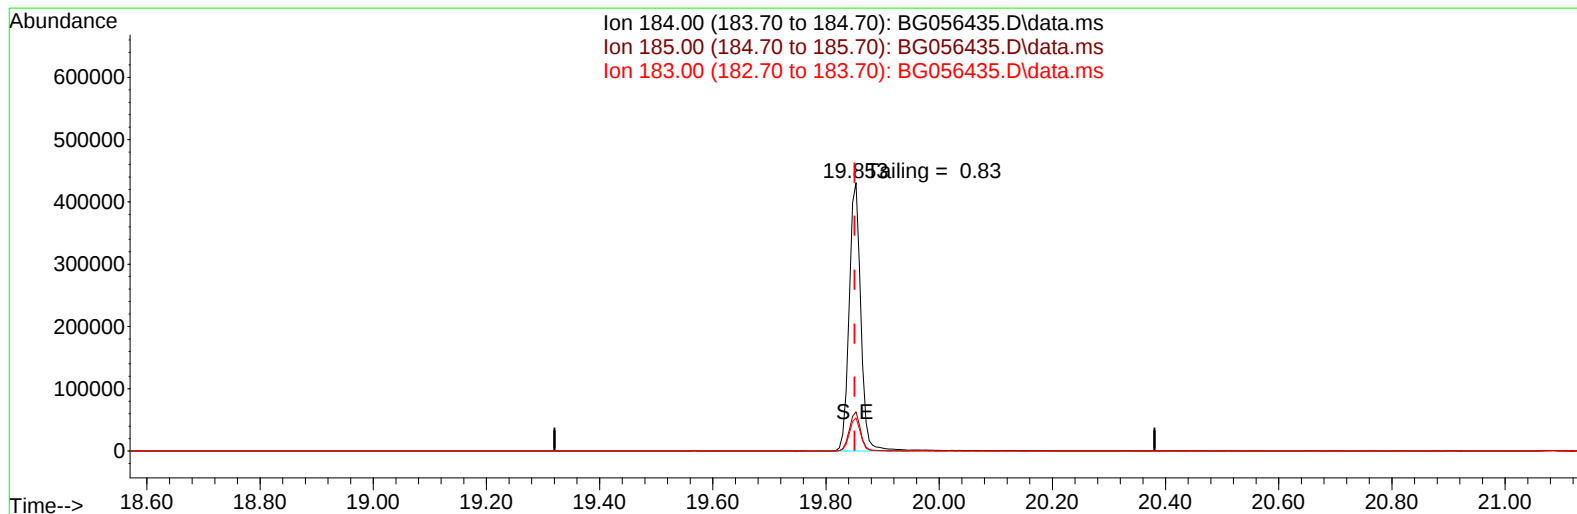

TIC: BG056435.D\data.ms

(77) Benzidine

19.853min (+ 0.003) 0.00 ng

response 614344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.64
183.00	11.70	12.33
0.00	0.00	0.00