


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012716\
Data File : BG020759.D
Acq On : 27 Jan 2016 9:33
Operator : SJ/IZ
Sample : DFTPP25
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP25

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 27 17:29:07 2016

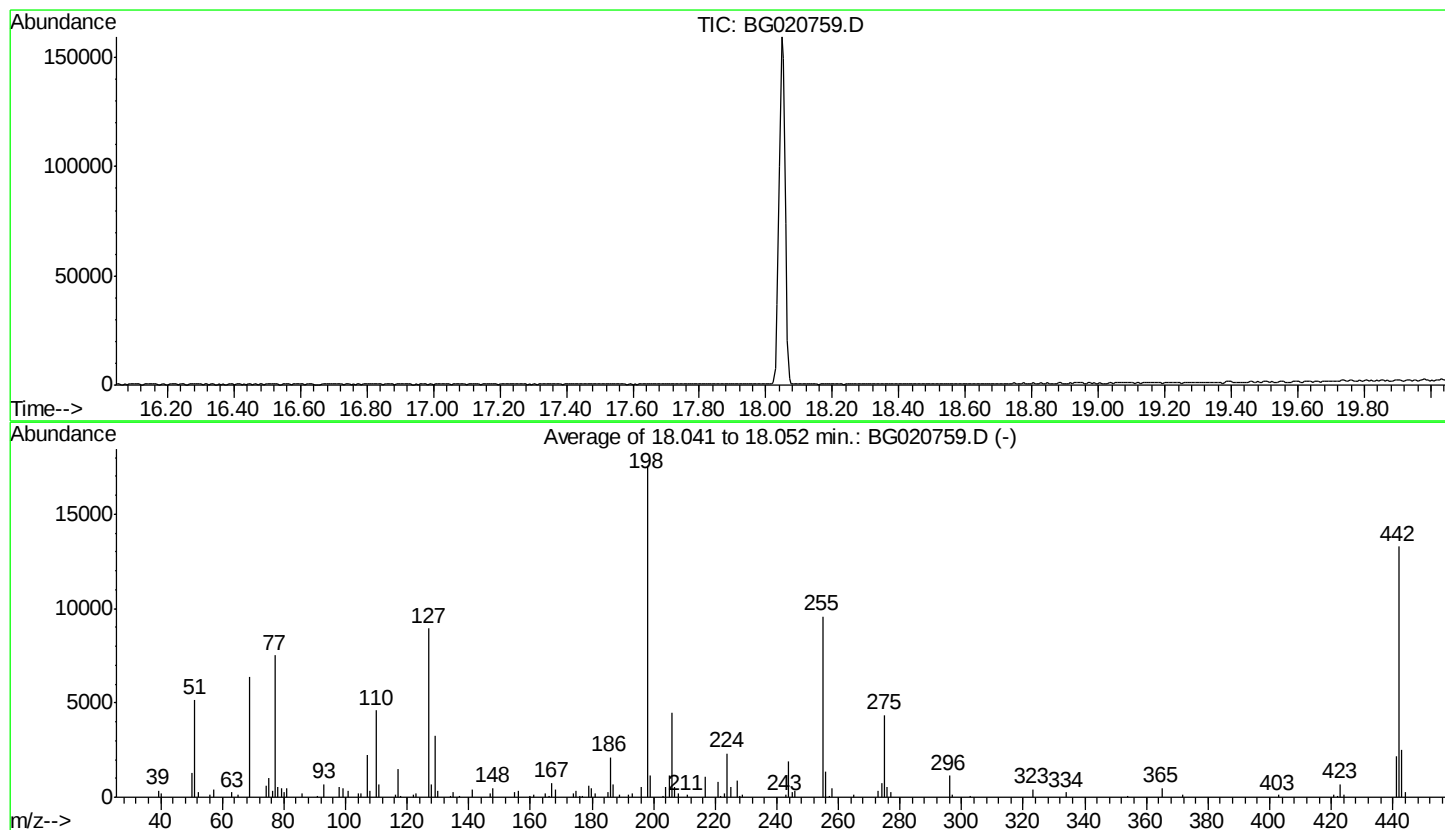

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	5161	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	6383	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	8933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17566	PASS
199	198	5	9	6.5	1143	PASS
275	198	10	60	24.7	4344	PASS
365	198	1	100	2.8	493	PASS
441	442	0.01	100	16.5	2190	PASS
442	198	50	100	75.6	13277	PASS
443	442	15	24	19.1	2542	PASS

m/z	Abundance
44.05	224.0
206.95	316.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25

m/z	Abundance
39.15	265.0
40.05	185.0
44.05	266.0
50.05	1154.0
51.15	4688.0
52.15	226.0
57.05	380.0
63.15	213.0
65.15	180.0
69.05	5485.0
74.05	475.0
75.05	960.0
76.15	323.0
77.15	6301.0
78.05	399.0
79.05	411.0
80.05	241.0
80.95	361.0
85.95	182.0
93.05	639.0
98.05	489.0
99.05	409.0
100.95	266.0
103.95	153.0
105.05	171.0
107.05	1743.0
107.95	231.0
110.05	3626.0
110.95	535.0
117.05	1240.0
122.95	238.0
127.05	7270.0
128.05	548.0
129.05	2623.0
129.95	297.0
135.05	212.0
141.05	333.0
147.05	218.0
147.95	374.0
155.05	193.0
156.05	206.0
164.95	206.0
167.05	616.0
167.95	327.0
173.95	155.0
175.05	205.0
178.95	470.0
179.95	336.0
181.05	150.0
184.95	249.0
185.95	1664.0
186.95	514.0
193.05	266.0
195.95	426.0
197.95	13323.0
198.95	906.0
203.95	415.0
204.95	783.0
205.95	3446.0
206.95	755.0
207.95	209.0
216.95	779.0
221.05	574.0
223.95	1681.0
224.95	438.0
226.95	581.0
243.95	1308.0
244.95	176.0
245.95	245.0
254.95	6643.0
255.95	902.0
257.95	347.0
272.95	243.0
273.95	482.0
274.95	3035.0
275.95	451.0
276.95	202.0
295.95	716.0
322.95	264.0
333.95	161.0
364.85	295.0
422.95	353.0
440.95	1210.0
441.95	7766.0
442.85	1319.0
443.85	171.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25

m/z	Abundance
39.15	439.0
40.05	163.0
44.05	171.0
50.15	1503.0
51.15	6253.0
52.15	402.0
56.05	159.0
57.05	454.0
63.05	310.0
69.05	7486.0
74.05	747.0
75.05	1253.0
76.15	353.0
77.15	8690.0
78.05	699.0
79.05	560.0
80.05	366.0
81.05	578.0
86.05	237.0
93.05	812.0
98.05	661.0
98.95	500.0
101.05	398.0
103.95	223.0
104.95	289.0
107.05	2584.0
107.95	456.0
110.05	5428.0
111.05	921.0
116.15	174.0
117.05	1707.0
121.95	191.0
123.05	244.0
127.05	10604.0
128.05	880.0
129.05	3813.0
130.05	336.0
133.95	183.0
135.05	325.0
136.95	162.0
141.05	517.0
147.05	243.0
147.95	527.0
155.05	298.0
156.05	395.0
159.95	190.0
161.05	234.0
164.95	245.0
165.95	170.0
166.95	820.0
167.95	418.0
173.95	181.0
175.05	376.0
175.95	162.0
176.95	197.0
178.95	686.0
179.95	455.0
181.05	251.0
185.05	322.0
185.95	2481.0
187.05	784.0
188.95	158.0
191.95	250.0
192.95	233.0
195.95	588.0
197.95	19848.0
198.95	1333.0
203.95	611.0
204.95	1299.0
205.95	5118.0
206.95	892.0
207.95	238.0
210.95	212.0
216.95	1173.0
220.95	911.0
221.95	190.0
222.95	299.0
223.95	2769.0
225.05	694.0
226.95	1093.0
227.85	176.0
228.85	275.0
242.95	197.0
243.95	2390.0
244.95	340.0
245.95	422.0
254.95	11167.0
255.95	1710.0
256.95	160.0
257.95	551.0
264.95	255.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25

272.95	440.0
273.95	888.0
274.95	4932.0
275.95	725.0
276.95	397.0
295.95	1220.0
296.95	157.0
302.95	175.0
322.95	483.0
333.95	319.0
353.95	154.0
364.95	641.0
371.95	198.0
402.85	173.0
420.85	165.0
422.95	754.0
423.95	209.0
440.95	2580.0
441.95	14194.0
442.95	3123.0
443.95	271.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25

m/z	Abundance
39.15	365.0
40.05	170.0
44.05	198.0
50.15	1218.0
51.15	4544.0
52.05	213.0
56.05	159.0
57.05	387.0
63.15	233.0
65.05	154.0
69.05	6178.0
74.05	541.0
75.05	921.0
76.15	347.0
77.15	7547.0
78.05	465.0
79.05	366.0
80.05	304.0
81.05	503.0
85.95	168.0
91.05	156.0
93.05	632.0
98.05	491.0
98.95	472.0
100.95	261.0
104.05	216.0
105.05	207.0
107.05	2303.0
108.05	280.0
110.05	4689.0
111.05	652.0
116.05	178.0
117.05	1539.0
117.95	153.0
121.95	156.0
122.95	236.0
127.05	8927.0
128.05	558.0
129.05	3327.0
129.95	304.0
135.05	304.0
140.95	463.0
147.05	217.0
147.95	525.0
154.95	246.0
156.05	345.0
161.05	209.0
164.95	169.0
167.05	866.0
168.05	402.0
174.05	205.0
174.95	394.0
178.95	646.0
179.95	578.0
180.95	235.0
185.05	295.0
186.05	2260.0
186.95	692.0
188.95	195.0
191.95	232.0
192.95	218.0
195.95	666.0
197.95	19528.0
198.95	1192.0
202.85	164.0
203.95	690.0
205.05	1305.0
206.05	4880.0
207.05	942.0
207.95	266.0
210.95	157.0
216.95	1238.0
220.95	905.0
222.95	370.0
223.95	2503.0
224.95	594.0
226.95	926.0
228.95	229.0
242.95	162.0
243.95	1936.0
244.95	296.0
245.95	360.0
254.95	10921.0
255.95	1475.0
257.95	574.0
264.95	249.0
272.85	351.0
273.95	800.0
274.95	5067.0
275.95	542.0
276.95	322.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25

295.95	1487.0
296.95	156.0
322.95	536.0
333.95	326.0
364.95	544.0
371.95	256.0
402.85	205.0
420.85	152.0
421.95	175.0
422.95	994.0
423.85	175.0
440.95	2780.0
441.95	17872.0
442.95	3184.0
443.95	332.0

Instrument :
BNA_G
ClientSampleId :
DFTPP25