

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012718\
 Data File : BG032374.D
 Acq On : 28 Jan 2018 3:07
 Operator : SJ/JU
 Sample : J1307-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jan 28 03:44:19 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 24 14:02:41 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.72	152	30918	20.00	ng	0.00
21) Naphthalene-d8	11.60	136	114201	20.00	ng	0.00
38) Acenaphthene-d10	15.36	164	76144	20.00	ng	0.00
63) Phenanthrene-d10	18.09	188	231393	20.00	ng	0.00
75) Chrysene-d12	22.42	240	312421	20.00	ng	0.00
86) Perylene-d12	26.12	264	196046	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.16	112	203473	120.36	ng	0.00
7) Phenol-d6	7.83	99	227334	106.78	ng	0.00
23) Nitrobenzene-d5	9.92	82	171435	101.56	ng	0.00
41) 2,4,6-Tribromophenol	16.83	330	224243	177.97	ng	0.00
44) 2-Fluorobiphenyl	13.98	172	606781	98.81	ng	0.00
78) Terphenyl-d14	20.63	244	1464784	103.52	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.50	88	8921	13.736	ng	# 1
15) Benzyl Alcohol	9.05	79	3775	2.441	ng	# 53
18) Hexachloroethane	9.85	117	2141	2.795	ng	# 1
19) n-Nitroso-di-n-propylamine	9.92	70	25631	19.403	ng	# 82
31) Naphthalene	11.66	128	27542	4.868	ng	# 97
37) 2-Methylnaphthalene	13.22	142	12129	2.700	ng	# 90
50) 2,6-Dinitrotoluene	15.36	165	10101	7.303	ng	# 18
56) 2,4-Dinitrotoluene	15.36	165	10101	5.425	ng	# 16
64) 4,6-Dinitro-2-methylphenol	16.83	198	754	5.342	ng	# 43
66) 4-Bromophenyl-phenylether	16.83	248	18248	5.543	ng	# 1
76) Benzidine	20.63	184	21339	2.731	ng	# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012718\
Data File : BG032374.D
Acq On : 28 Jan 2018 3:07
Operator : SJ/JU
Sample : J1307-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jan 28 03:44:19 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

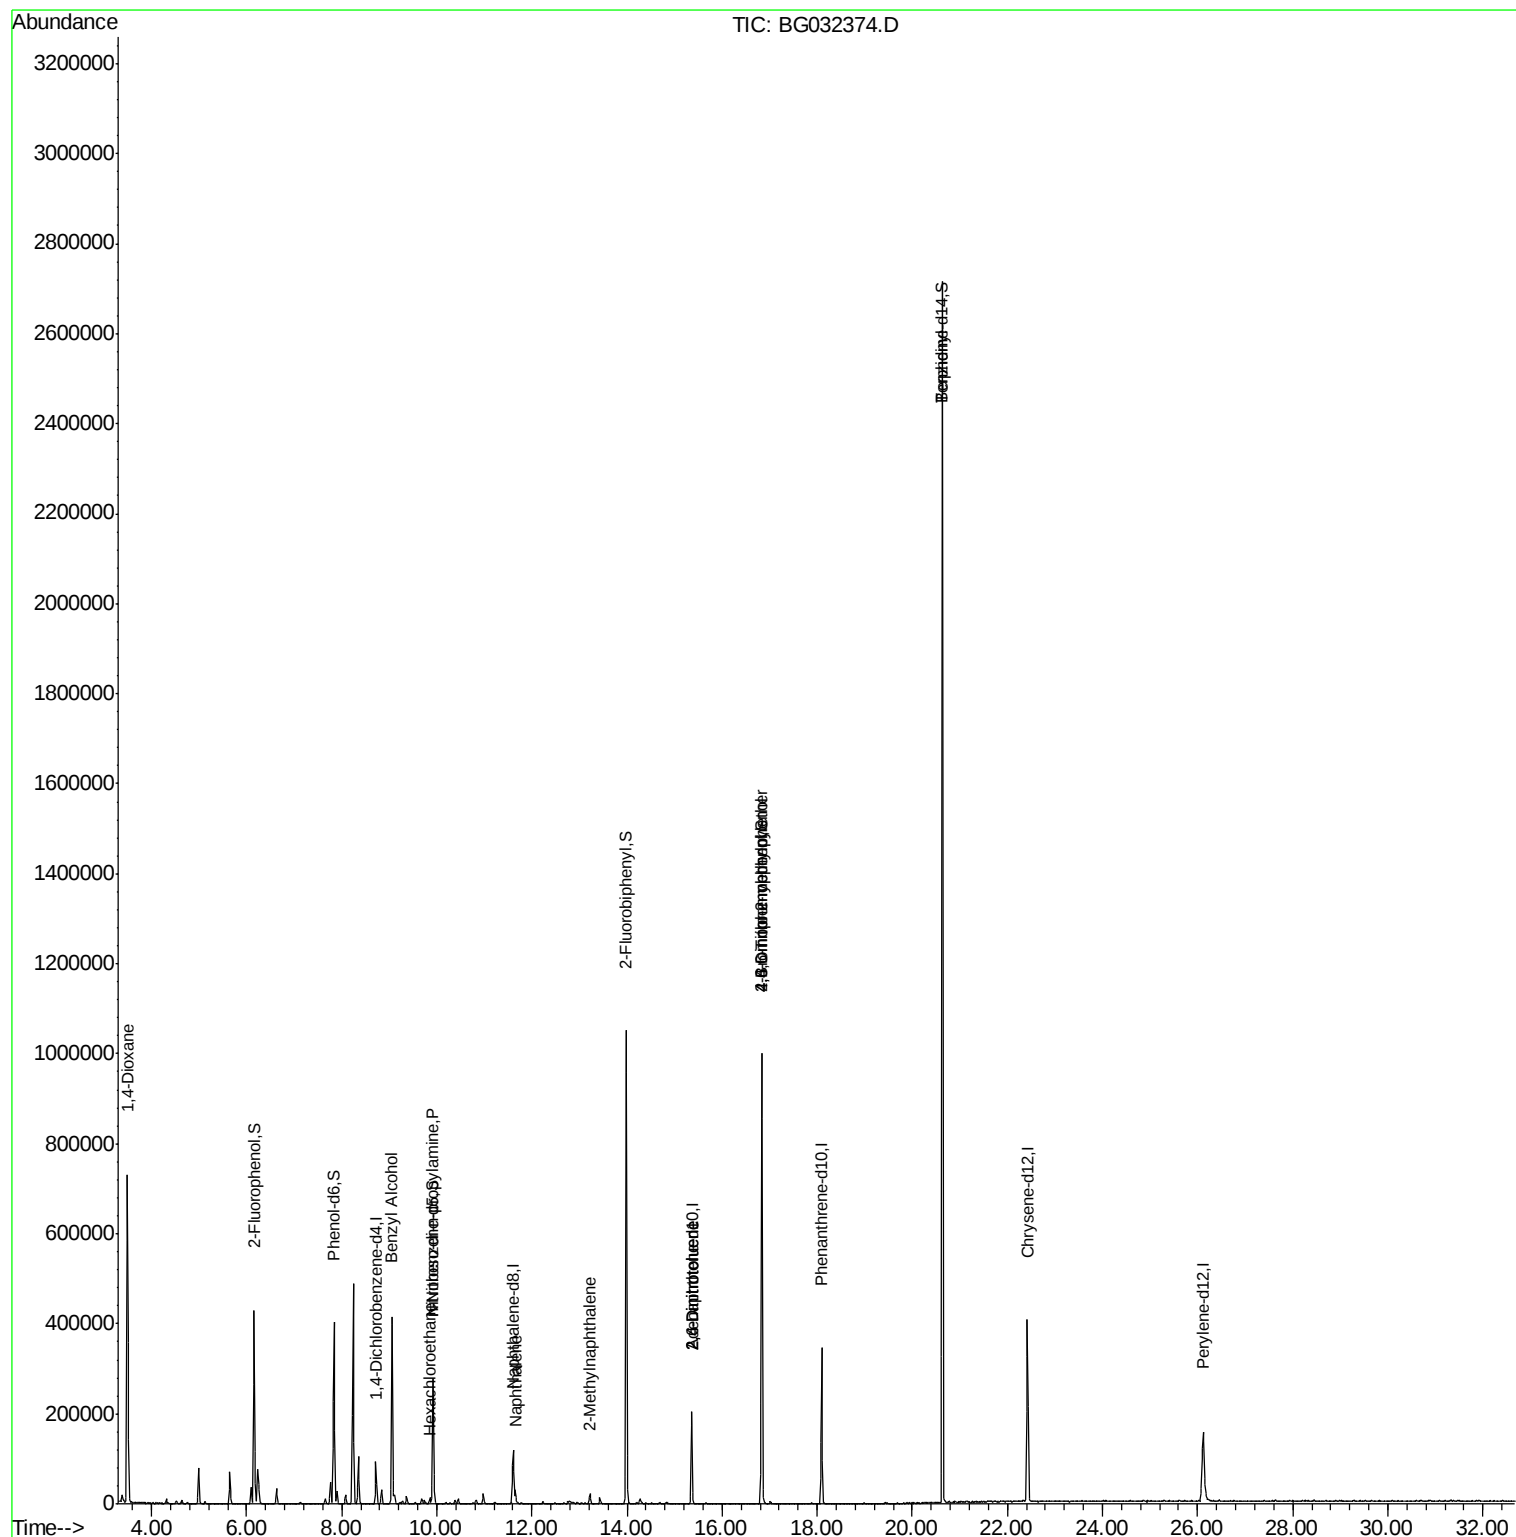



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.72 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07

Instrument :

BNA_G

ClientSampleId :





Tot Ion:152 Resp: 30918

Ion Ratio Lower Upper

152 100

150 140.0 126.6 189.8

115 55.6 53.0 79.4

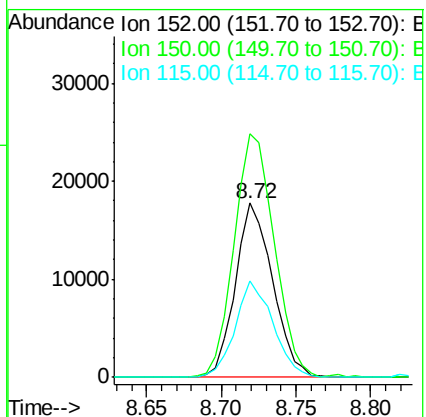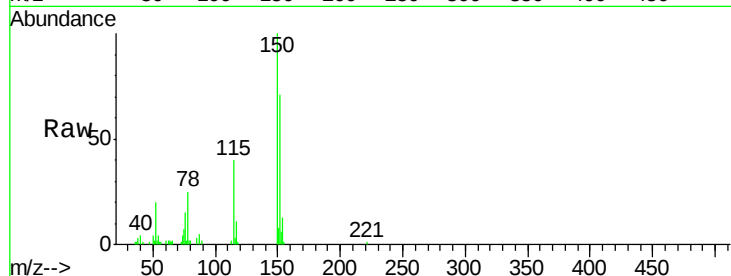

#2

1,4-Dioxane

Concen: 13.736 ng

RT: 3.50 min Scan# 35

Delta R.T. -0.33 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07




Tgt Ion: 88 Resp: 8921


Ion Ratio Lower Upper

88 100

58 41.3 79.6 119.4#

43 2129.2 27.4 41.0#

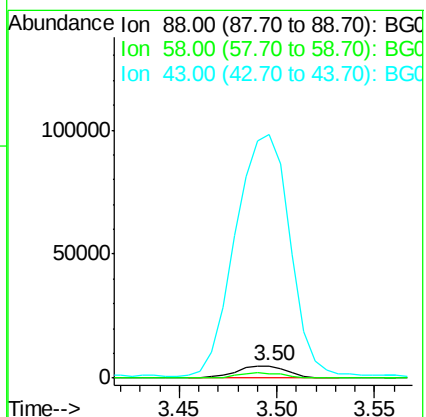



#5

2-Fluorophenol

Concen: 120.363 ng

RT: 6.16 min Scan# 488

Delta R.T. 0.00 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07

Instrument :

BNA_G

ClientSampleId :


Tot Ion:112 Resp: 203473

Ion Ratio Lower Upper




112 100

64 51.8 56.3 84.5#

63 32.3 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): BGC
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

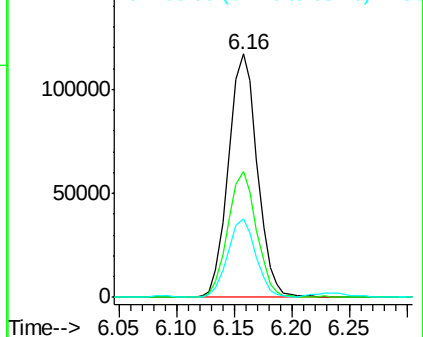

#7

Phenol-d6

Concen: 106.776 ng

RT: 7.83 min Scan# 773

Delta R.T. -0.00 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07


Tgt Ion: 99 Resp: 227334

Ion Ratio Lower Upper



99 100


42 19.0 14.1 21.1

71 49.2 26.1 39.1#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

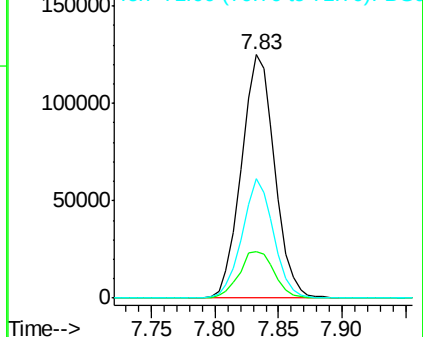

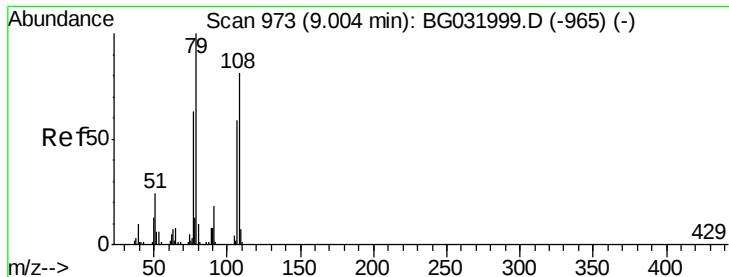

#15

Benzyl Alcohol

Concen: 2.441 ng

RT: 9.05 min Scan# 980

Delta R.T. 0.08 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 79 Resp: 3775

Ion Ratio Lower Upper

79 100

108 21.4 57.2 85.8#

77 80.7 46.1 69.1#

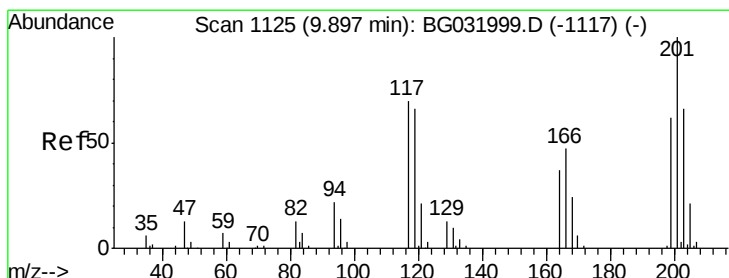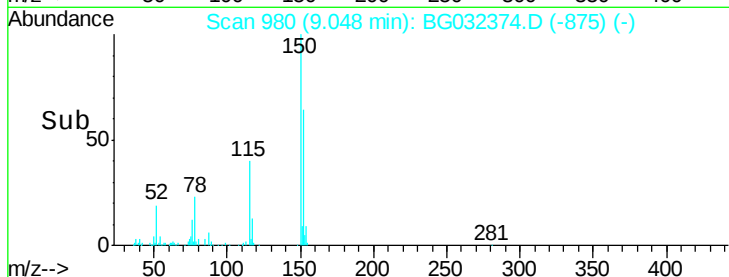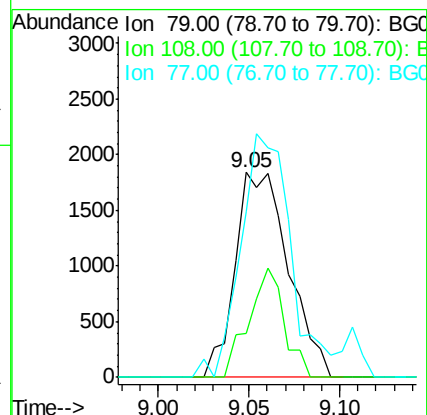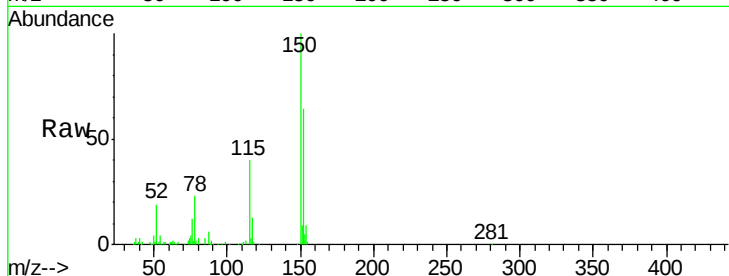

#18

Hexachloroethane

Concen: 2.795 ng

RT: 9.85 min Scan# 1116

Delta R.T. 0.00 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07




Tgt Ion: 117 Resp: 2141


Ion Ratio Lower Upper

117 100

119 428.9 76.7 115.1#

201 0.0 95.7 143.5#


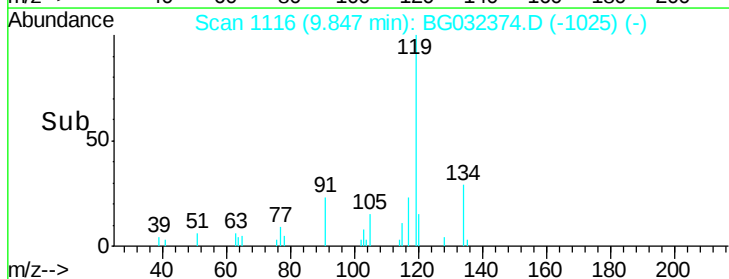
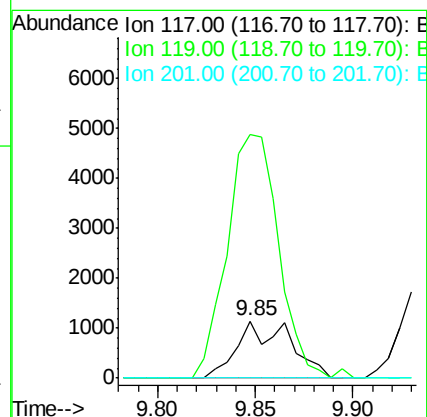
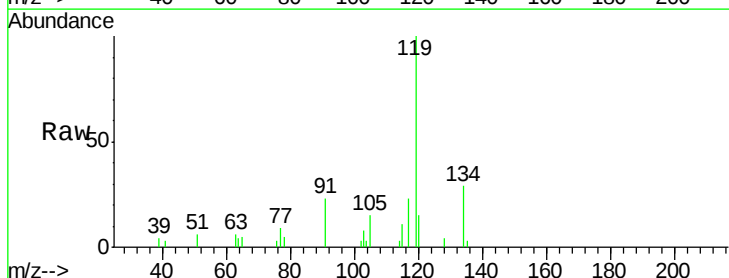


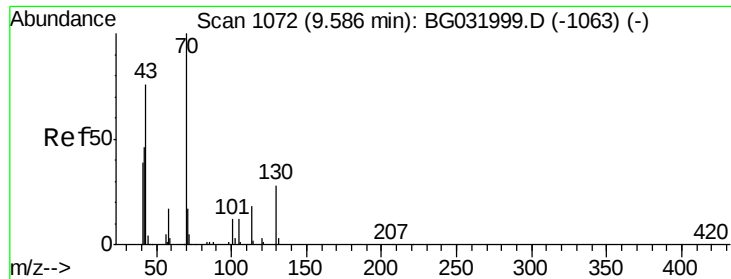

#19
n-Nitroso-di-n-propylamine
Concen: 19.403 ng
RT: 9.92 min Scan# 1129
Delta R.T. 0.38 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
70	100		
42	51.9	49.1	73.7
101	0.0	8.5	12.7#
130	2.3	13.4	20.0#

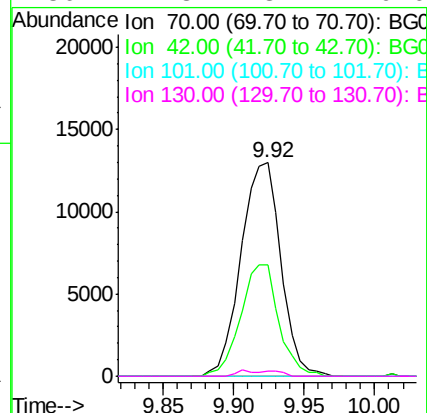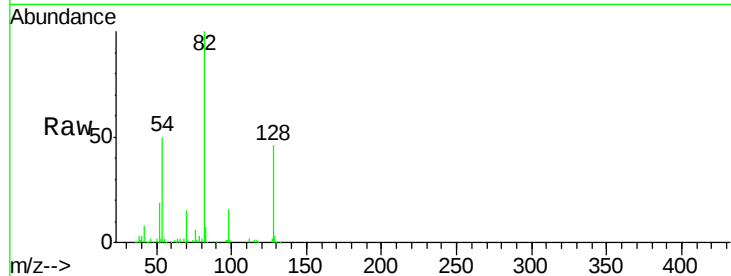

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.60 min Scan# 1415
Delta R.T. -0.00 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.2	13.8
54	5.0	10.3	15.5#
68	3.0	4.5	6.7#


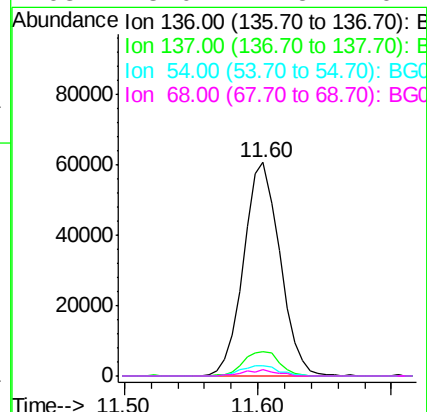




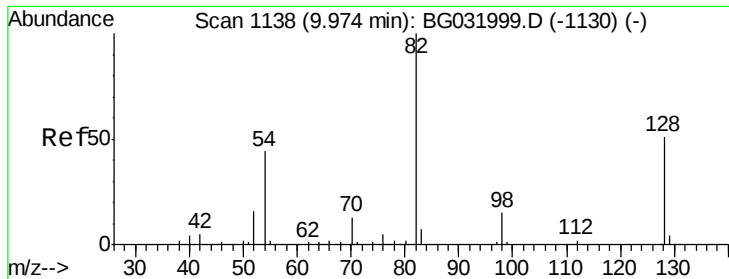

#23
 Nitrobenzene-d5
 Concen: 101.561 ng
 RT: 9.92 min Scan# 1128
 Delta R.T. -0.00 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07




Instrument :
 BNA_G
 ClientSampled :


Tot Ion: 82 Resp: 171435
 Ion Ratio Lower Upper
 82 100
 128 46.9 29.7 44.5#
 54 52.0 43.1 64.7

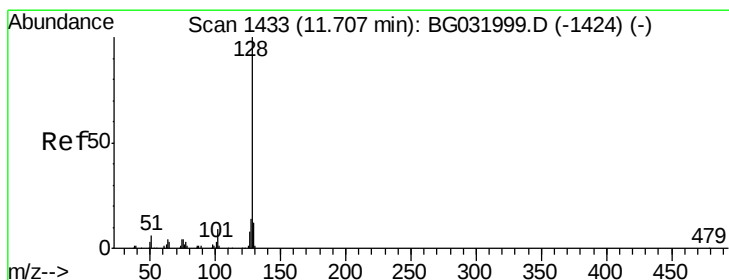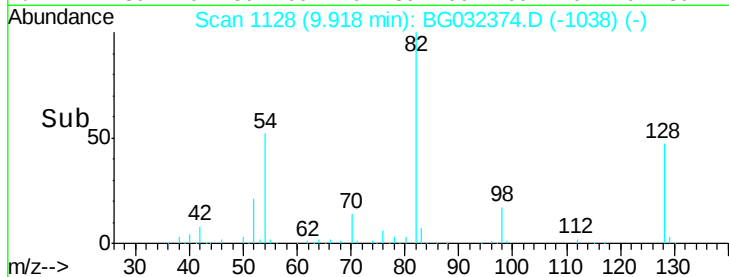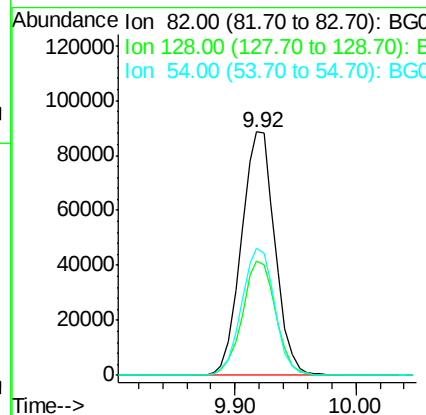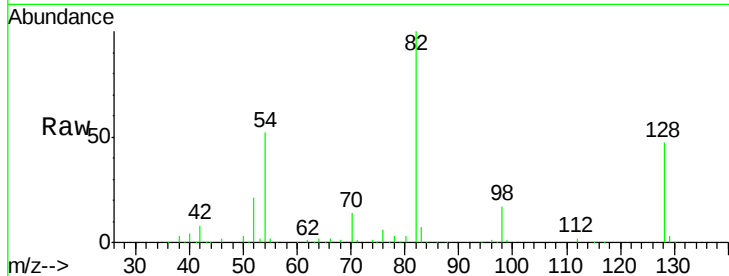

#31
 Naphthalene
 Concen: 4.868 ng
 RT: 11.66 min Scan# 1424
 Delta R.T. -0.00 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Tgt Ion: 128 Resp: 27542
 Ion Ratio Lower Upper
 128 100
 129 12.2 8.6 12.8
 127 13.9 11.6 17.4


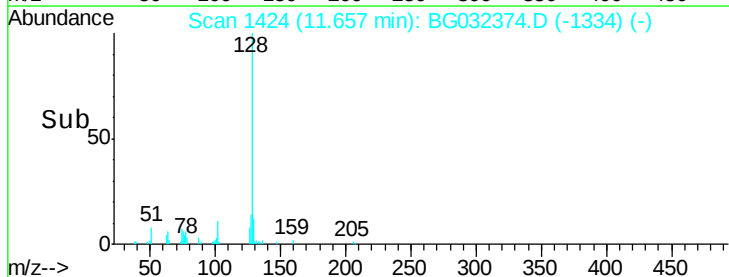
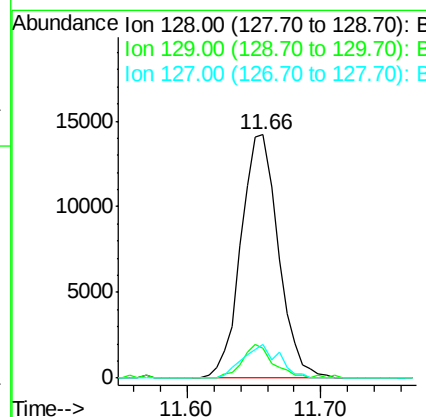
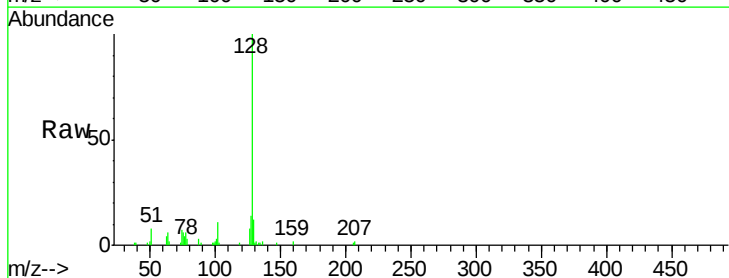


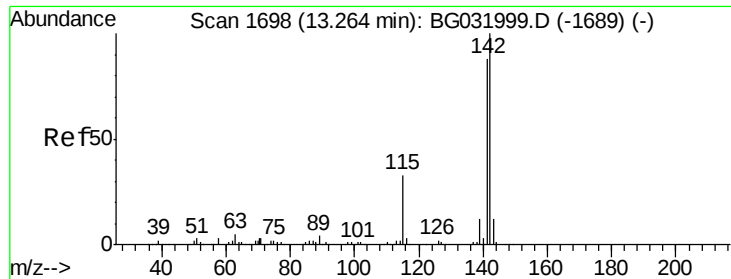

#37
2-Methylnaphthalene
Concen: 2.700 ng
RT: 13.22 min Scan# 1690
Delta R.T. -0.00 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07




Instrument :
BNA_G
ClientSampleId :


Tot Ion:142 Resp: 12129
Ion Ratio Lower Upper
142 100
141 94.6 67.1 100.7
115 42.2 30.7 46.1

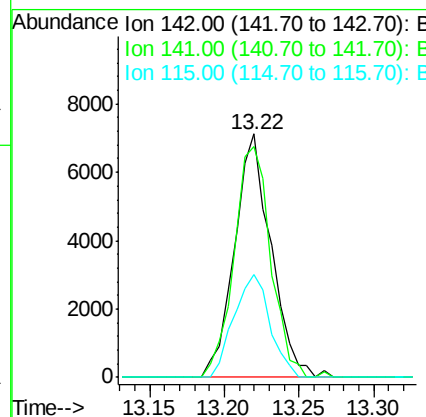

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.36 min Scan# 2054
Delta R.T. -0.00 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07

Tgt Ion:164 Resp: 76144
Ion Ratio Lower Upper
164 100
162 105.6 78.8 118.2
160 48.4 35.4 53.0

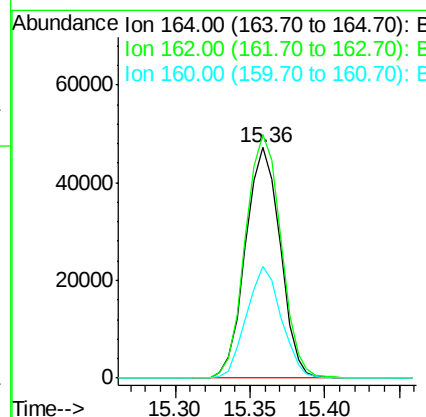


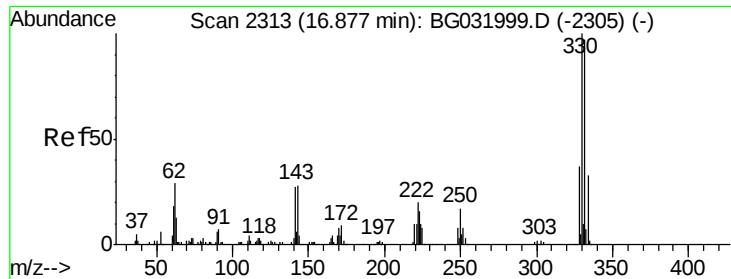




#41
 2,4,6-Tribromophenol
 Concen: 177.970 ng
 RT: 16.83 min Scan# 2305
 Delta R.T. -0.00 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	77.0	115.6
141	28.6	25.2	37.8

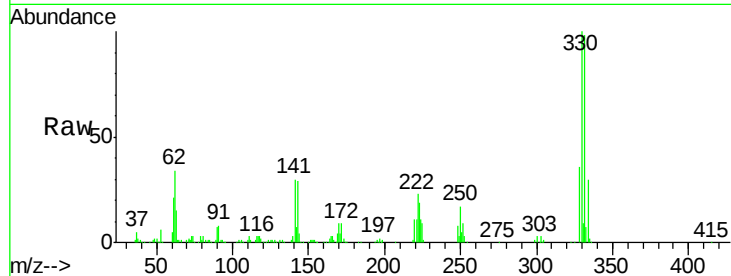


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

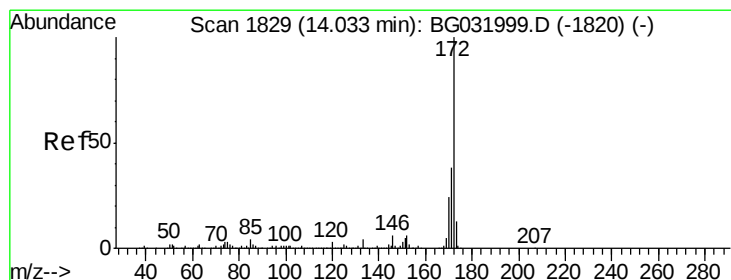
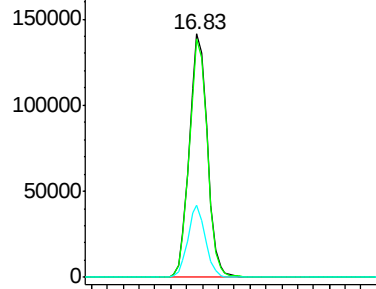



#44
 2-Fluorobiphenyl
 Concen: 98.810 ng
 RT: 13.98 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	30.0	45.0
170	23.0	19.5	29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




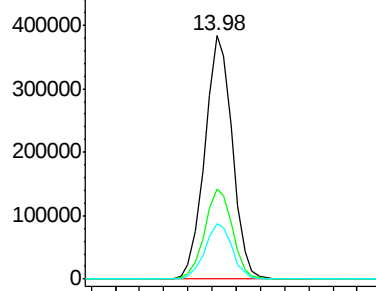


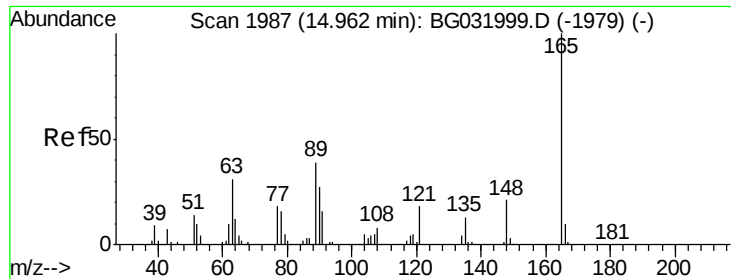

#50
 2,6-Dinitrotoluene
 Concen: 7.303 ng
 RT: 15.36 min Scan# 2054
 Delta R.T. 0.44 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	52.7	79.1#
89	0.0	49.2	73.8#

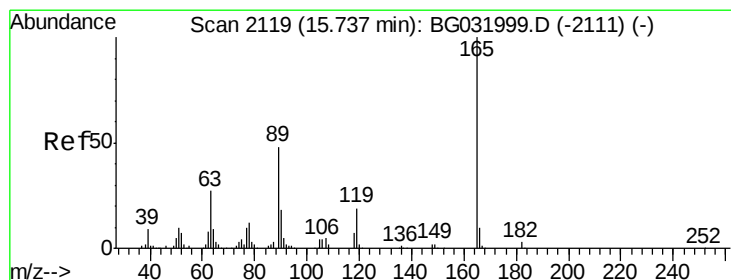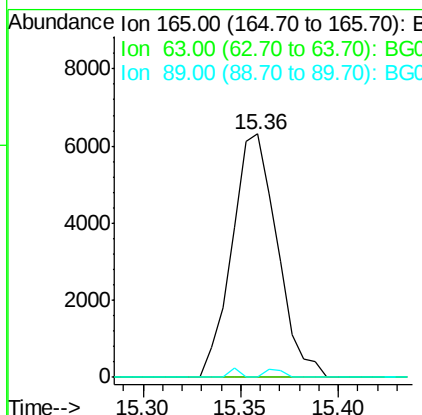

#56
 2,4-Dinitrotoluene
 Concen: 5.425 ng
 RT: 15.36 min Scan# 2054
 Delta R.T. -0.34 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	42.0	63.0#
89	0.0	66.9	100.3#
182	0.0	2.6	3.8#

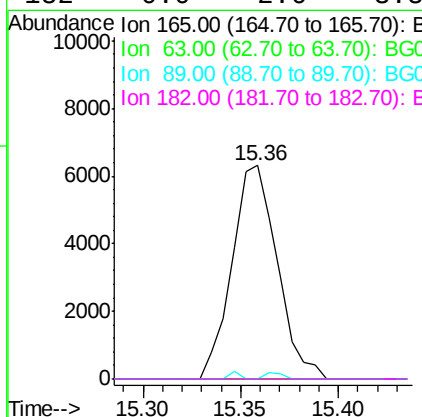







#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 18.09 min Scan# 2519
 Delta R.T. -0.00 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:188 Resp: 231393
 Ion Ratio Lower Upper
 188 100
 94 3.8 6.9 10.3#
 80 3.9 7.7 11.5#




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

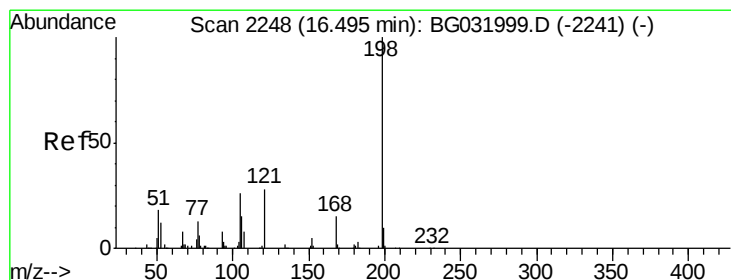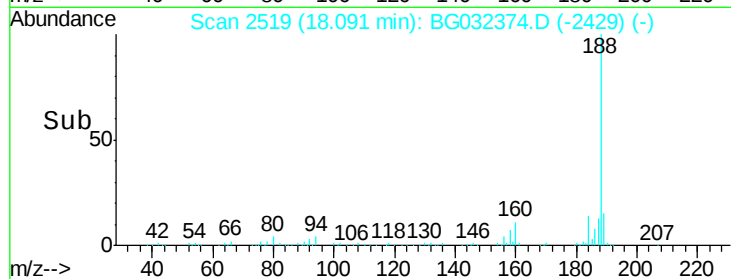
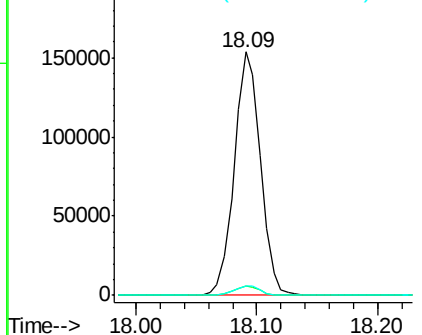



#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.342 ng
 RT: 16.83 min Scan# 2305
 Delta R.T. 0.38 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Tgt Ion:198 Resp: 754
 Ion Ratio Lower Upper
 198 100
 51 95.5 30.6 70.6#
 105 75.1 23.8 63.8#



Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BGC
 Ion 105.00 (104.70 to 105.70): E

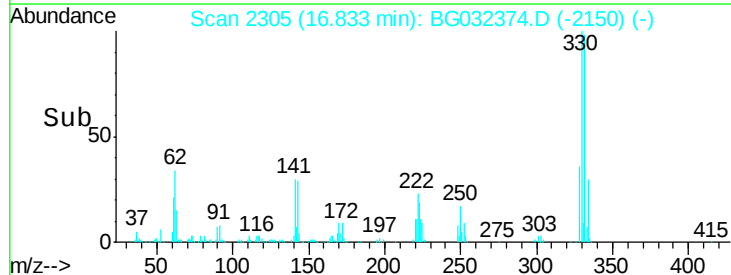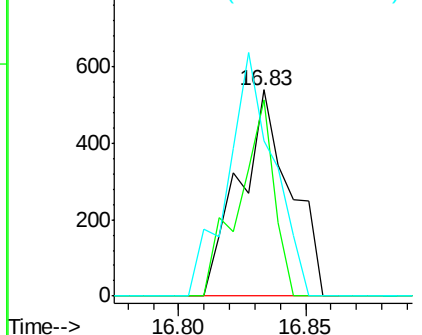


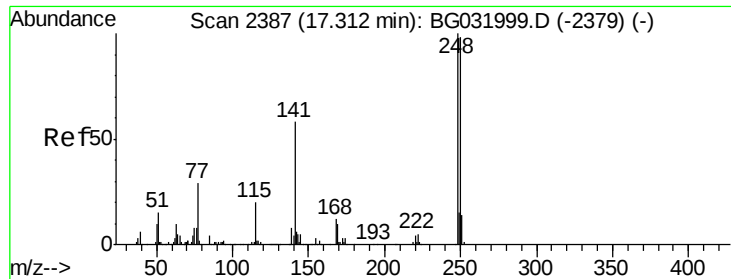




#66
4-Bromophenyl-phenylether
Concen: 5.543 ng
RT: 16.83 min Scan# 2305
Delta R.T. -0.43 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07

Instrument :
BNA_G
ClientSampled :

Tot Ion:248 Resp: 18248
Ion Ratio Lower Upper
248 100
250 215.5 77.1 115.7#
141 371.1 50.8 76.2#

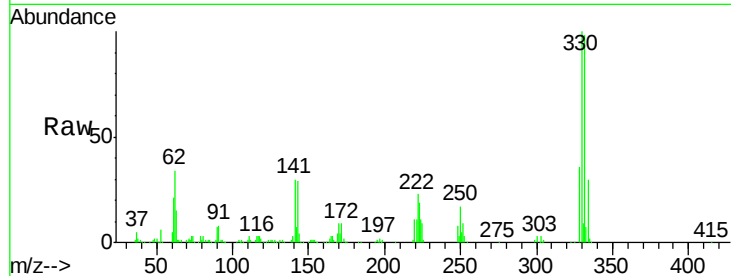


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

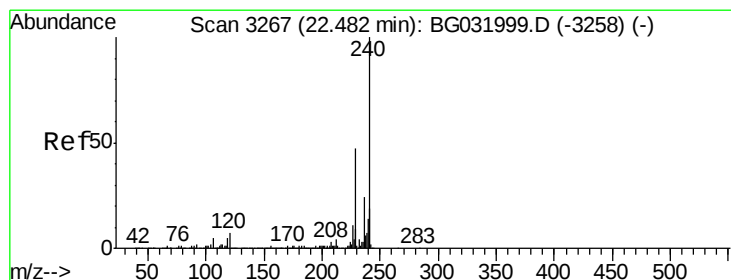
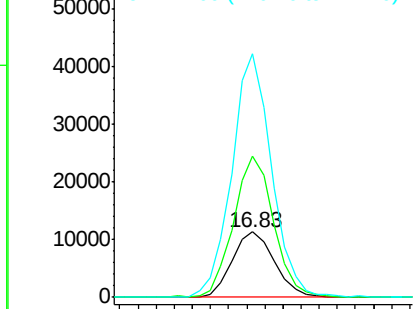



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.42 min Scan# 3256
Delta R.T. -0.00 min
Lab File: BG032374.D
Acq: 28 Jan 2018 3:07

Tgt Ion:240 Resp: 312421
Ion Ratio Lower Upper
240 100
120 4.3 6.8 10.2#
236 25.2 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

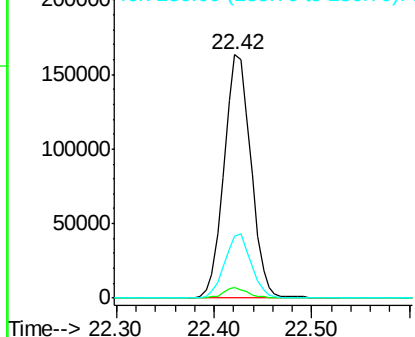



#76

Benzidine

Concen: 2.731 ng

RT: 20.63 min Scan# 2951

Delta R.T. 0.37 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 21339

Ion Ratio Lower Upper

184 100

185 14.6 11.1 16.7




183 10.1 10.6 16.0#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

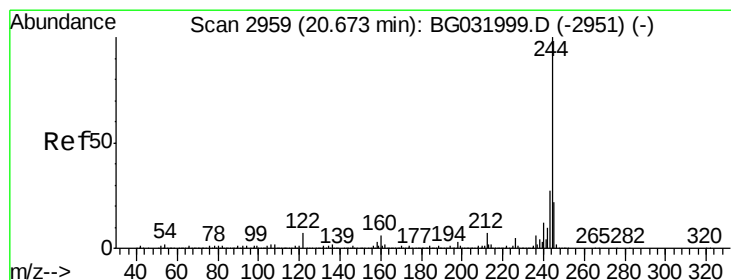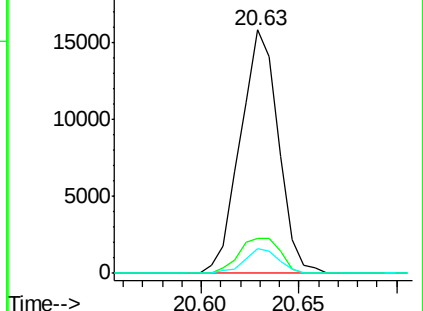

#78

Terphenyl-d14

Concen: 103.524 ng

RT: 20.63 min Scan# 2951

Delta R.T. -0.00 min

Lab File: BG032374.D

Acq: 28 Jan 2018 3:07


Tgt Ion:244 Resp: 1464784

Ion Ratio Lower Upper

244 100

212 7.5 5.8 8.8



122 5.7 7.0 10.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

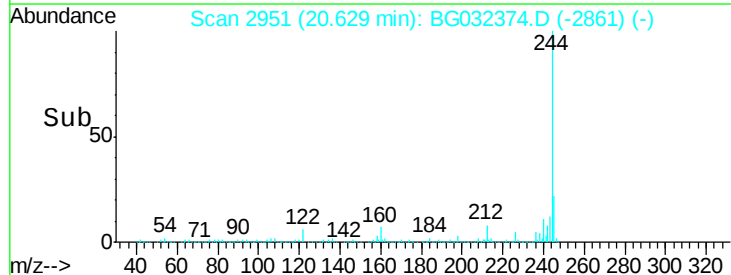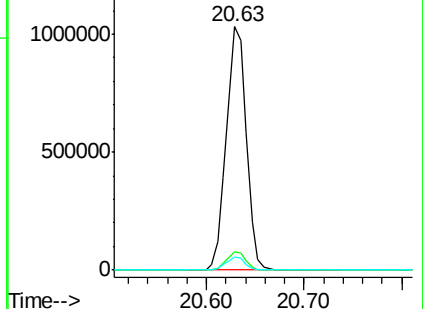

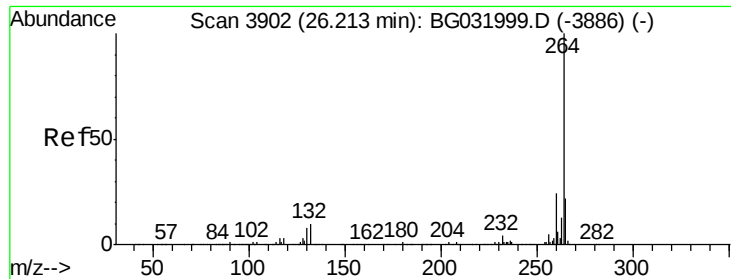

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 26.12 min Scan# 3885
 Delta R.T. 0.01 min
 Lab File: BG032374.D
 Acq: 28 Jan 2018 3:07

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	26.5	17.4	26.0#
265	19.6	17.7	26.5

