
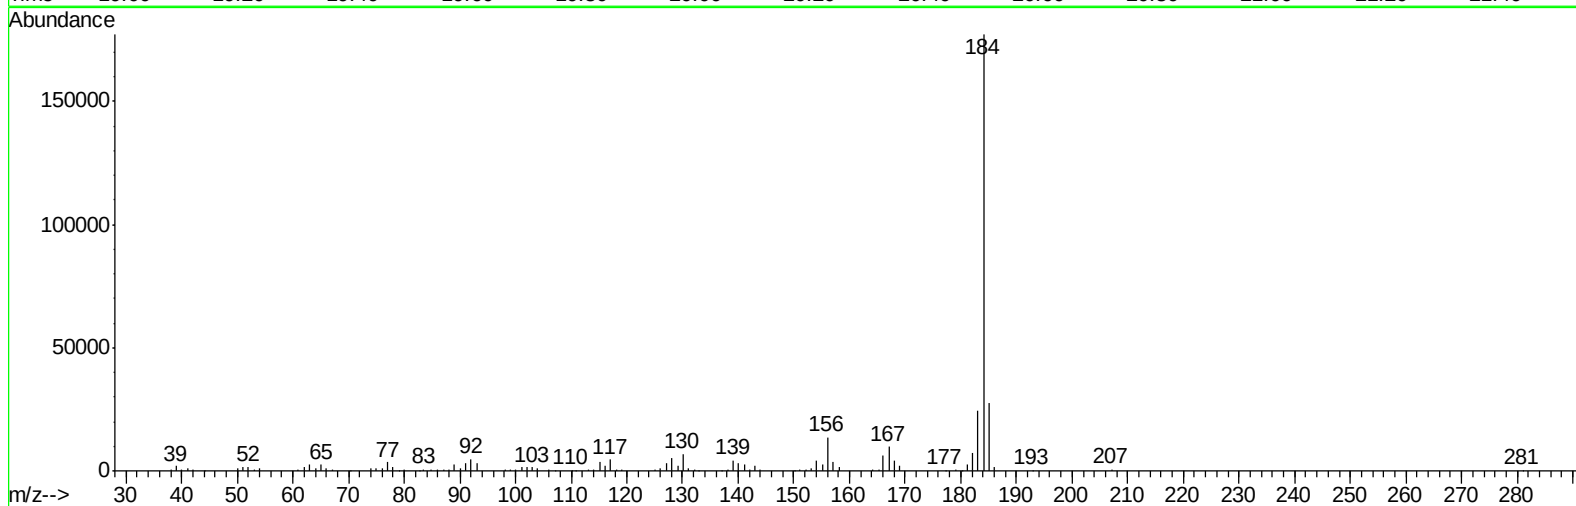


Data Path : Z:\HPCHEM1\BNA G\DATA\BG012718\
Data File : BG032346.D
Acq On : 27 Jan 2018 8:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:02:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

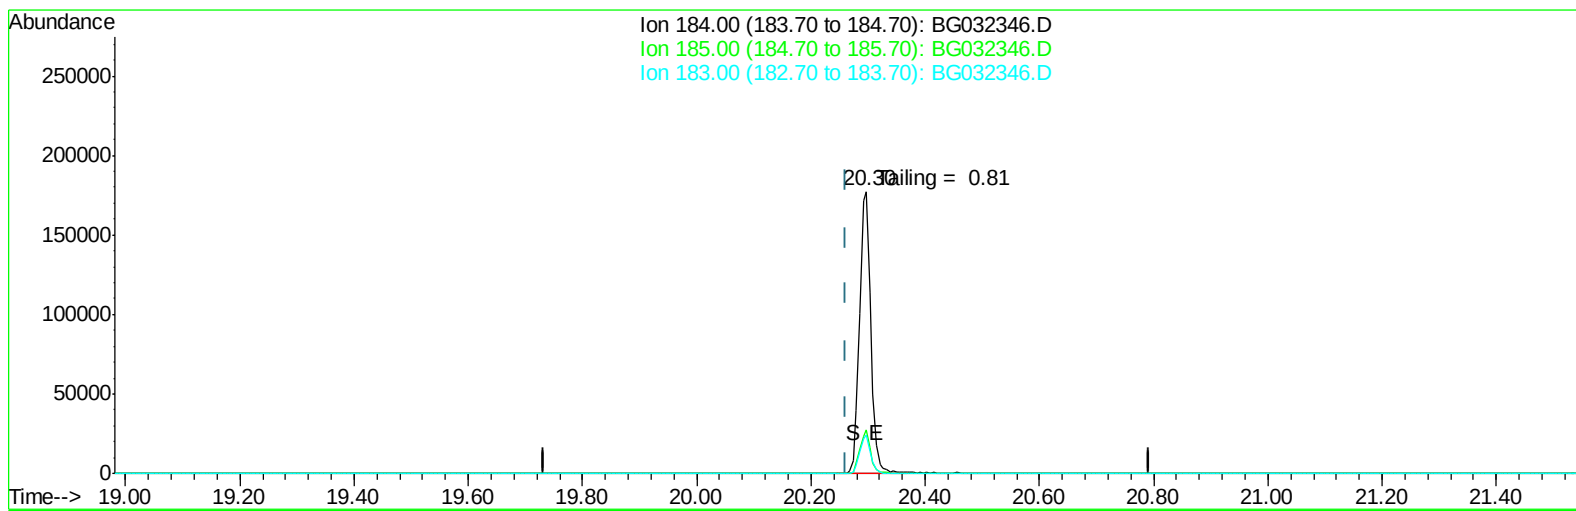

TIC: BG032346.D

(76) Benzidine



20.297min (+0.035) 0.00ng

response 246968

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.60
183.00	13.30	13.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012718\
Data File : BG032346.D
Acq On : 27 Jan 2018 8:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:02:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

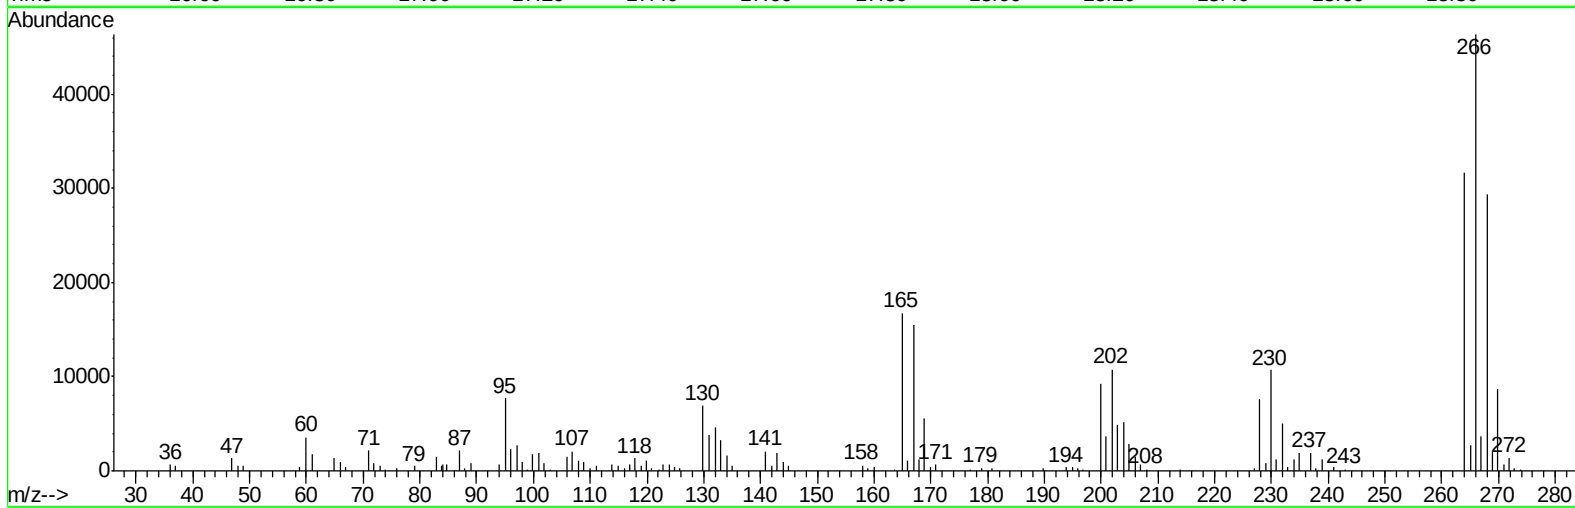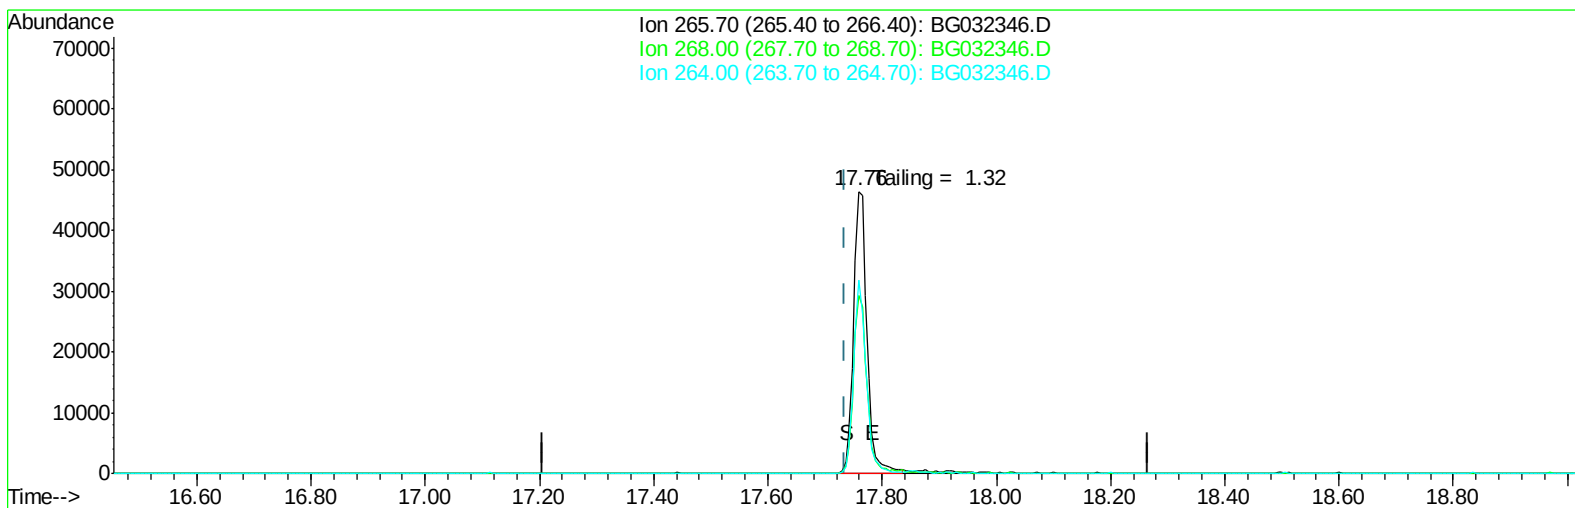

TIC: BG032346.D

(69) Pentachlorophenol (C)

17.759min (+0.023) 39378.64ng

response 76469

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.31
264.00	62.00	68.45
0.00	0.00	0.00