

Data Path : U:\HPCHEM1\BNA G\DATA\BG012718\
 Data File : BG032370.D
 Acq On : 28 Jan 2018 00:36
 Operator : SJ/JU
 Sample : J1010-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BU-01-012518

Quant Time: Jan 28 03:36:58 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 24 14:02:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.72	152	33818	20.00	ng	0.00
21) Naphthalene-d8	11.60	136	127512	20.00	ng	0.00
38) Acenaphthene-d10	15.36	164	86402	20.00	ng	0.00
63) Phenanthrene-d10	18.09	188	236773	20.00	ng	0.00
75) Chrysene-d12	22.41	240	321245	20.00	ng	-0.01
86) Perylene-d12	26.10	264	293134	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.16	112	231768	125.34	ng	0.00
7) Phenol-d6	7.84	99	256516	110.15	ng	0.00
23) Nitrobenzene-d5	9.92	82	198154	105.13	ng	0.00
41) 2,4,6-Tribromophenol	16.83	330	237359	166.01	ng	0.00
44) 2-Fluorobiphenyl	13.98	172	672745	96.55	ng	0.00
78) Terphenyl-d14	20.63	244	1496040	102.83	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG012718\
Data File : BG032370.D
Acq On : 28 Jan 2018 00:36
Operator : SJ/JU
Sample : J1010-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BU-01-012518

Quant Time: Jan 28 03:36:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 14:02:41 2018
Response via : Initial Calibration

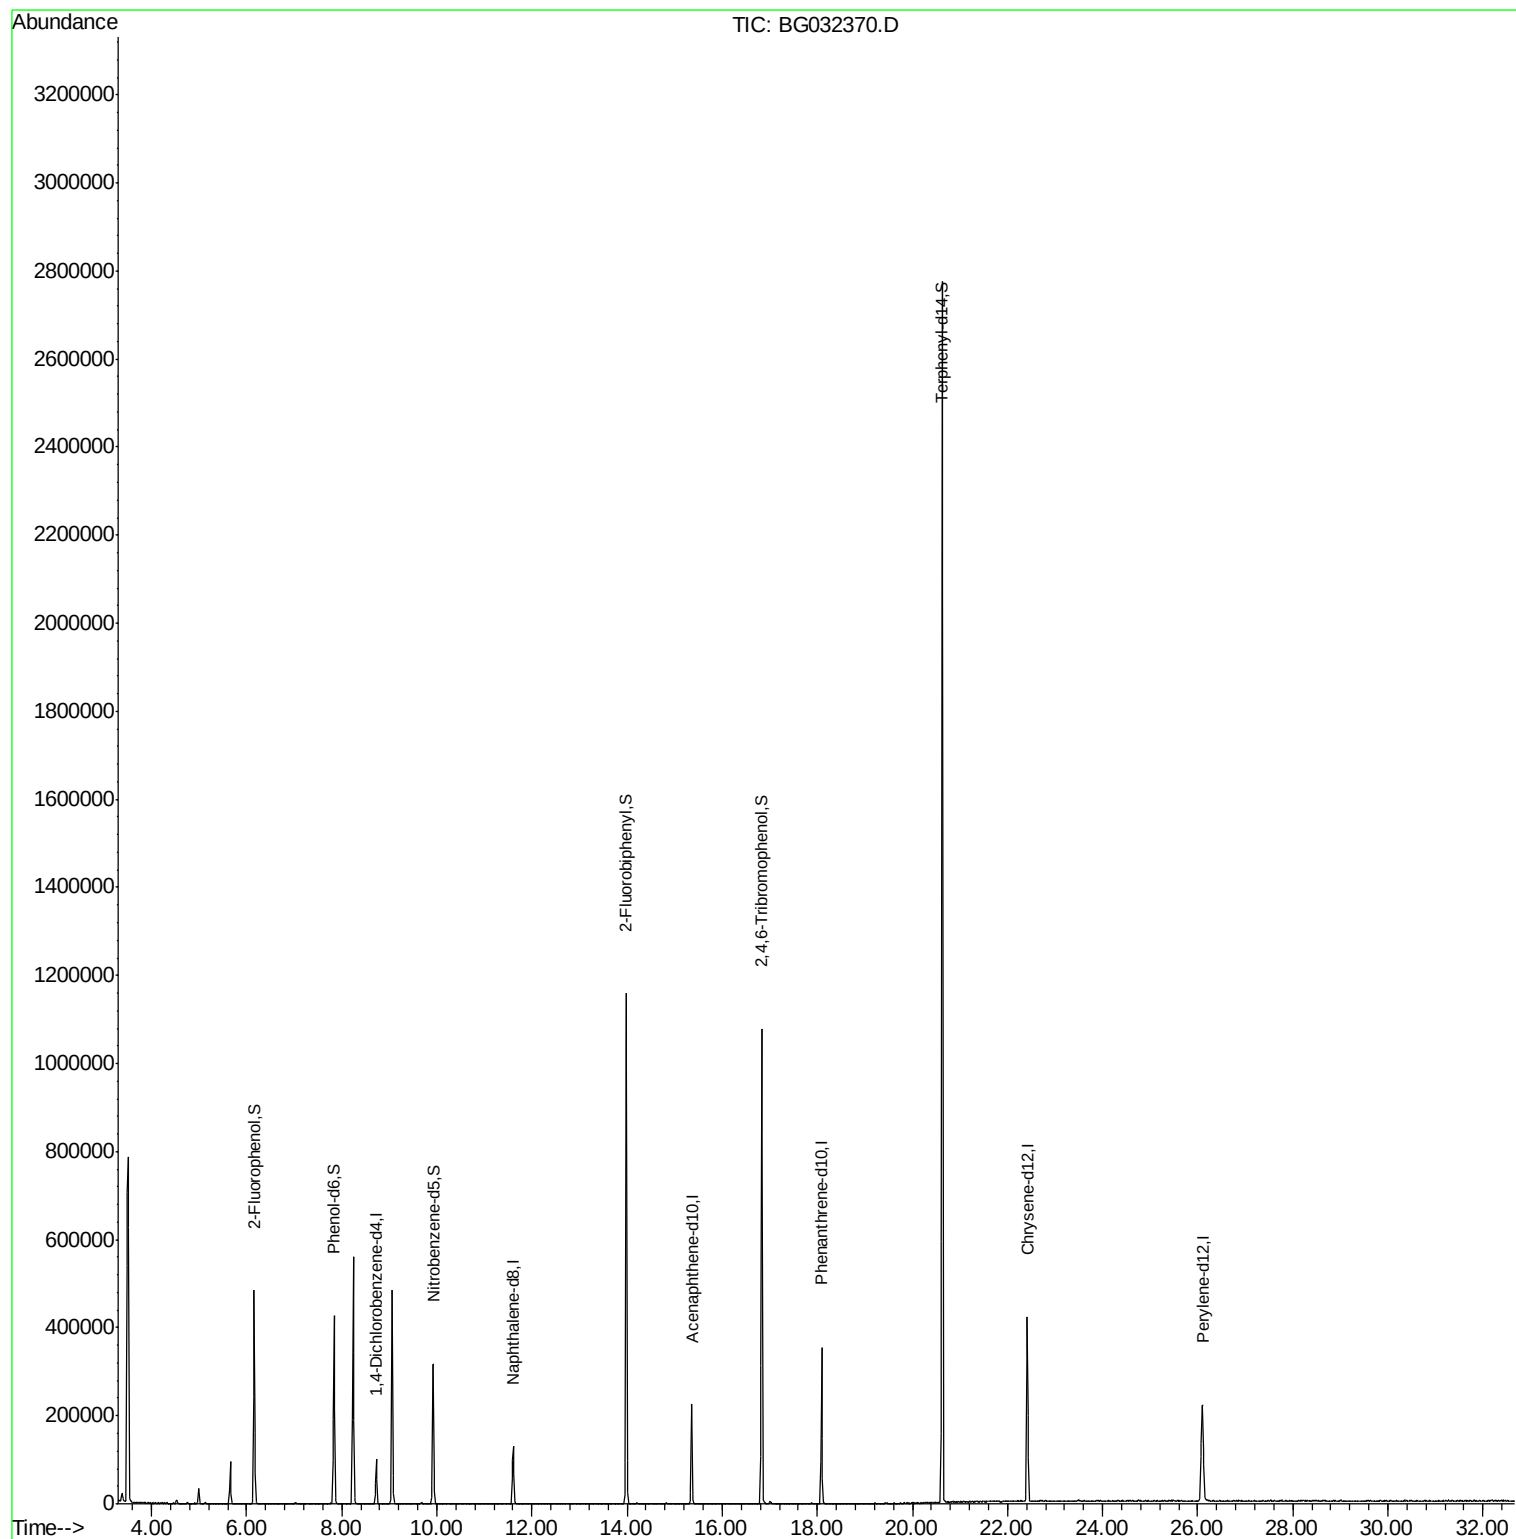

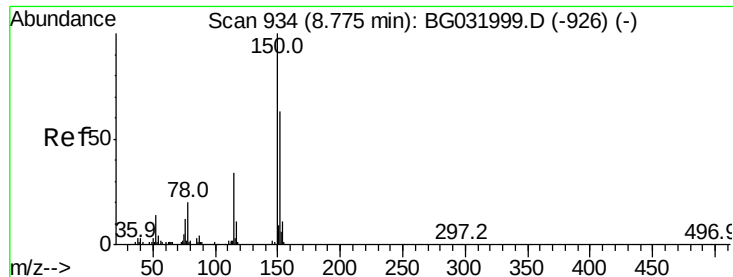

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.72 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG032370.D

Acq: 28 Jan 2018 00:36

Instrument :

BNA_G

ClientSampleId :

BU-01-012518


Tot Ion:152 Resp: 33818

Ion Ratio Lower Upper

152 100

150 146.6 126.6 189.8




115 50.5 53.0 79.4#

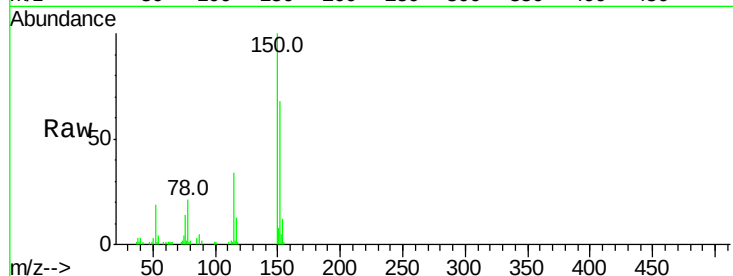

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

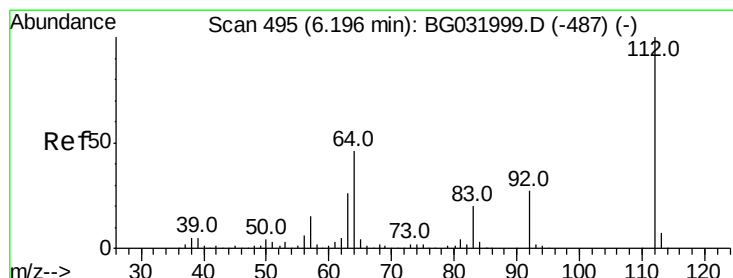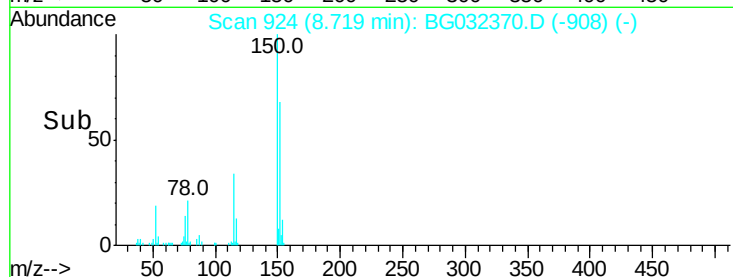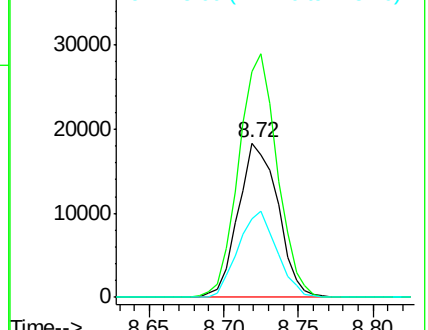

#5

2-Fluorophenol

Concen: 125.344 ng

RT: 6.16 min Scan# 488

Delta R.T. 0.00 min

Lab File: BG032370.D

Acq: 28 Jan 2018 00:36


Tgt Ion:112 Resp: 231768

Ion Ratio Lower Upper

112 100

64 53.8 56.3 84.5#



63 31.2 30.1 45.1

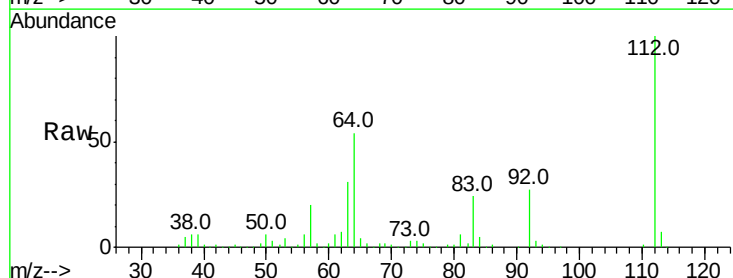


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

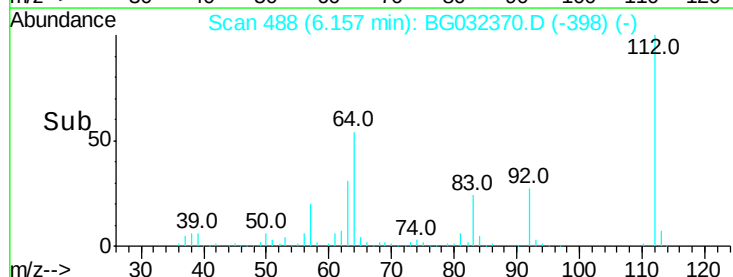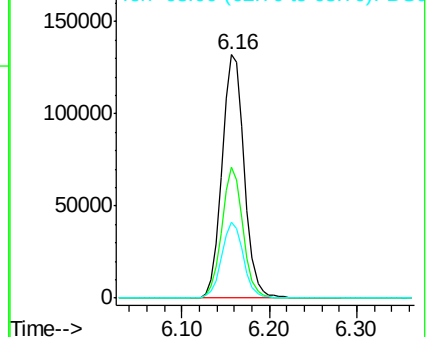

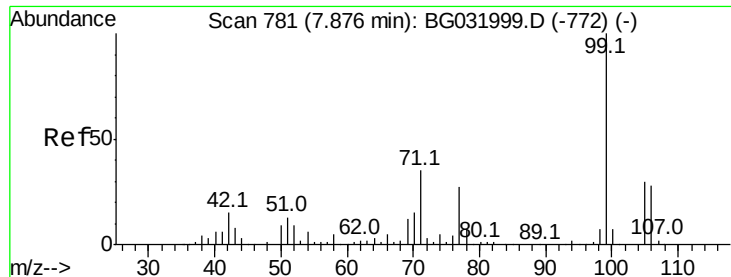

#7

Phenol-d6

Concen: 110.151 ng

RT: 7.84 min Scan# 774

Delta R.T. 0.00 min

Lab File: BG032370.D

Acq: 28 Jan 2018 00:36

Instrument :

BNA_G

ClientSampleId :

BU-01-012518


Tot Ion: 99 Resp: 256516

Ion Ratio Lower Upper




99 100

42 20.1 14.1 21.1

71 45.1 26.1 39.1#

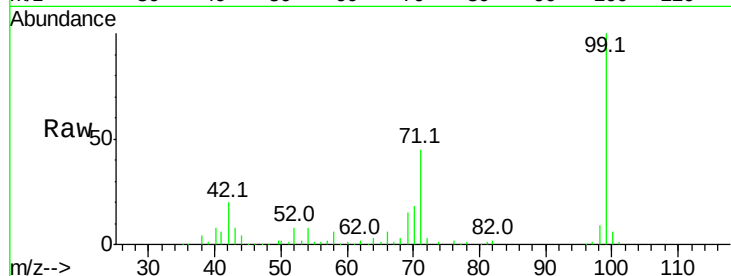

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

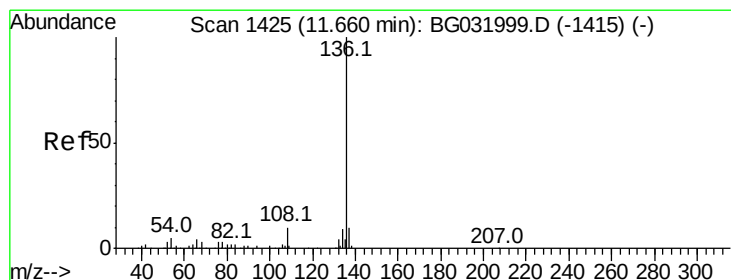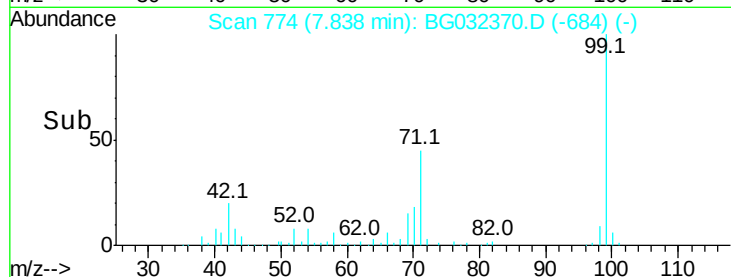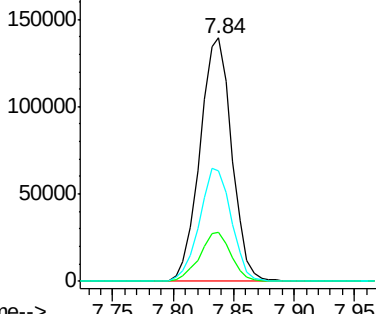

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.60 min Scan# 1415

Delta R.T. -0.00 min

Lab File: BG032370.D

Acq: 28 Jan 2018 00:36

Tgt Ion: 136 Resp: 127512


Ion Ratio Lower Upper

136 100



137 9.7 9.2 13.8


54 4.9 10.3 15.5#

68 2.7 4.5 6.7#

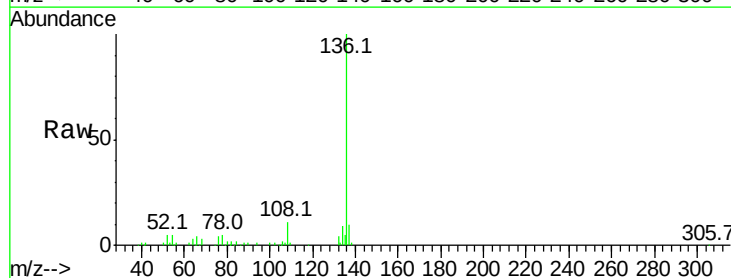

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

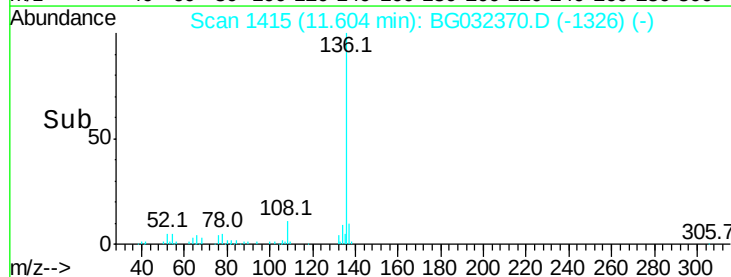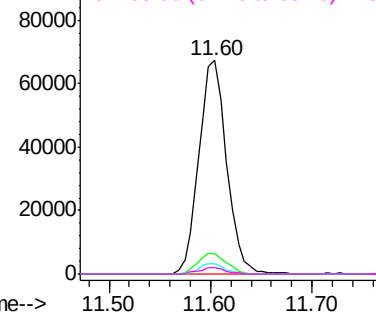


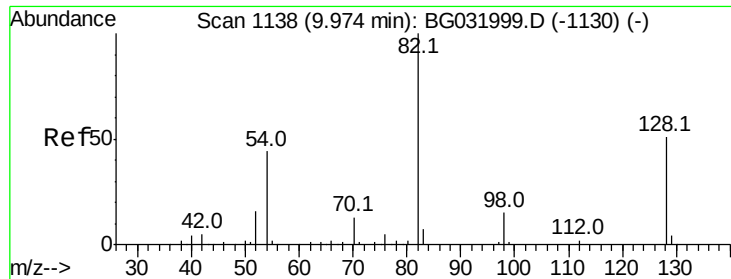




#23
 Nitrobenzene-d5
 Concen: 105.135 ng
 RT: 9.92 min Scan# 1129
 Delta R.T. 0.00 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36

Instrument :
 BNA_G
 ClientSampleId :
 BU-01-012518

Tot Ion: 82 Resp: 198154
 Ion Ratio Lower Upper
 82 100
 128 47.6 29.7 44.5#
 54 49.8 43.1 64.7

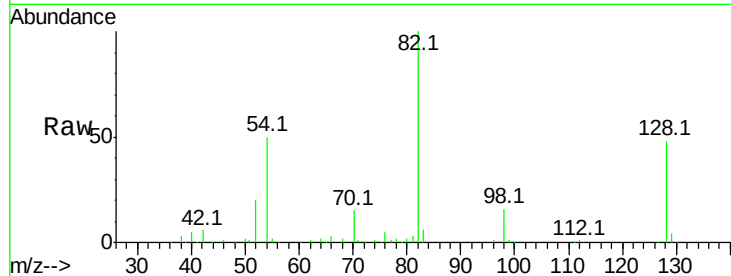


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

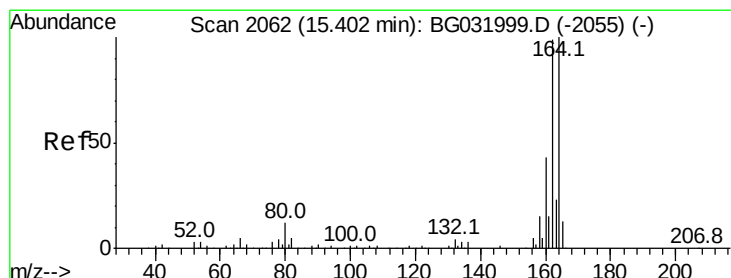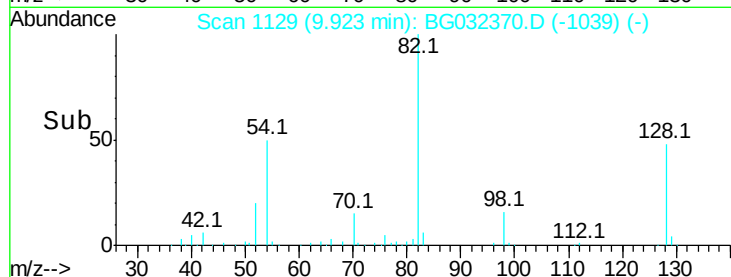
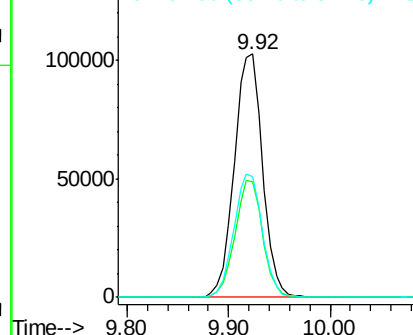



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.36 min Scan# 2054
 Delta R.T. -0.00 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36

Tgt Ion:164 Resp: 86402
 Ion Ratio Lower Upper
 164 100
 162 107.8 78.8 118.2
 160 47.0 35.4 53.0

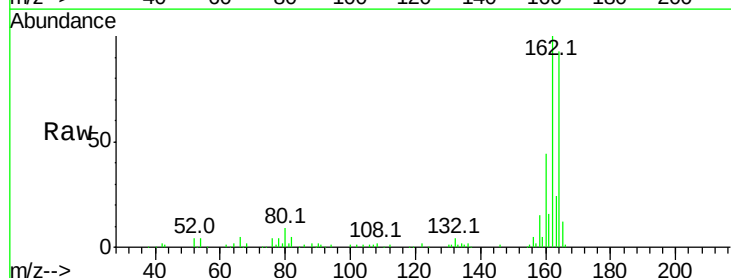

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



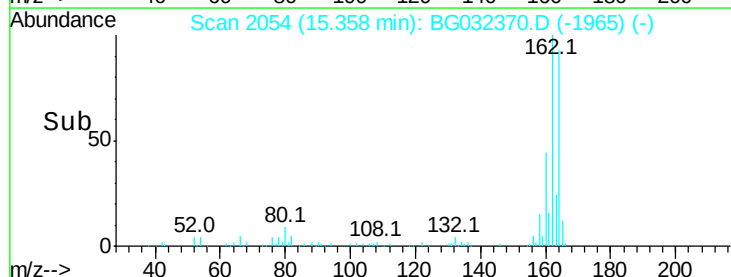
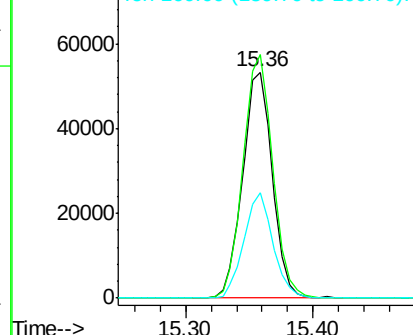


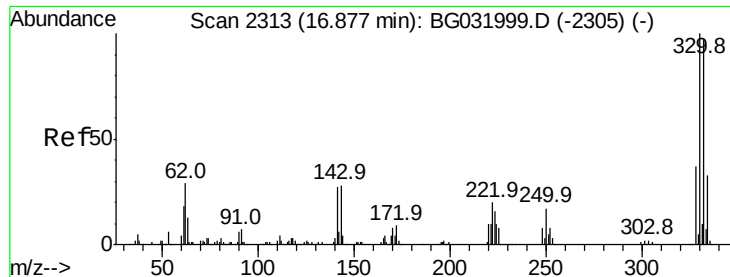

#41
 2,4,6-Tribromophenol
 Concen: 166.014 ng
 RT: 16.83 min Scan# 2305
 Delta R.T. -0.00 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36




Instrument :
 BNA_G
 ClientSampleId :
 BU-01-012518


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	77.0	115.6
141	29.3	25.2	37.8

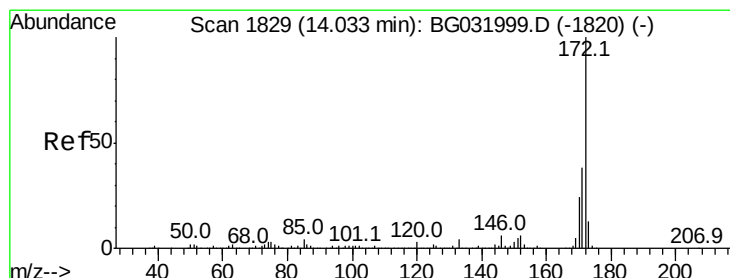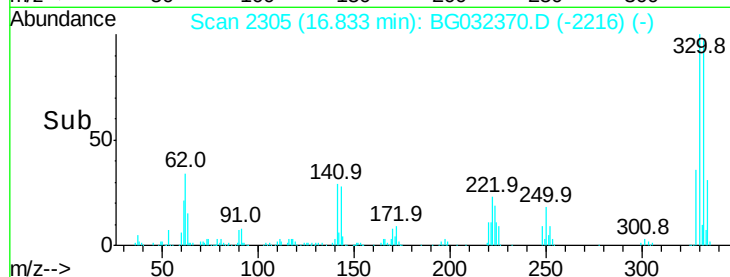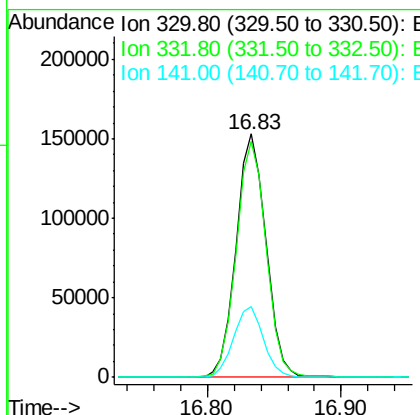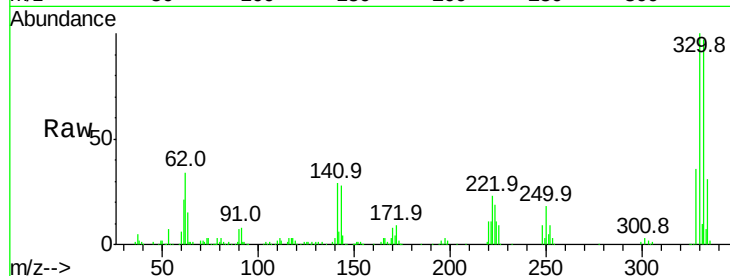

#44
 2-Fluorobiphenyl
 Concen: 96.545 ng
 RT: 13.98 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	30.0	45.0
170	23.0	19.5	29.3

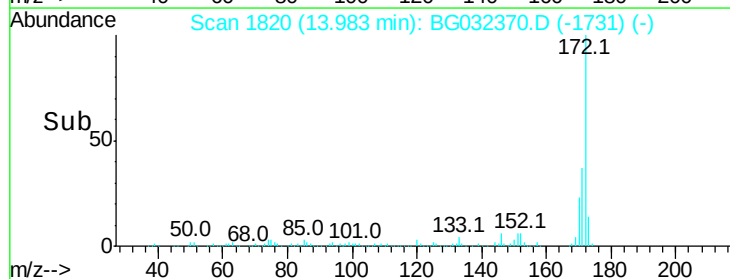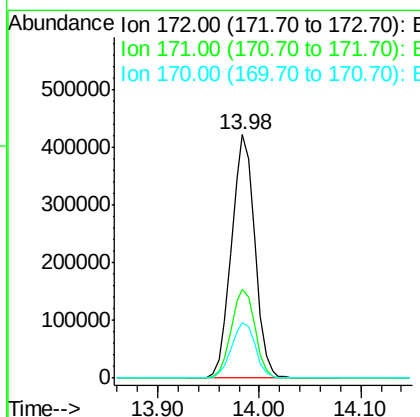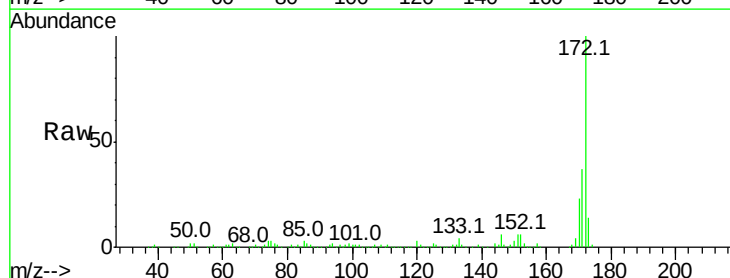


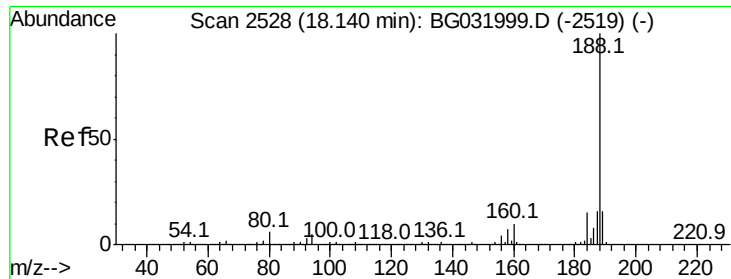




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.09 min Scan# 2519
Delta R.T. -0.00 min
Lab File: BG032370.D
Acq: 28 Jan 2018 00:36

Instrument :
BNA_G
ClientSampleId :
BU-01-012518

Tot Ion:188 Resp: 236773
Ion Ratio Lower Upper
188 100
94 3.5 6.9 10.3#
80 3.7 7.7 11.5#

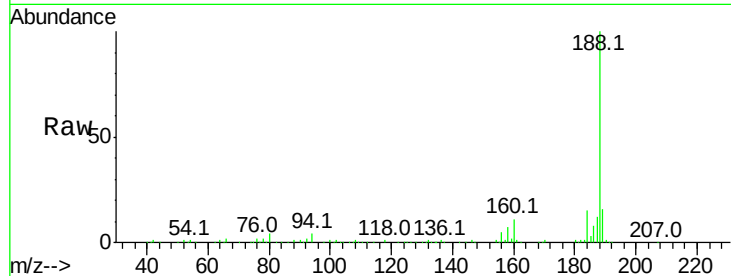


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

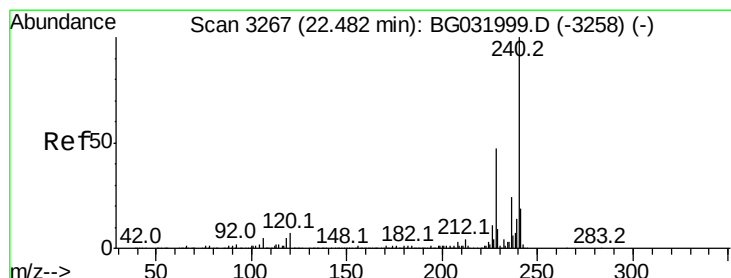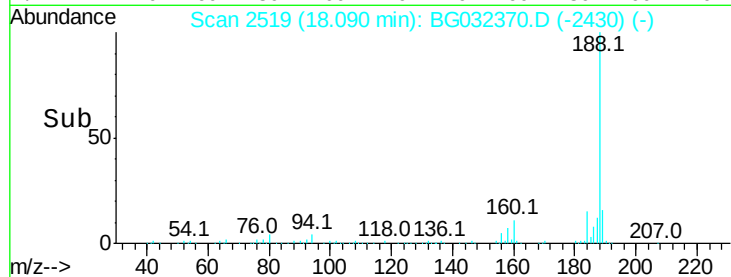
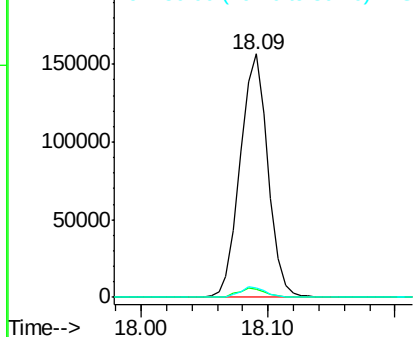



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.41 min Scan# 3255
Delta R.T. -0.01 min
Lab File: BG032370.D
Acq: 28 Jan 2018 00:36

Tgt Ion:240 Resp: 321245
Ion Ratio Lower Upper
240 100
120 3.5 6.8 10.2#
236 25.2 20.9 31.3

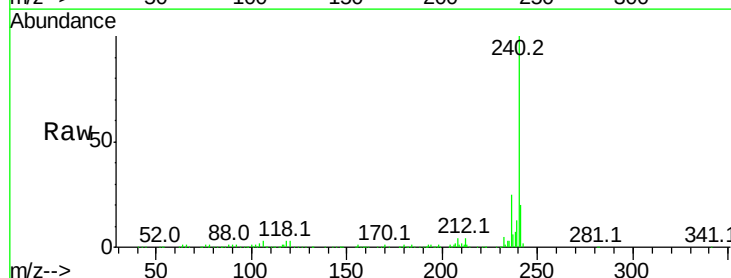

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

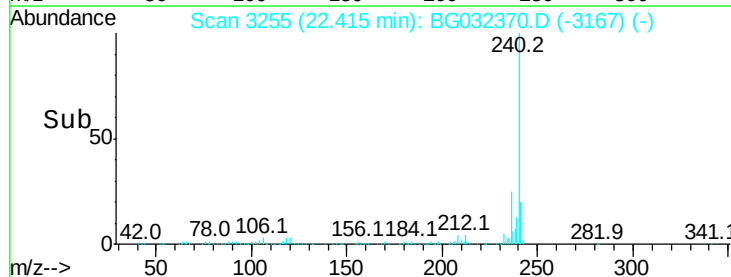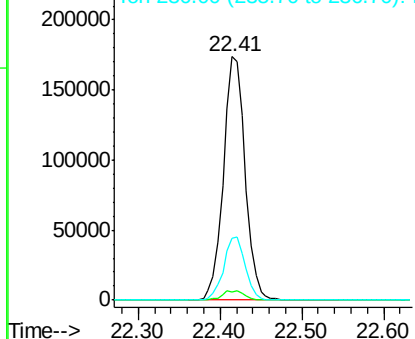


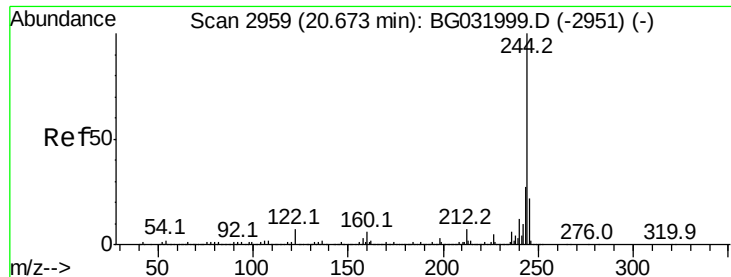




#78
 Terphenyl-d14
 Concen: 102.829 ng
 RT: 20.63 min Scan# 2951
 Delta R.T. -0.00 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36

Instrument :
 BNA_G
 ClientSampleId :
 BU-01-012518

Tot Ion:244 Resp: 1496040
 Ion Ratio Lower Upper
 244 100
 212 7.7 5.8 8.8
 122 5.4 7.0 10.4#

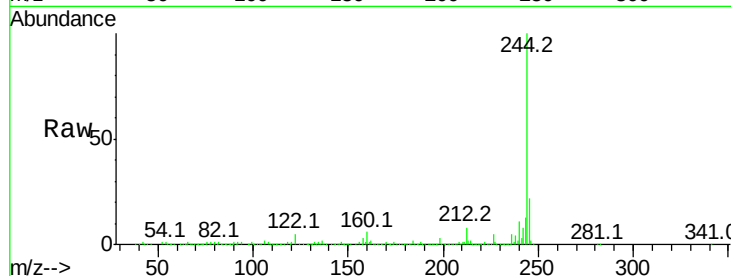


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

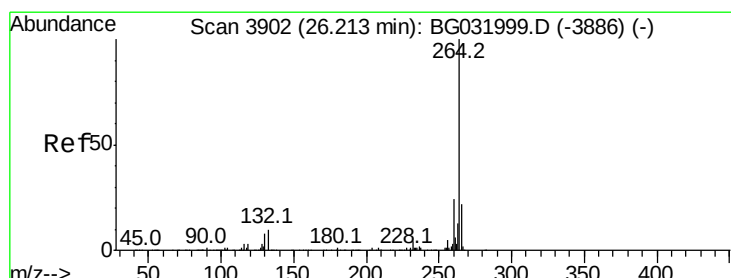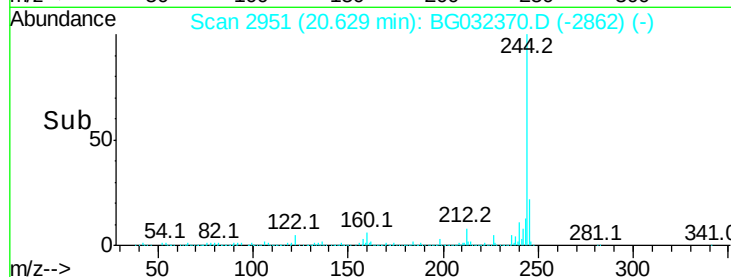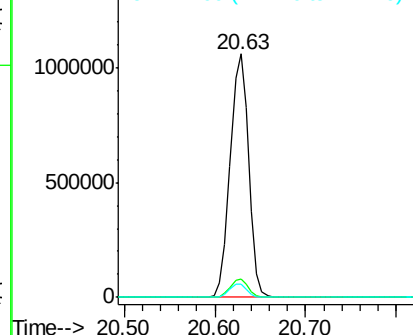

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 26.10 min Scan# 3882
 Delta R.T. -0.01 min
 Lab File: BG032370.D
 Acq: 28 Jan 2018 00:36

Tgt Ion:264 Resp: 293134
 Ion Ratio Lower Upper
 264 100
 260 25.3 17.4 26.0
 265 21.5 17.7 26.5

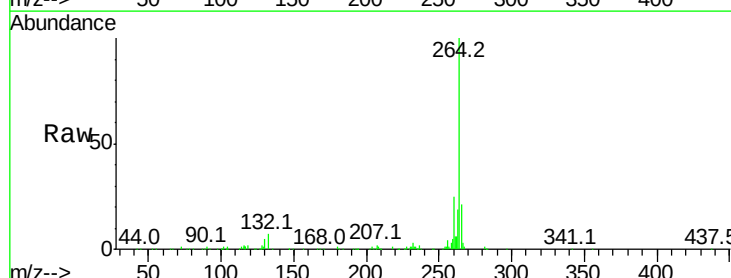

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

