


Data Path : U:\HPCHEM1\BNA G\Data\BG012718\
 Data File : BG032346.D
 Acq On : 27 Jan 2018 8:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

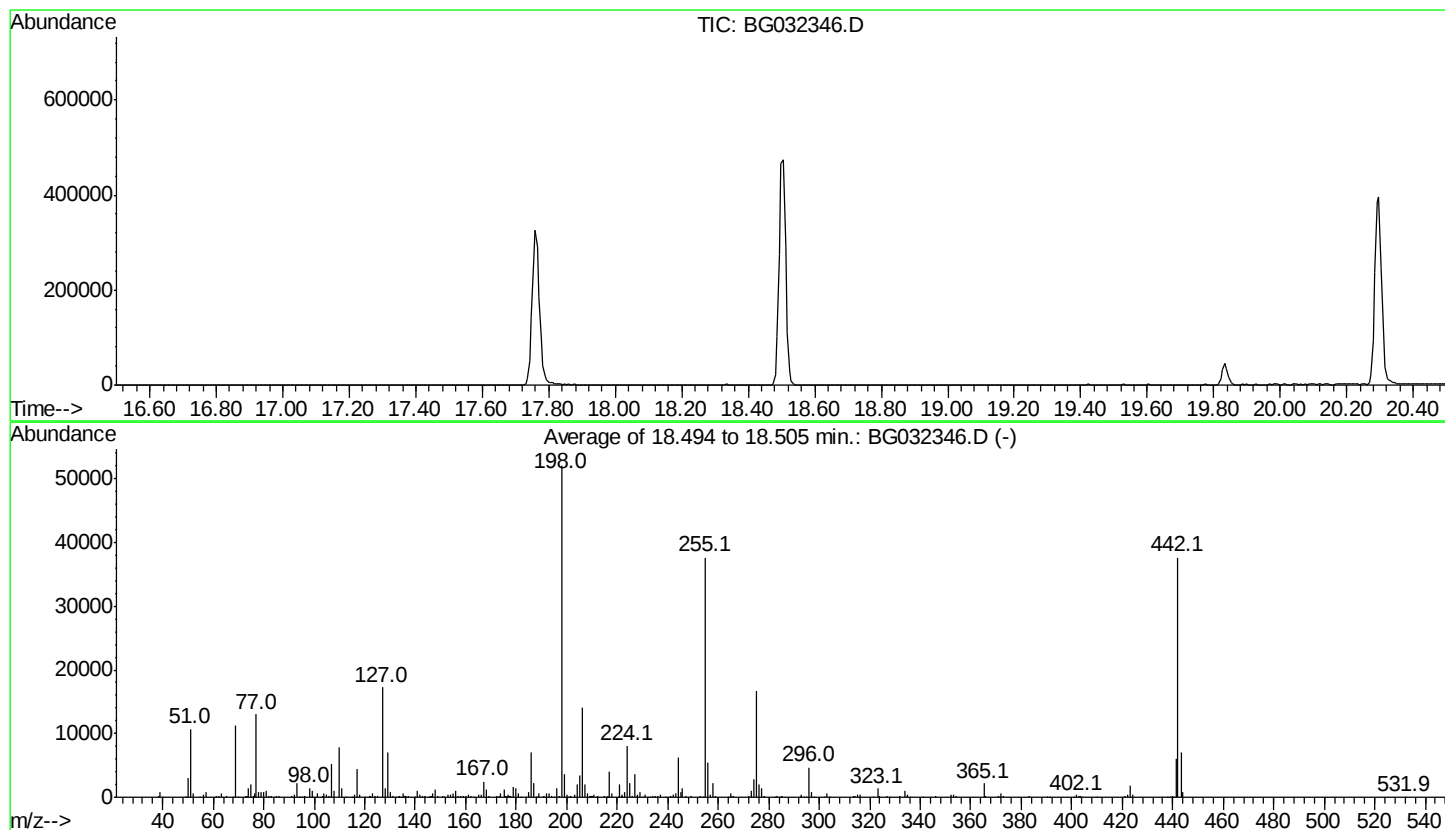

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.6	10721	PASS
68	69	0.00	2	0.9	106	PASS
69	198	0.00	100	21.7	11283	PASS
70	69	0.00	2	0.5	51	PASS
127	198	10	80	33.1	17208	PASS
197	198	0.00	2	0.4	207	PASS
198	198	100	100	100.0	52064	PASS
199	198	5	9	7.0	3659	PASS
275	198	10	60	32.1	16723	PASS
365	198	1	100	4.1	2137	PASS
441	442	0.01	24	15.9	5964	PASS
442	198	50	100	72.2	37592	PASS
443	442	15	24	18.7	7047	PASS