
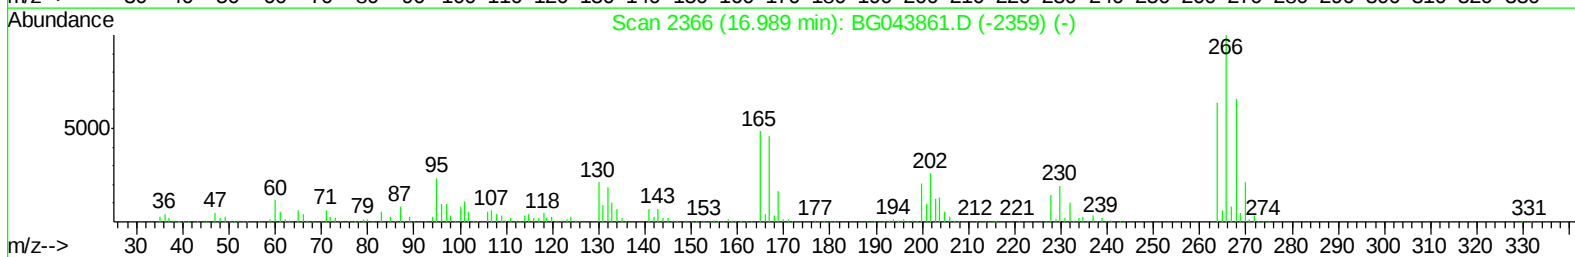
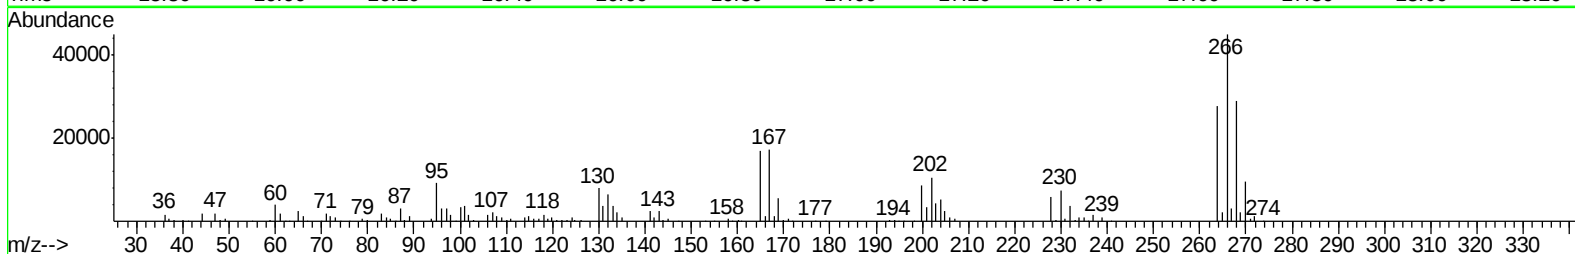


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012720\
Data File : BG044211.D
Acq On : 27 Jan 2020 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 00:37:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

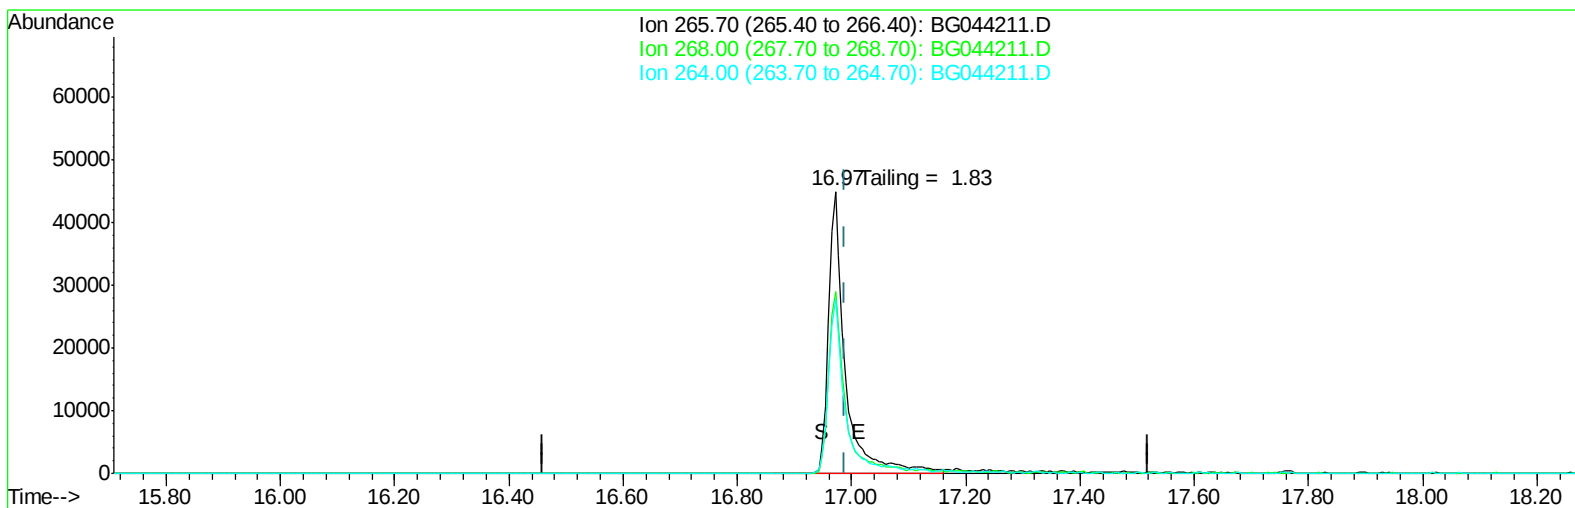

TIC: BG044211.D

(70) Pentachlorophenol (C)




16.971min (-0.018) 21452.99ng

response 85131

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	64.72
264.00	63.50	62.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012720\
Data File : BG044211.D
Acq On : 27 Jan 2020 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 00:37:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

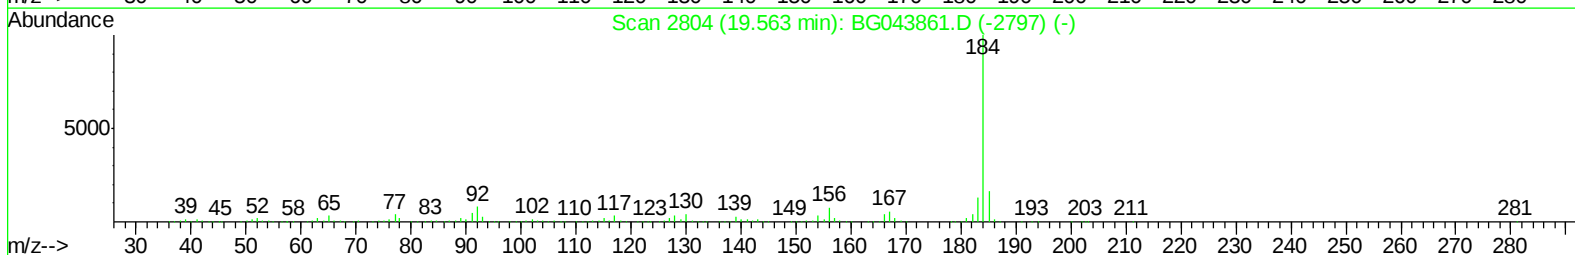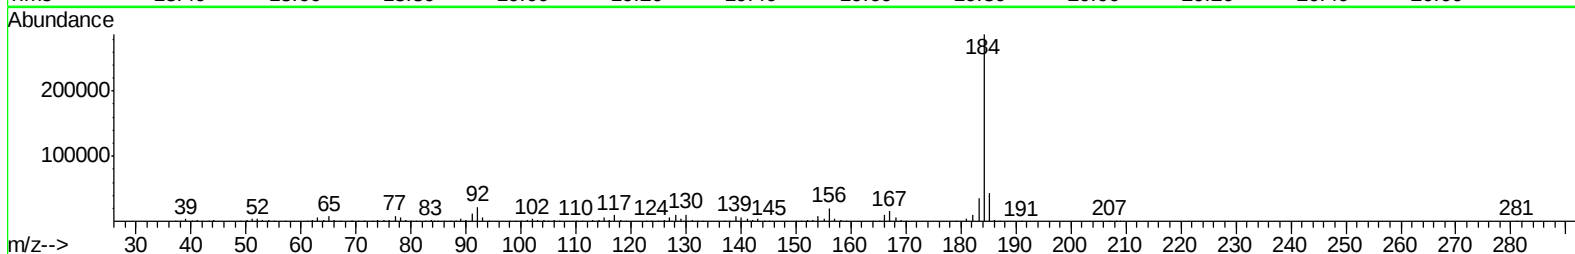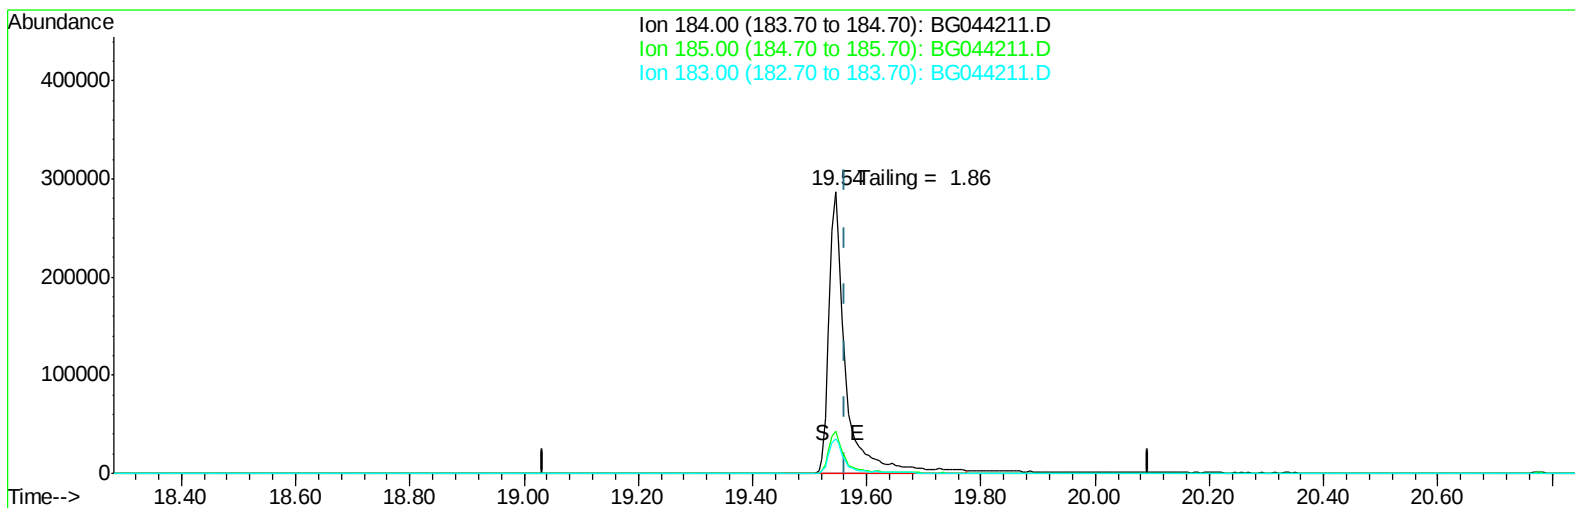

TIC: BG044211.D

(77) Benzidine

19.545min (-0.018) 0.00ng

response 570128

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.10
183.00	13.20	12.49
0.00	0.00	0.00