


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012720\
 Data File : BG044211.D
 Acq On : 27 Jan 2020 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

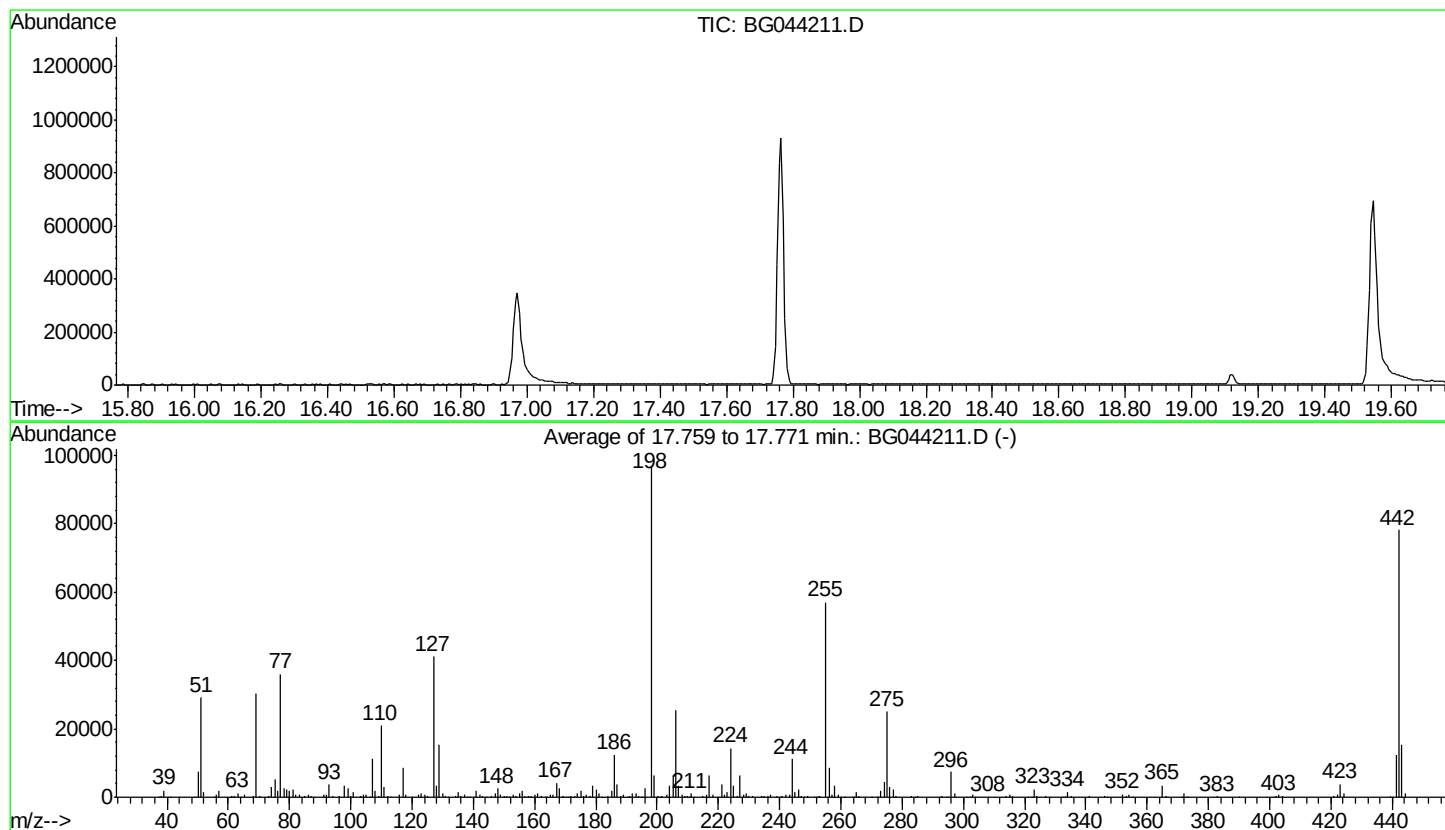

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	29152	PASS
68	69	0.00	2	0.8	250	PASS
69	198	0.00	100	31.1	30160	PASS
70	69	0.00	2	0.7	209	PASS
127	198	10	80	42.4	41085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96946	PASS
199	198	5	9	6.6	6395	PASS
275	198	10	60	25.8	25016	PASS
365	198	1	100	3.5	3419	PASS
441	198	0.01	100	12.9	12541	PASS
442	198	50	100	80.6	78144	PASS
443	442	15	24	19.7	15366	PASS