
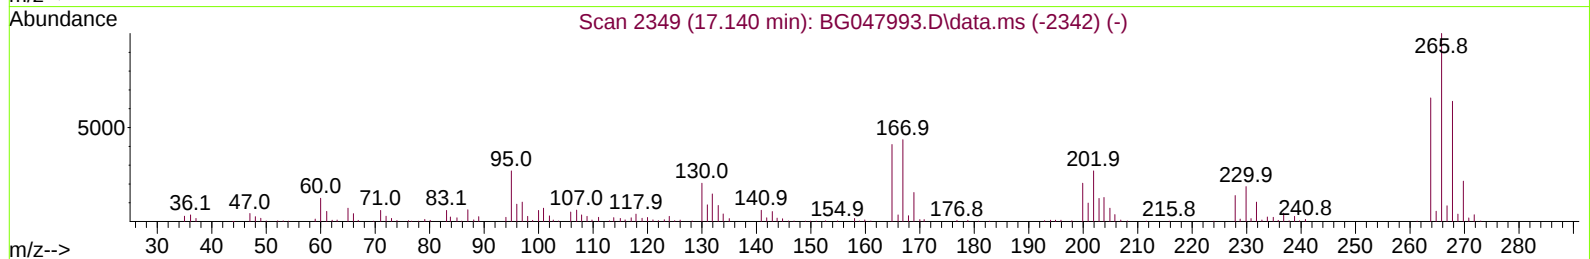
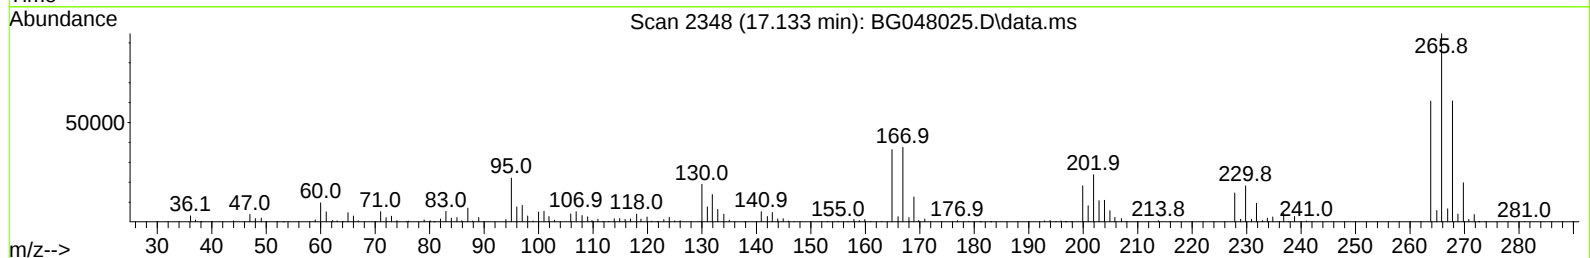


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
Data File : BG048025.D
Acq On : 27 Jan 2021 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:56:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

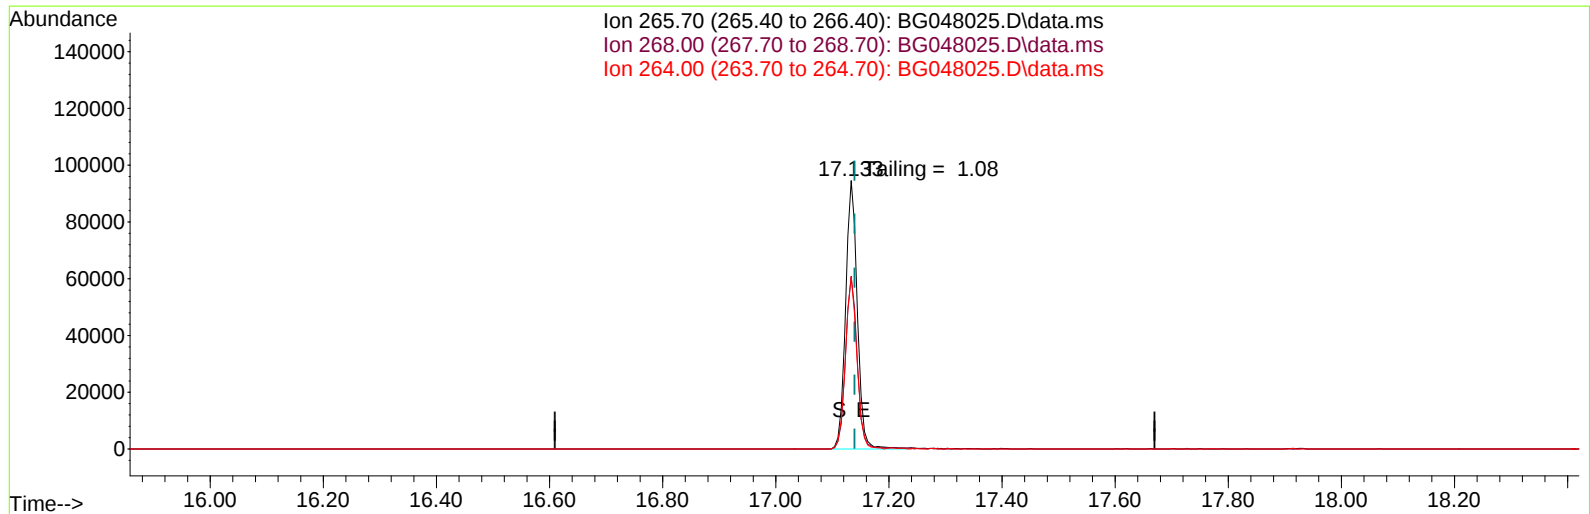

TIC: BG048025.D\data.ms

(70) Pentachlorophenol (C)




17.133min (-0.006) 274937.11 ng

response 135855

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.29
264.00	61.60	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
Data File : BG048025.D
Acq On : 27 Jan 2021 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:56:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

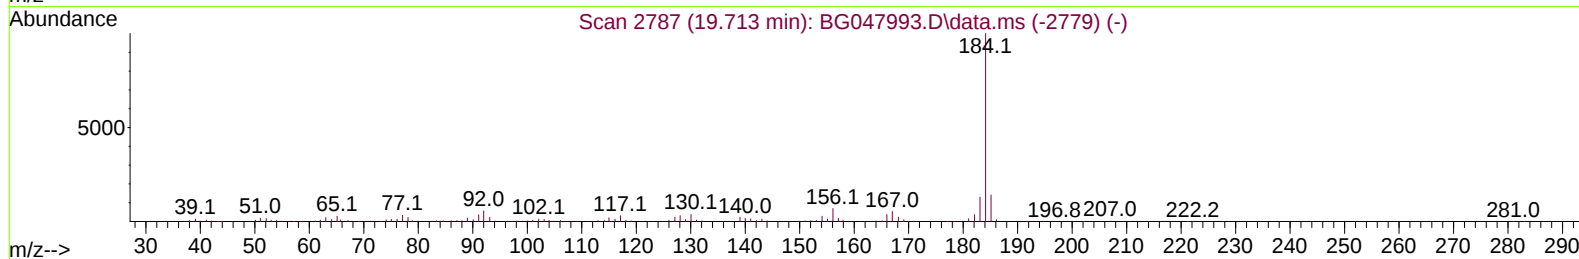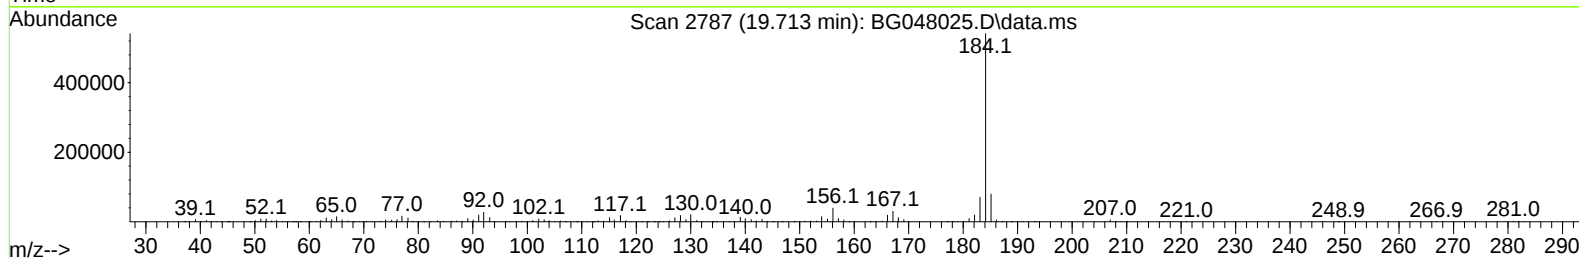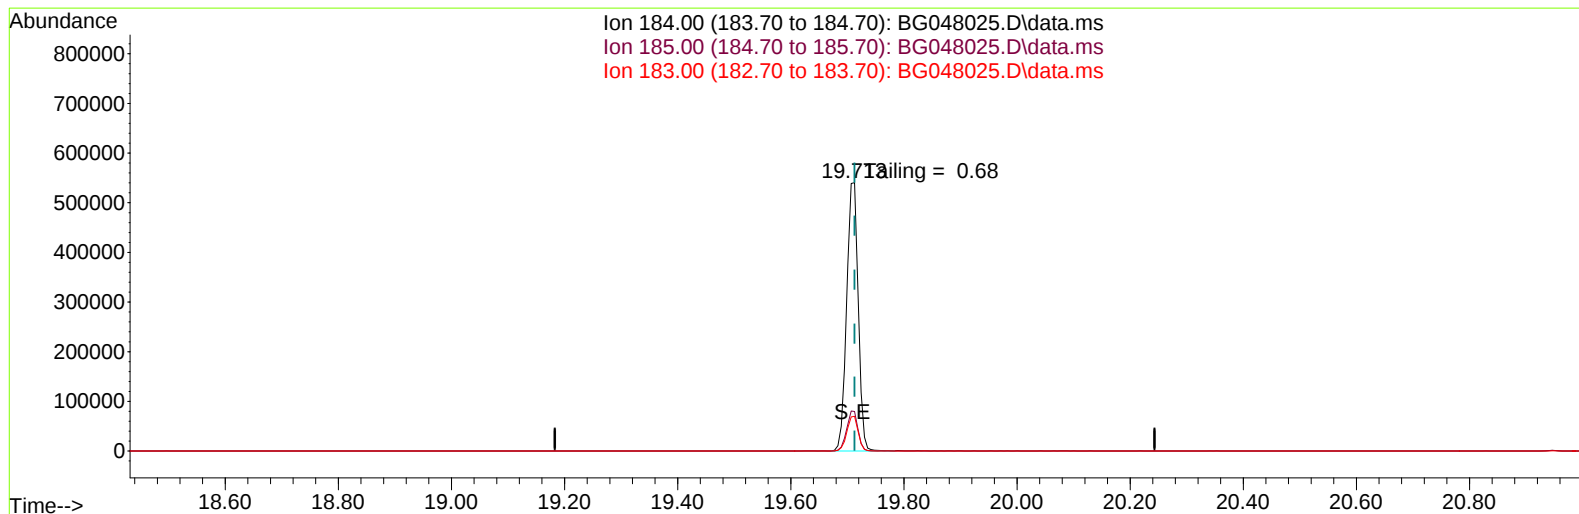

TIC: BG048025.D\data.ms

(77) Benzidine**19.713min (-0.000) 5581.23 ng****response 769131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.75
183.00	13.20	12.94
0.00	0.00	0.00