
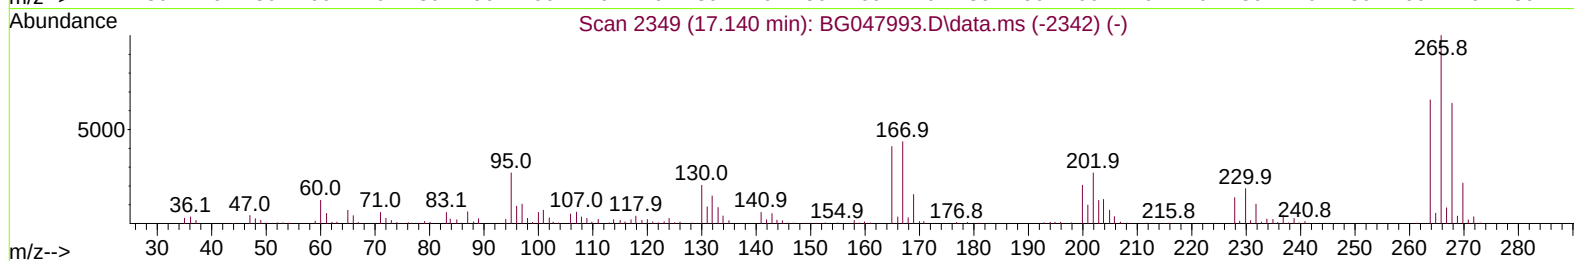
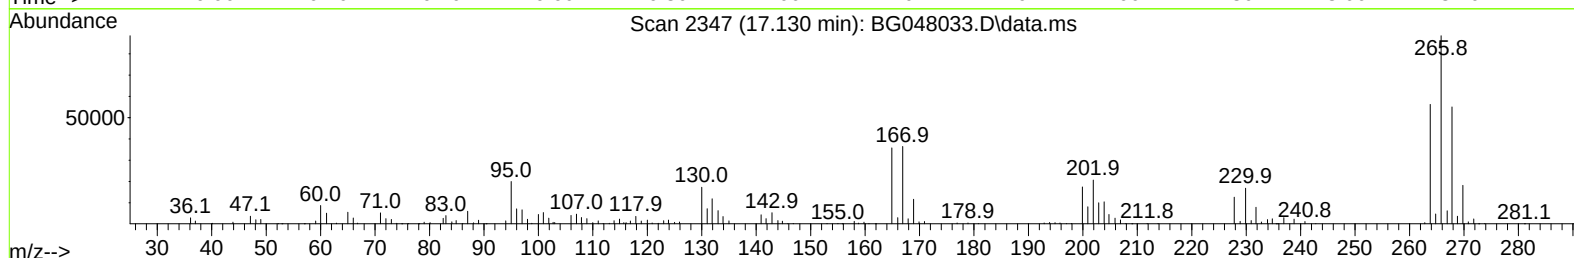


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
Data File : BG048033.D
Acq On : 27 Jan 2021 18:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:02:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration

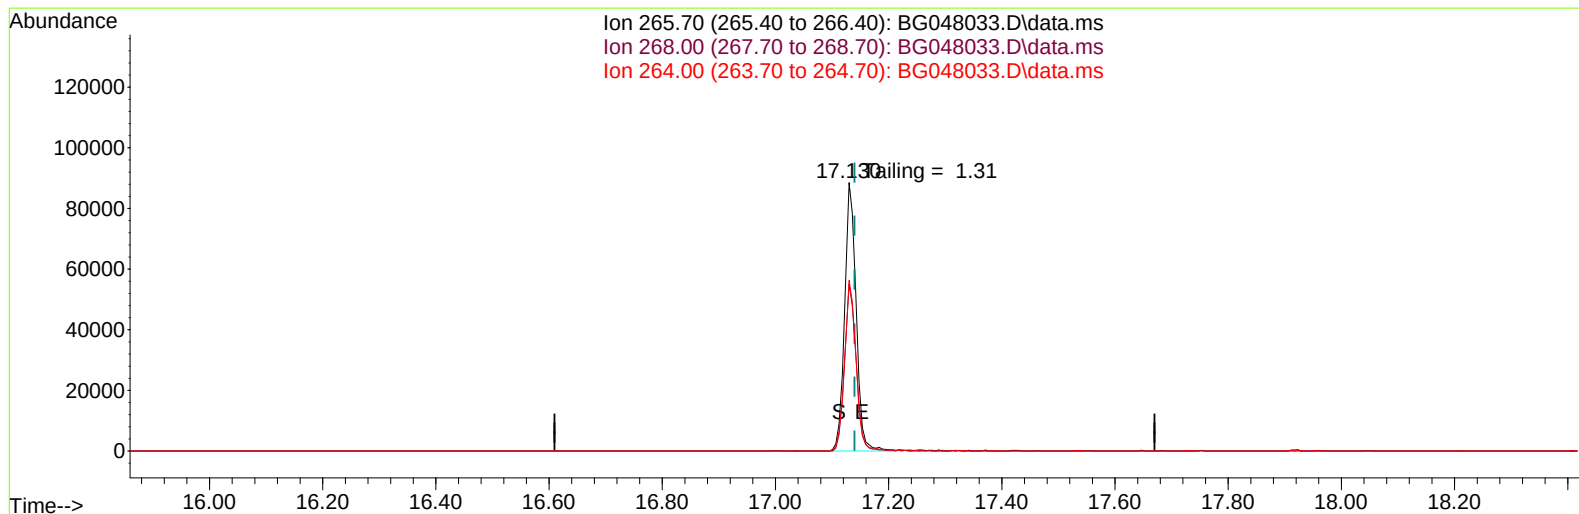

TIC: BG048033.D\data.ms

(70) Pentachlorophenol (C)




17.130min (-0.010) 29443.29 ng

response 125224

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
 Data File : BG048033.D
 Acq On : 27 Jan 2021 18:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:02:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 25 19:39:42 2021
 Response via : Initial Calibration

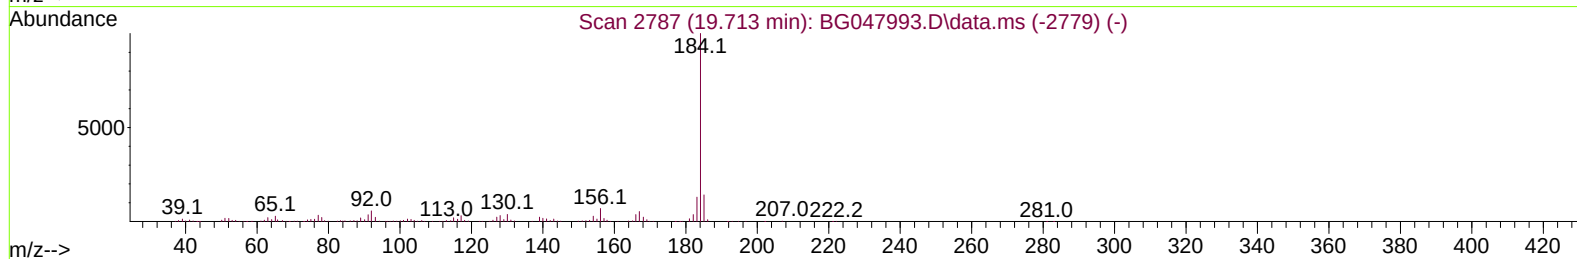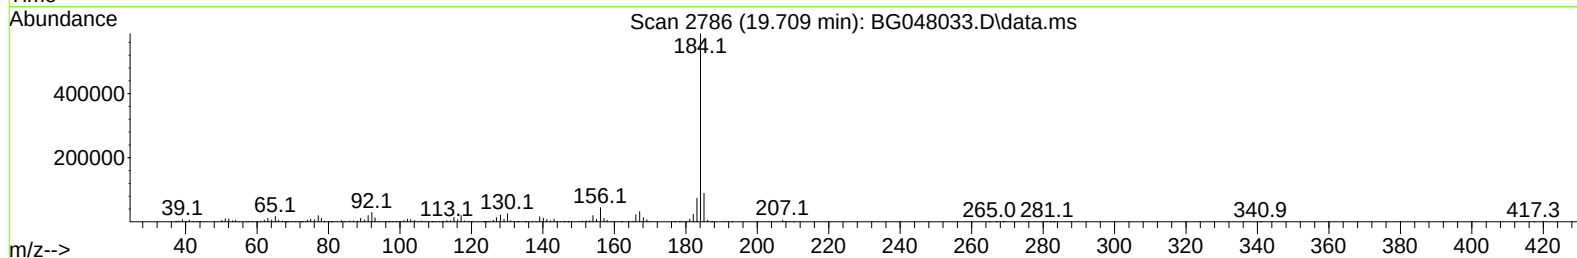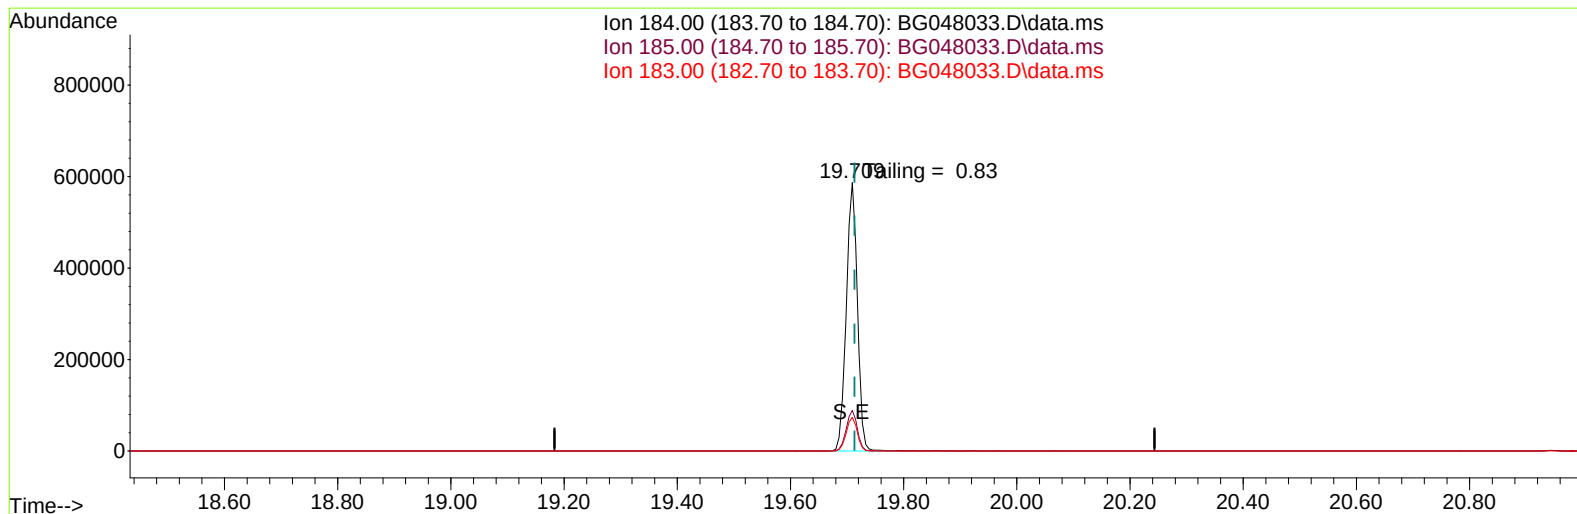

TIC: BG048033.D\data.ms

(77) Benzidine**19.709min (-0.004) 477457.61 ng****response 798874**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.18
183.00	13.20	12.53
0.00	0.00	0.00