

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
 Data File : BG048039.D
 Acq On : 27 Jan 2021 22:18
 Operator : CG/JU
 Sample : M1212-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0021-SITE-WATER-042

Quant Time: Jan 27 23:31:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 25 19:39:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.125	152	48454	20.00	ng	# 0.00
21) Naphthalene-d8	10.940	136	187097	20.00	ng	0.00
39) Acenaphthene-d10	14.747	164	135935	20.00	ng	0.00
64) Phenanthrene-d10	17.485	188	330504	20.00	ng	-0.01
76) Chrysene-d12	21.762	240	357584	20.00	ng	#-0.01
86) Perylene-d12	25.047	264	354355	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.681	112	191373	60.70	ng	0.00
7) Phenol-d6	7.268	99	180537	37.66	ng	-0.01
23) Nitrobenzene-d5	9.289	82	375708	79.46	ng	0.00
42) 2,4,6-Tribromophenol	16.228	330	291209	128.62	ng	-0.01
45) 2-Fluorobiphenyl	13.372	172	820336	78.02	ng	-0.01
79) Terphenyl-d14	20.094	244	1375364	66.69	ng	0.00
Target Compounds						
10) Phenol	7.297	94	27129	5.90	ng	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
Data File : BG048039.D
Acq On : 27 Jan 2021 22:18
Operator : CG/JU
Sample : M1212-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042

Quant Time: Jan 27 23:31:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration




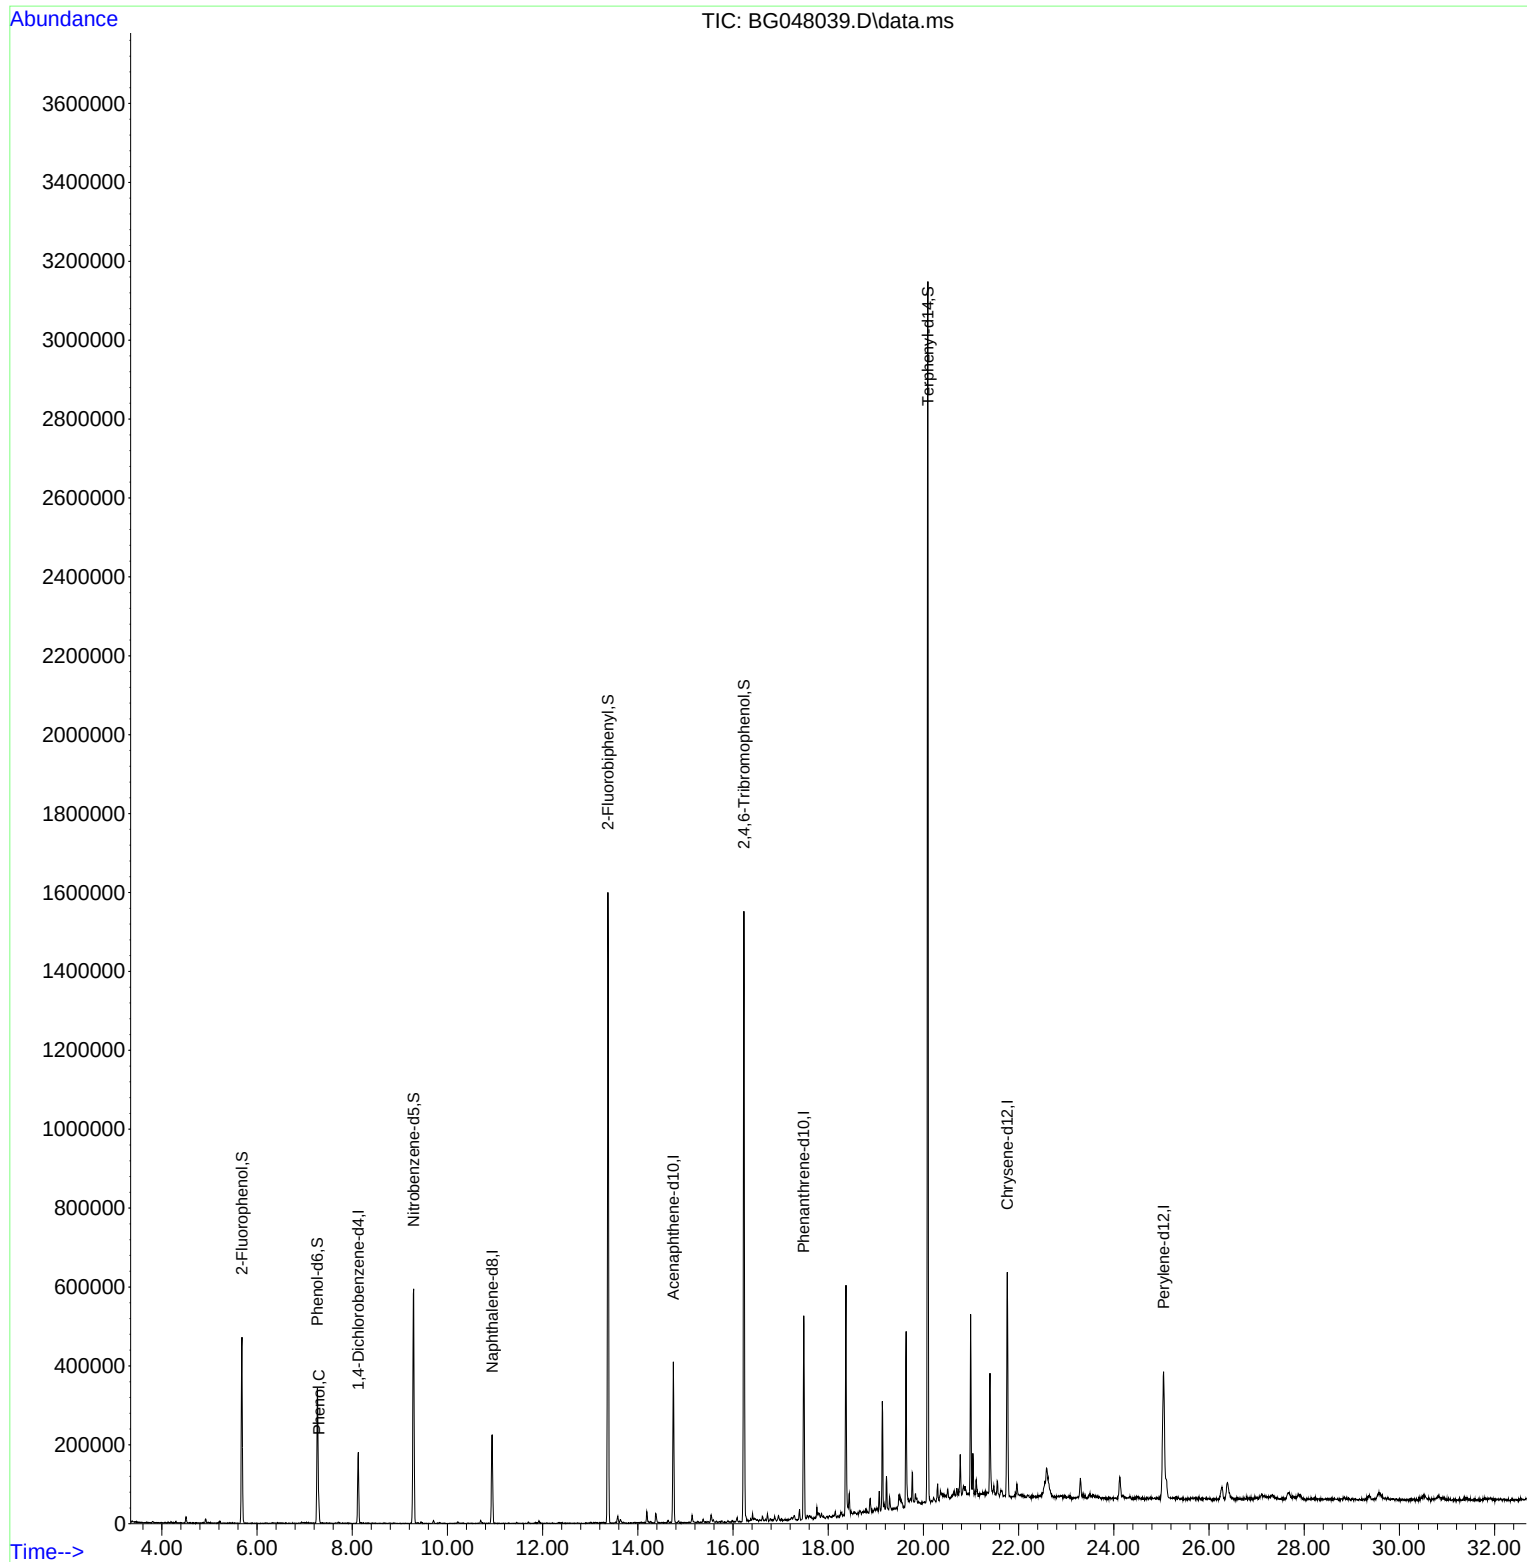




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.125 min Scan# 815
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18




Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042


Tgt Ion:152 Resp: 48454
Ion Ratio Lower Upper
152 100
150 156.8 125.0 187.6
115 63.4 41.8 62.6#

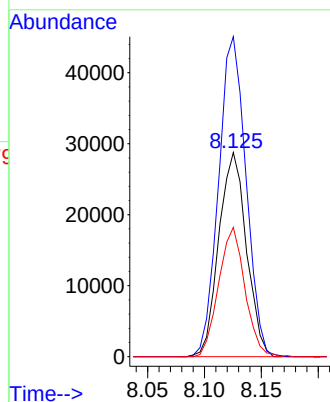

#5
2-Fluorophenol
Concen: 60.70 ng
RT: 5.681 min Scan# 399
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Tgt Ion:112 Resp: 191373
Ion Ratio Lower Upper
112 100
64 66.0 46.7 70.1
63 37.4 22.8 34.2#


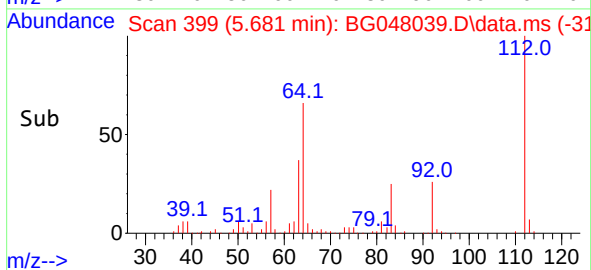
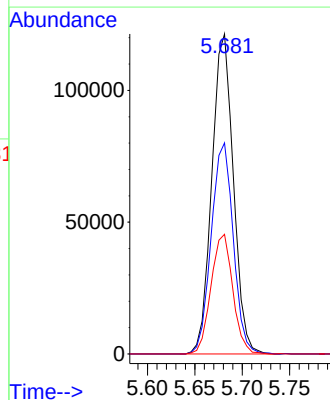





#7
Phenol-d6
Concen: 37.66 ng
RT: 7.268 min Scan# 669
Delta R.T. -0.013 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18




Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042


Tgt Ion: 99 Resp: 180537
Ion Ratio Lower Upper
99 100
42 20.4 12.8 19.2#
71 46.3 24.6 36.8#

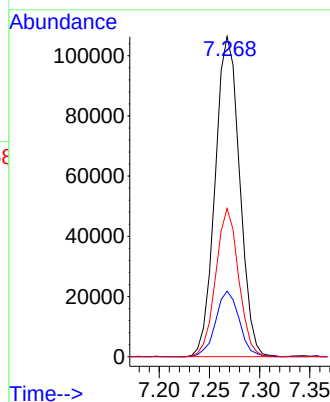

#10
Phenol
Concen: 5.90 ng
RT: 7.297 min Scan# 674
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18


Tgt Ion: 94 Resp: 27129
Ion Ratio Lower Upper
94 100
65 28.2 6.6 46.6
66 44.6 13.9 53.9

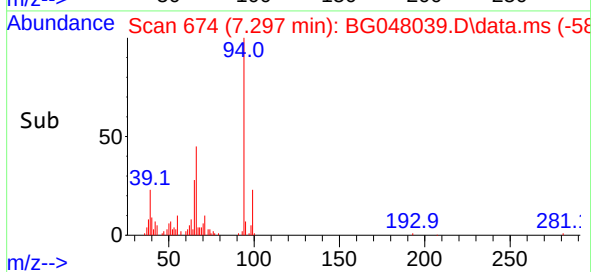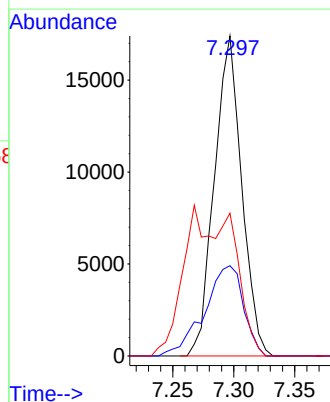






#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.940 min Scan# 1294
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042



Tgt Ion:136 Resp: 187097




Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.1	13.7
54	8.4	6.2	9.4
68	6.6	5.0	7.4

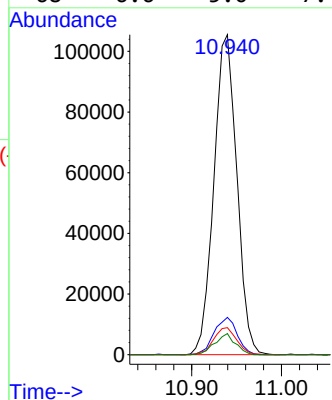


#23
Nitrobenzene-d5
Concen: 79.46 ng
RT: 9.289 min Scan# 1013
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Tgt Ion: 82 Resp: 375708


Ion	Ratio	Lower	Upper
82	100		
128	36.8	37.0	55.6#
54	47.7	39.0	58.4

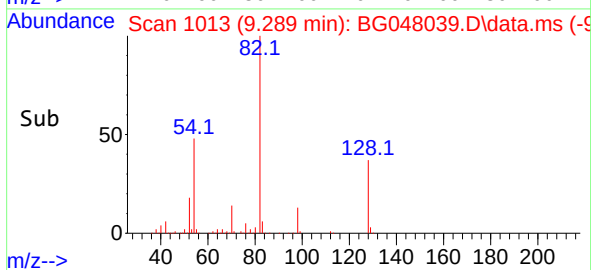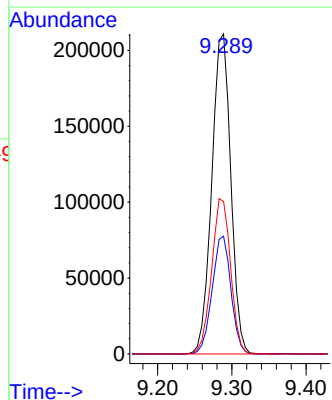






#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.747 min Scan# 1942
Delta R.T. -0.007 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042



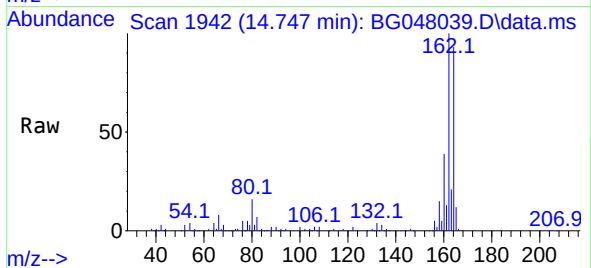



Tgt Ion:164 Resp: 135935
Ion Ratio Lower Upper
164 100
162 107.8 82.3 123.5
160 41.8 35.3 52.9

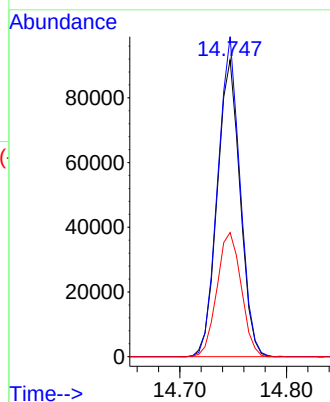

#42
2,4,6-Tribromophenol
Concen: 128.62 ng
RT: 16.228 min Scan# 2194
Delta R.T. -0.013 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Tgt Ion:330 Resp: 291209
Ion Ratio Lower Upper
330 100
332 95.6 76.5 114.7
141 33.4 26.0 39.0

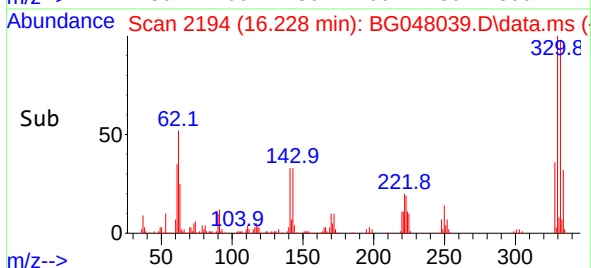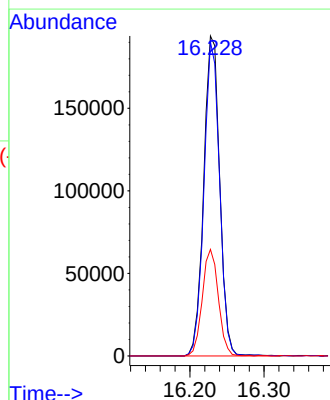







#45
2-Fluorobiphenyl
Concen: 78.02 ng
RT: 13.372 min Scan# 1708
Delta R.T. -0.013 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042

Tgt Ion:172 Resp: 820336




Ion	Ratio	Lower	Upper
172	100		
171	35.4	31.3	46.9
170	24.2	20.8	31.2

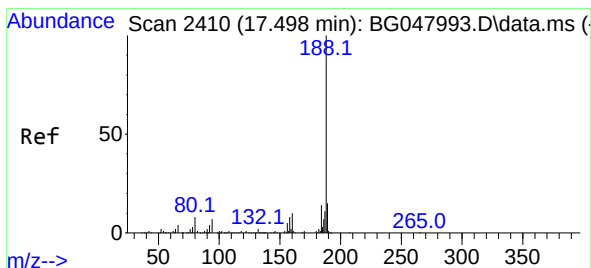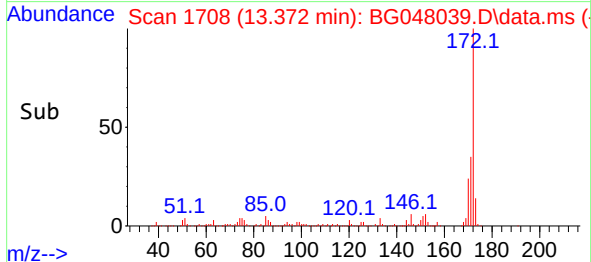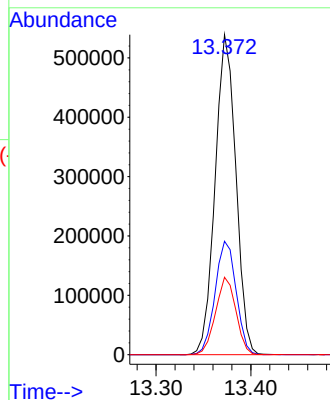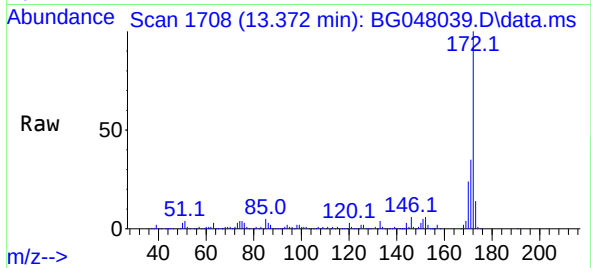


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.485 min Scan# 2408
Delta R.T. -0.013 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Tgt Ion:188 Resp: 330504

Ion	Ratio	Lower	Upper
188	100		
94	7.1	6.3	9.5
80	8.7	7.0	10.6


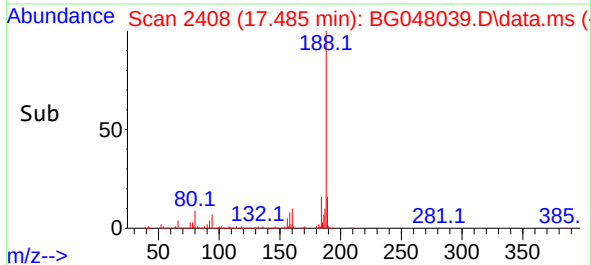
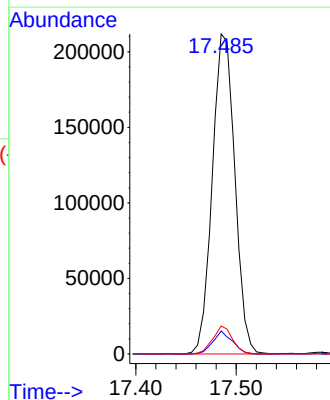
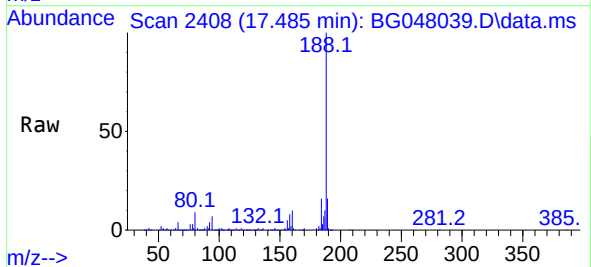




#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.762 min Scan# 3136
Delta R.T. -0.013 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18




Instrument :
BNA_G
ClientSampleId :
0021-SITE-WATER-042


Tgt Ion:240 Resp: 357584
Ion Ratio Lower Upper
240 100
120 5.4 6.2 9.4#
236 27.8 20.5 30.7

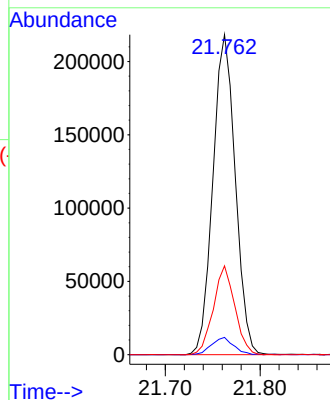

#79
Terphenyl-d14
Concen: 66.69 ng
RT: 20.094 min Scan# 2852
Delta R.T. -0.001 min
Lab File: BG048039.D
Acq: 27 Jan 2021 22:18

Tgt Ion:244 Resp: 1375364
Ion Ratio Lower Upper
244 100
212 8.2 6.7 10.1
122 6.5 7.8 11.6#

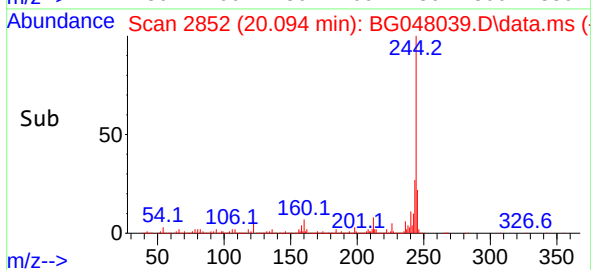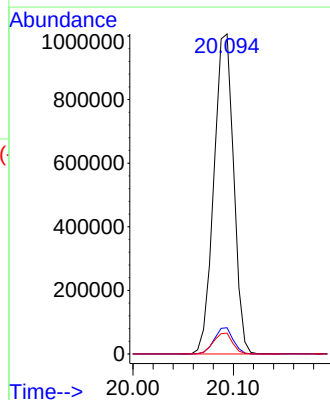

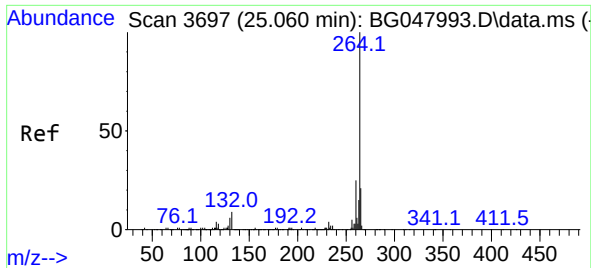

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.047 min Scan# 3695
 Delta R.T. -0.013 min
 Lab File: BG048039.D
 Acq: 27 Jan 2021 22:18

Instrument :
 BNA_G
 ClientSampleId :
 0021-SITE-WATER-042

Tgt Ion:264	Resp:	354355
Ion Ratio	Lower	Upper
264	100	
260	25.1	18.8 28.2
265	21.3	17.8 26.8

