

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
 Data File : BG048042.D
 Acq On : 28 Jan 2021 00:20
 Operator : CG/JU
 Sample : M1226-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0051-045-COMP-E-ELUTRIATE

Quant Time: Jan 28 03:57:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 25 19:39:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	47501	20.00	ng	0.00
21) Naphthalene-d8	10.937	136	183161	20.00	ng	-0.01
39) Acenaphthene-d10	14.744	164	130419	20.00	ng	-0.01
64) Phenanthrene-d10	17.488	188	321215	20.00	ng	#-0.01
76) Chrysene-d12	21.759	240	366521	20.00	ng	#-0.02
86) Perylene-d12	25.050	264	365141	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.678	112	223905	72.44	ng	-0.01
7) Phenol-d6	7.264	99	211958	45.10	ng	-0.02
23) Nitrobenzene-d5	9.286	82	352100	76.06	ng	-0.01
42) 2,4,6-Tribromophenol	16.230	330	268186	123.46	ng	-0.01
45) 2-Fluorobiphenyl	13.375	172	774451	76.78	ng	-0.01
79) Terphenyl-d14	20.091	244	1315420	62.23	ng	0.00
Target Compounds						
10) Phenol	7.294	94	20532	4.56	ng	# 67
50) Dimethylphthalate	14.192	163	28285	2.40	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
Data File : BG048042.D
Acq On : 28 Jan 2021 00:20
Operator : CG/JU
Sample : M1226-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE

Quant Time: Jan 28 03:57:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 19:39:42 2021
Response via : Initial Calibration




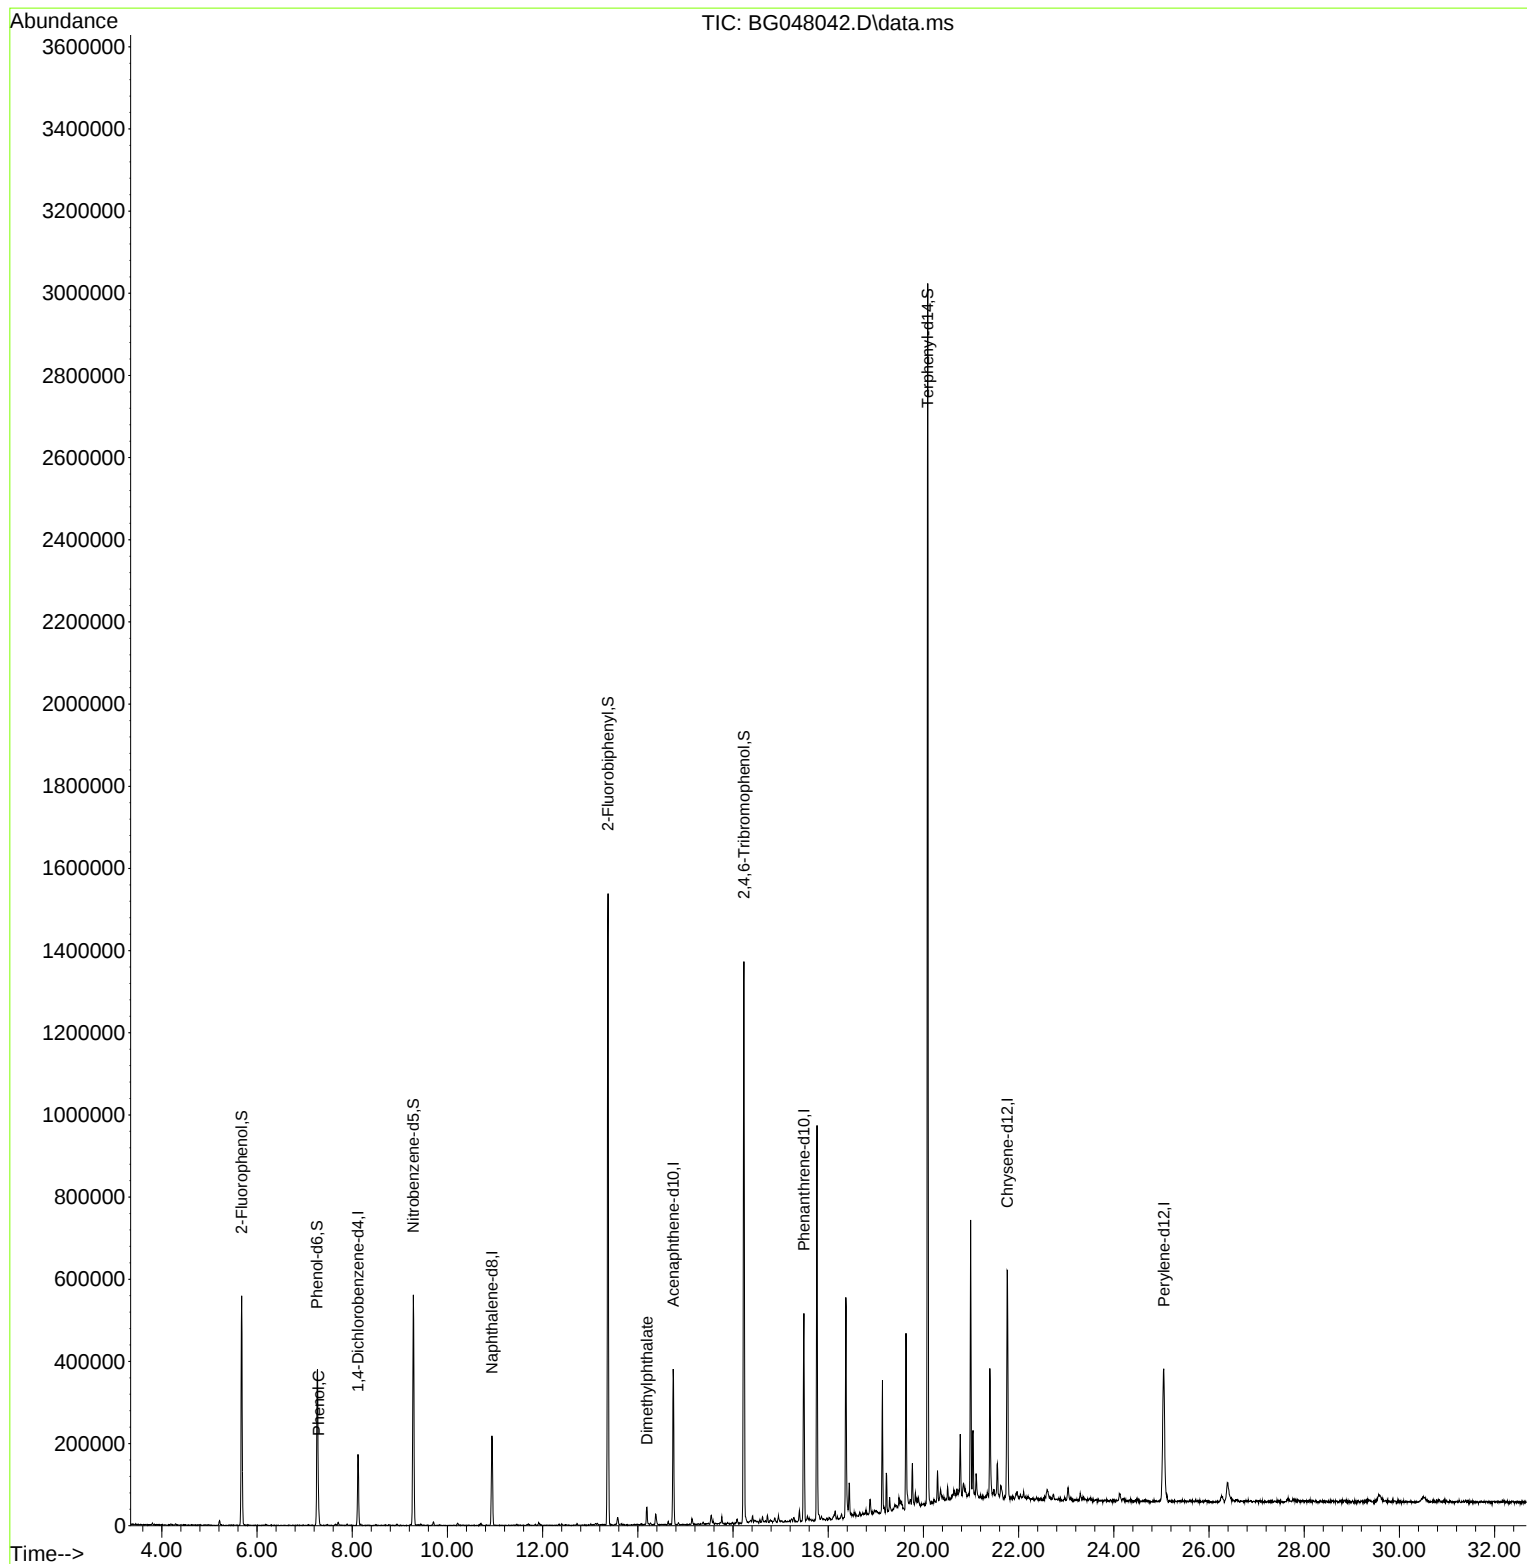




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.122 min Scan# 814
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion:152 Resp: 47501
Ion Ratio Lower Upper
152 100
150 152.9 125.0 187.6
115 56.3 41.8 62.6

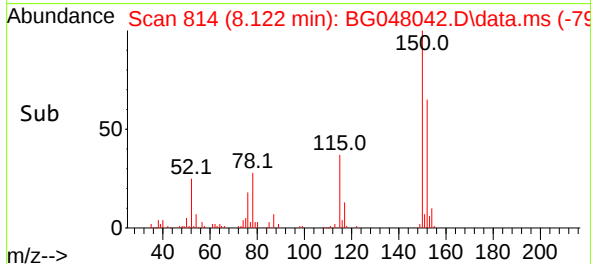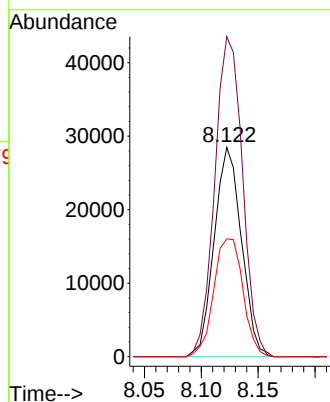

#5
2-Fluorophenol
Concen: 72.44 ng
RT: 5.678 min Scan# 398
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion:112 Resp: 223905
Ion Ratio Lower Upper
112 100
64 66.4 46.7 70.1
63 39.9 22.8 34.2#


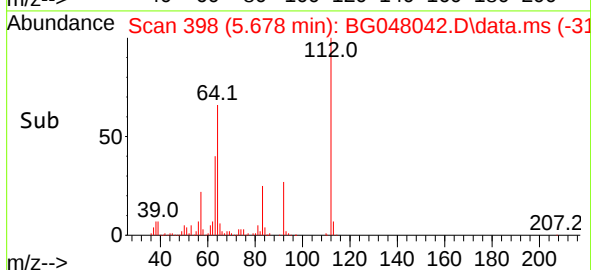
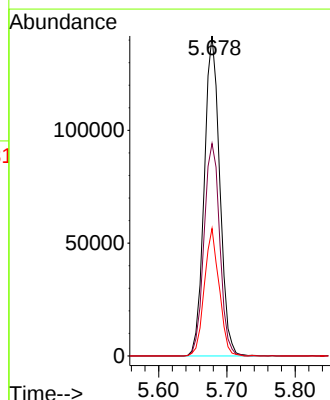





#7
Phenol-d6
Concen: 45.10 ng
RT: 7.264 min Scan# 668
Delta R.T. -0.016 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion: 99 Resp: 211958
Ion Ratio Lower Upper
99 100
42 20.1 12.8 19.2#
71 42.4 24.6 36.8#

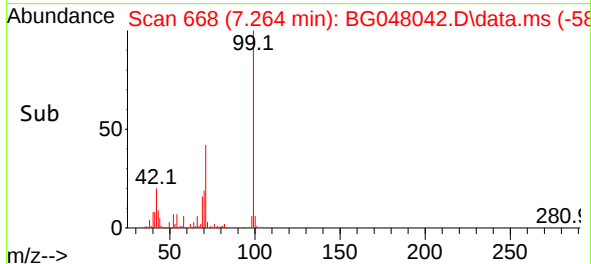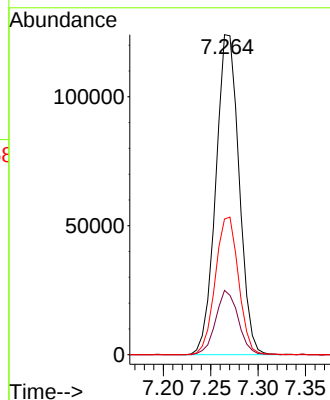

#10
Phenol
Concen: 4.56 ng
RT: 7.294 min Scan# 673
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion: 94 Resp: 20532
Ion Ratio Lower Upper
94 100
65 39.7 6.6 46.6
66 55.7 13.9 53.9#


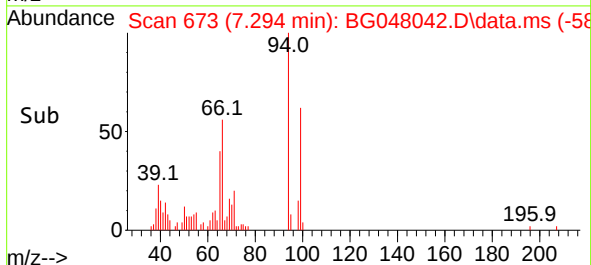
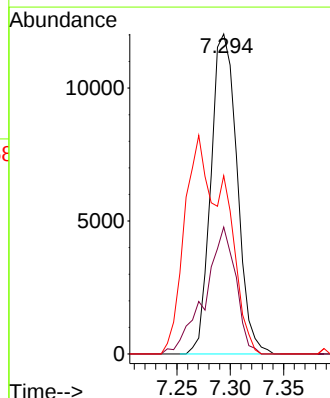
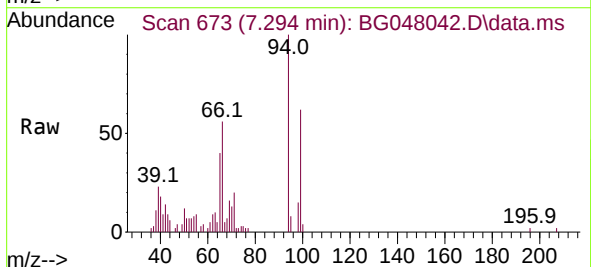




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.937 min Scan# 1293
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion:136	Resp: 183161
Ion Ratio	Lower Upper
136 100	
137 11.4	9.1 13.7
54 7.8	6.2 9.4
68 5.8	5.0 7.4

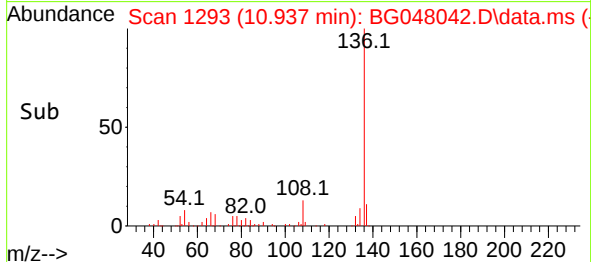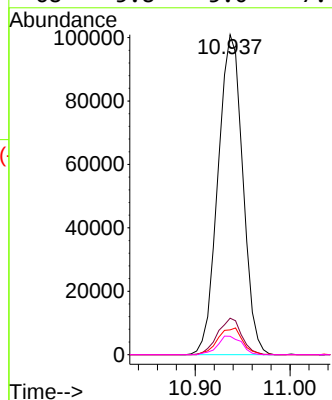

#23
Nitrobenzene-d5
Concen: 76.06 ng
RT: 9.286 min Scan# 1012
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion: 82	Resp: 352100
Ion Ratio	Lower Upper
82 100	
128 37.1	37.0 55.6
54 49.2	39.0 58.4


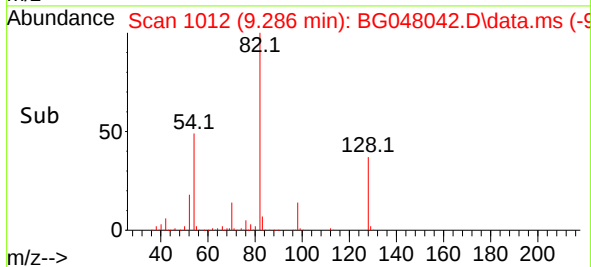
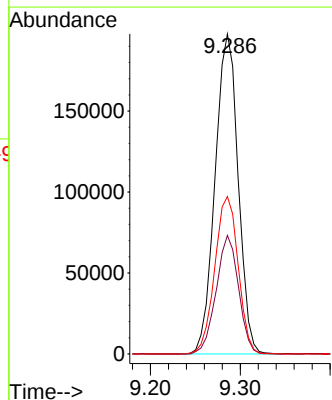
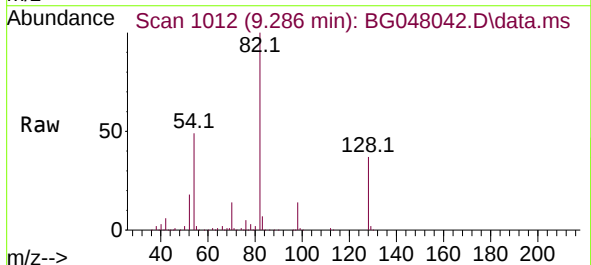




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.744 min Scan# 1941
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion:	164	Resp:	130419
Ion Ratio	Lower	Upper	
164	100		
162	107.1	82.3	123.5
160	43.1	35.3	52.9

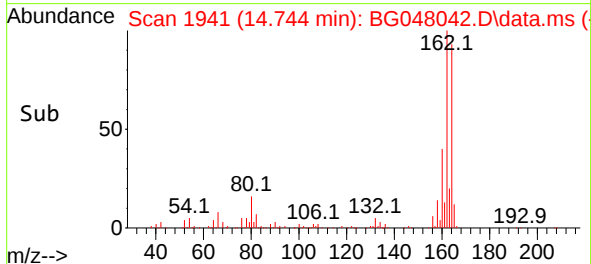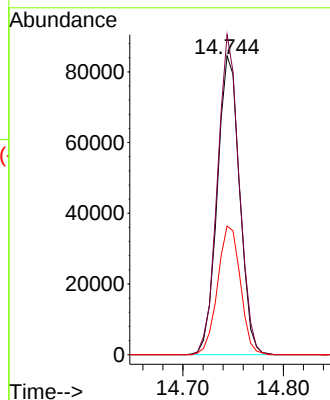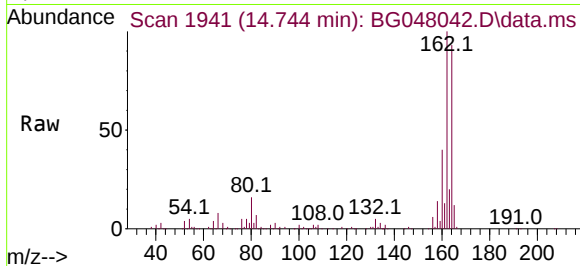

#42
2,4,6-Tribromophenol
Concen: 123.46 ng
RT: 16.230 min Scan# 2194
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion:	330	Resp:	268186
Ion Ratio	Lower	Upper	
330	100		
332	94.2	76.5	114.7
141	33.9	26.0	39.0


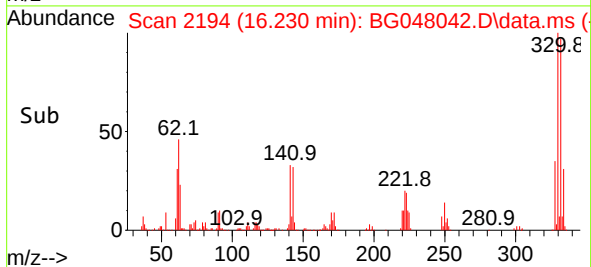
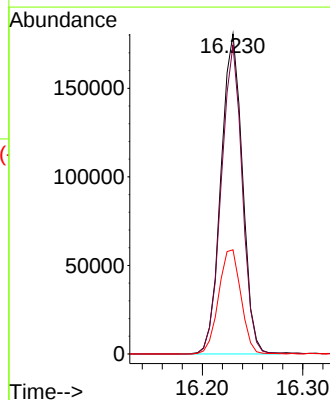
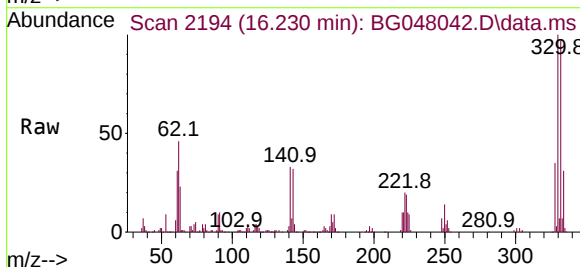




#45
2-Fluorobiphenyl
Concen: 76.78 ng
RT: 13.375 min Scan# 1708
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion:	172	Resp:	774451
Ion Ratio	Lower	Upper	
172	100		
171	36.8	31.3	46.9
170	25.0	20.8	31.2

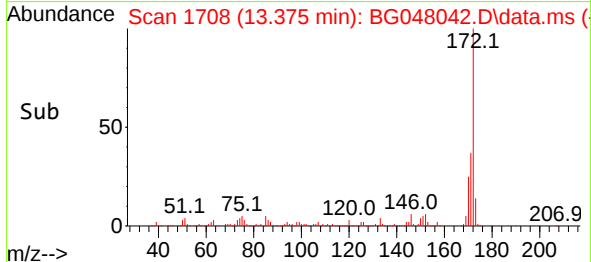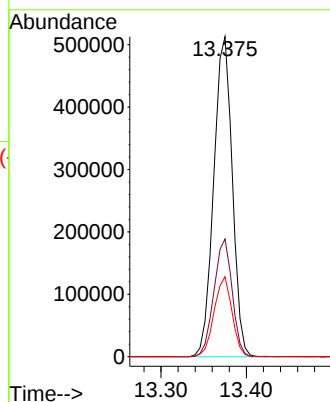

#50
Dimethylphthalate
Concen: 2.40 ng
RT: 14.192 min Scan# 1847
Delta R.T. -0.016 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion:	163	Resp:	28285
Ion Ratio	Lower	Upper	
163	100		
194	5.2	3.8	5.8
164	8.7	8.8	13.2#


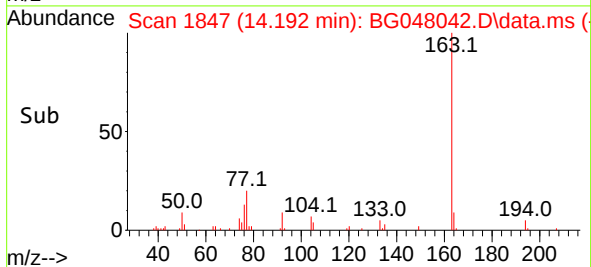
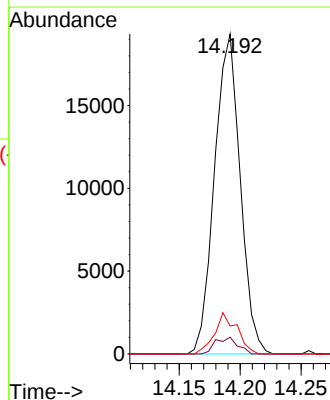
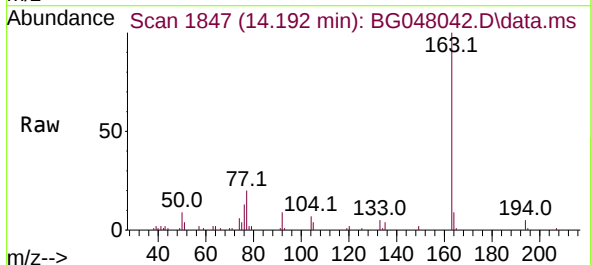




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.488 min Scan# 2408
Delta R.T. -0.010 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20




Instrument :
BNA_G
ClientSampleId :
0051-045-COMP-E-ELUTRIATE


Tgt Ion:188 Resp: 321215
Ion Ratio Lower Upper
188 100
94 5.9 6.3 9.5#
80 7.3 7.0 10.6

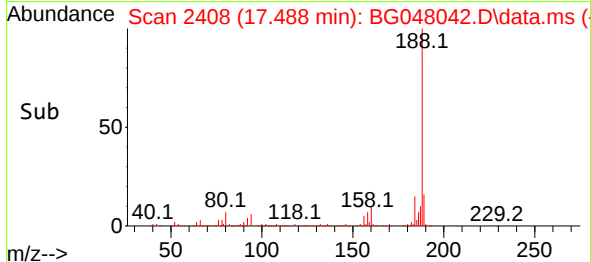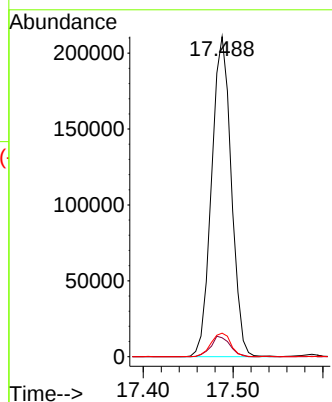

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.759 min Scan# 3135
Delta R.T. -0.016 min
Lab File: BG048042.D
Acq: 28 Jan 2021 00:20

Tgt Ion:240 Resp: 366521
Ion Ratio Lower Upper
240 100
120 5.5 6.2 9.4#
236 27.1 20.5 30.7


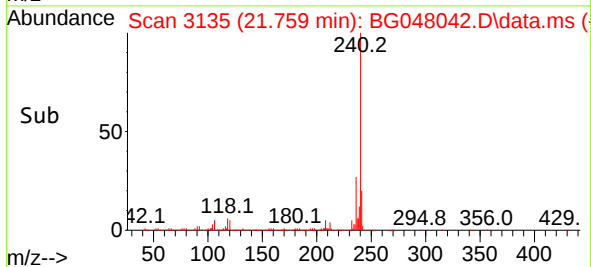
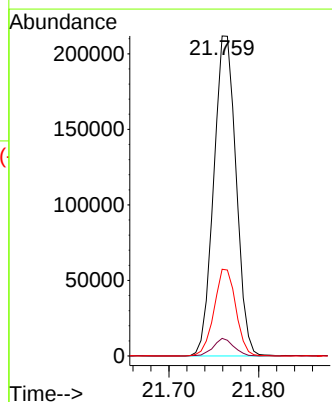
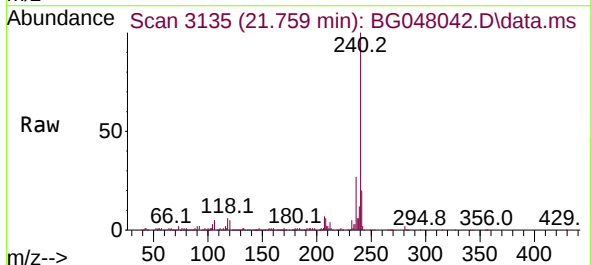




#79
 Terphenyl-d14
 Concen: 62.23 ng
 RT: 20.091 min Scan# 2851
 Delta R.T. -0.004 min
 Lab File: BG048042.D
 Acq: 28 Jan 2021 00:20

Instrument :
 BNA_G
 ClientSampleId :
 0051-045-COMP-E-ELUTRIATE

Tgt Ion:244 Resp: 1315420
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.7 10.1
 122 6.2 7.8 11.6#

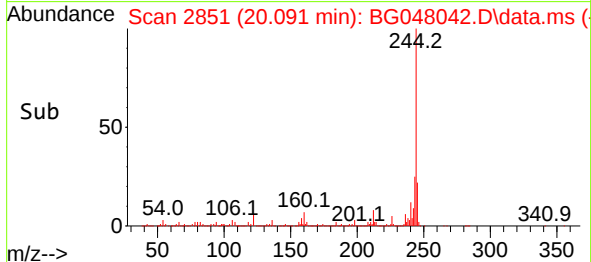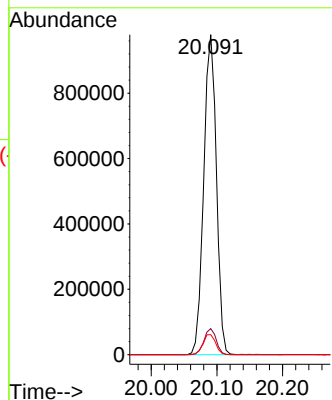

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.050 min Scan# 3695
 Delta R.T. -0.010 min
 Lab File: BG048042.D
 Acq: 28 Jan 2021 00:20

Tgt Ion:264 Resp: 365141
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.8 28.2
 265 22.7 17.8 26.8

