
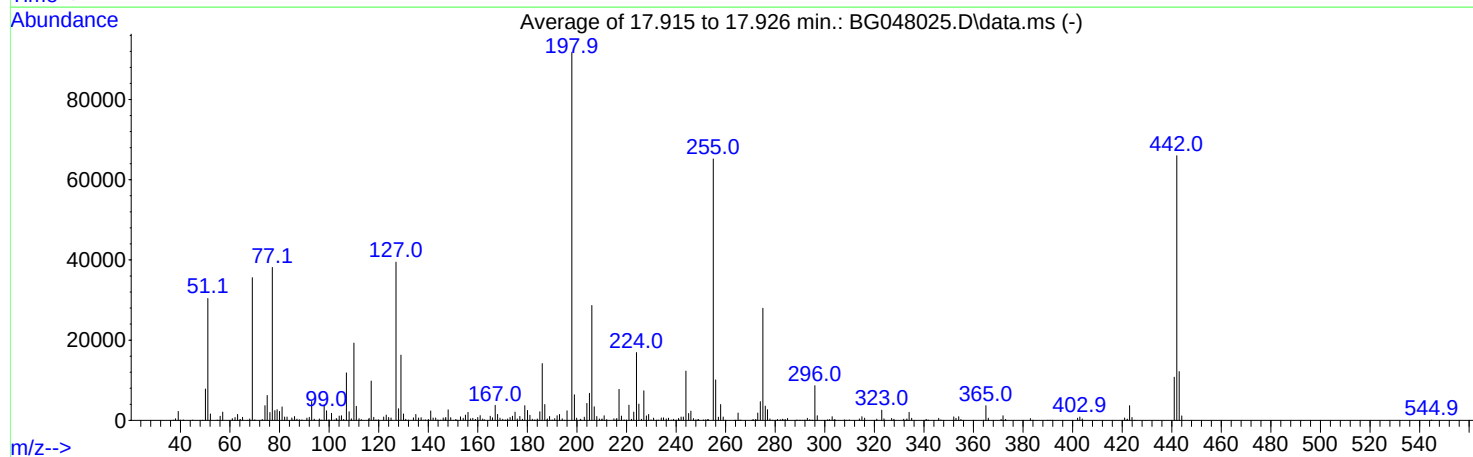


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
 Data File : BG048025.D
 Acq On : 27 Jan 2021 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 19:39:42 2021

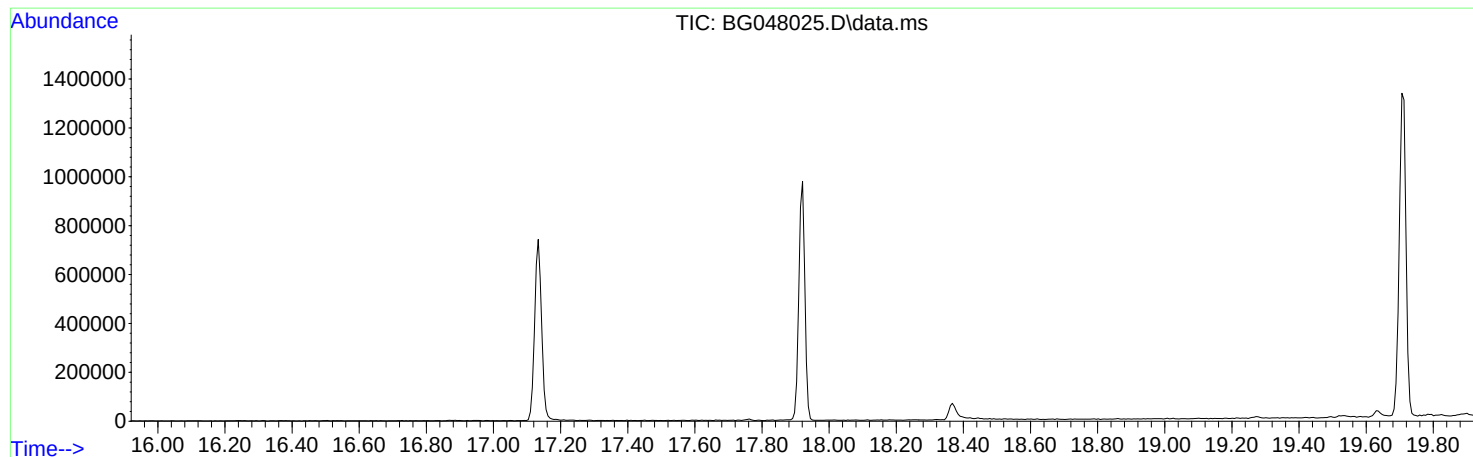

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	30400	PASS
68	69	0.00	2	1.0	358	PASS
69	198	0.00	100	38.8	35589	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	43.0	39477	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91720	PASS
199	198	5	9	7.0	6386	PASS
275	198	10	60	30.5	27973	PASS
365	198	1	100	4.0	3656	PASS
441	198	0.01	100	11.7	10757	PASS
442	198	50	100	72.0	65995	PASS
443	442	15	24	18.5	12190	PASS