
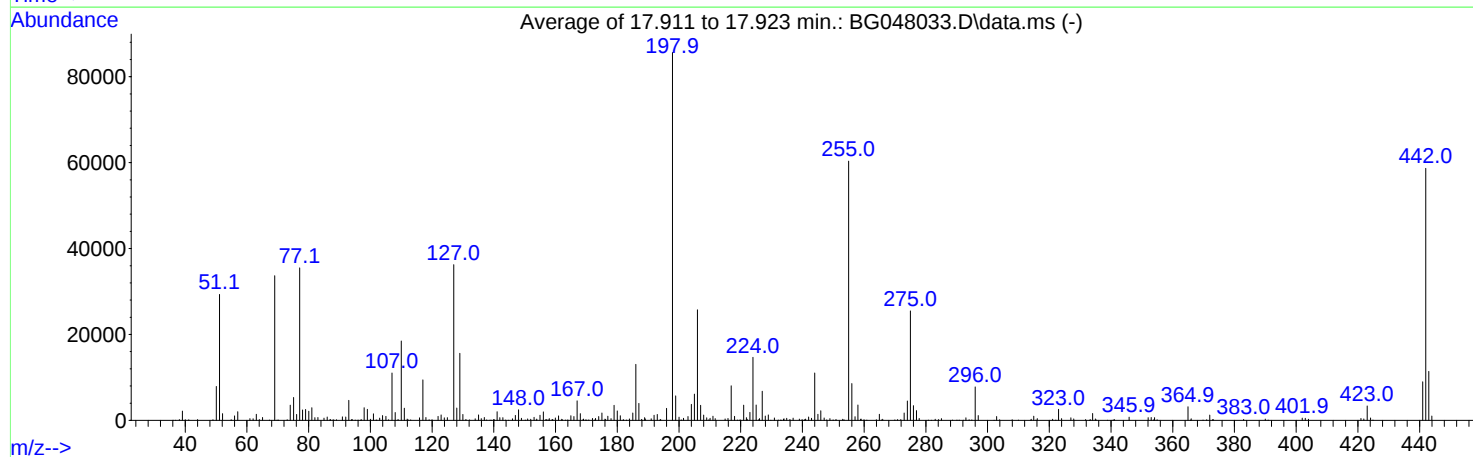


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012721\
 Data File : BG048033.D
 Acq On : 27 Jan 2021 18:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 19:39:42 2021

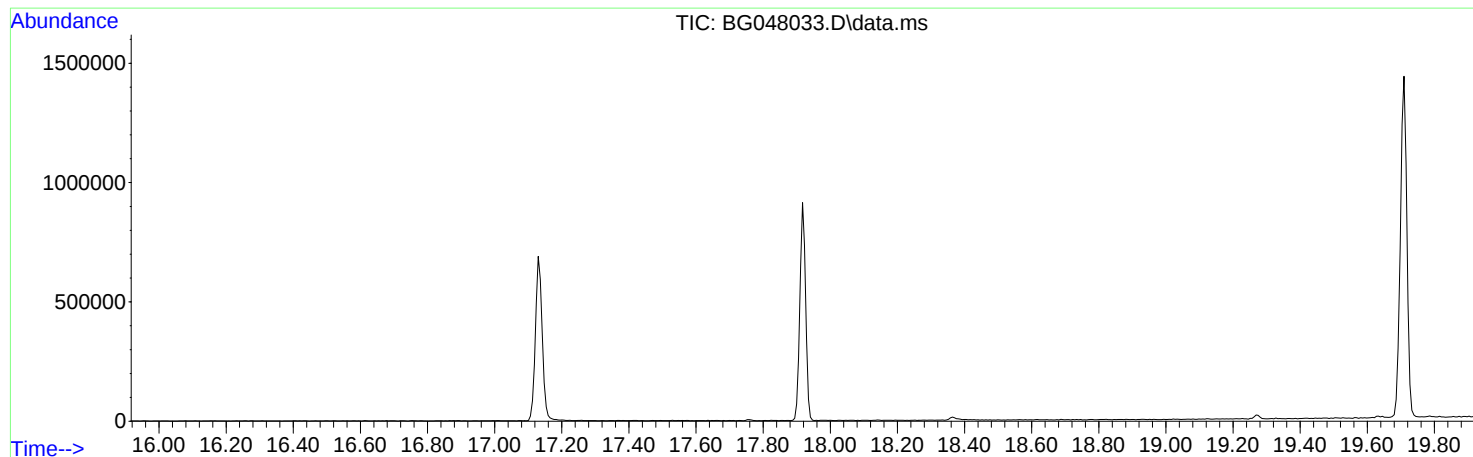

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	29323	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.3	33656	PASS
70	69	0.00	2	0.2	75	PASS
127	198	10	80	42.3	36248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85637	PASS
199	198	5	9	6.6	5688	PASS
275	198	10	60	29.7	25464	PASS
365	198	1	100	3.7	3176	PASS
441	198	0.01	100	10.5	8996	PASS
442	198	50	100	68.5	58672	PASS
443	442	15	24	19.4	11388	PASS