
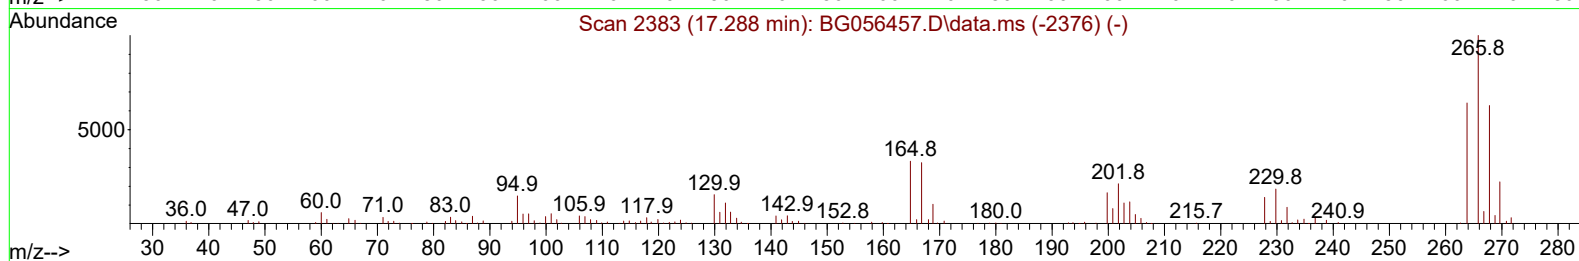
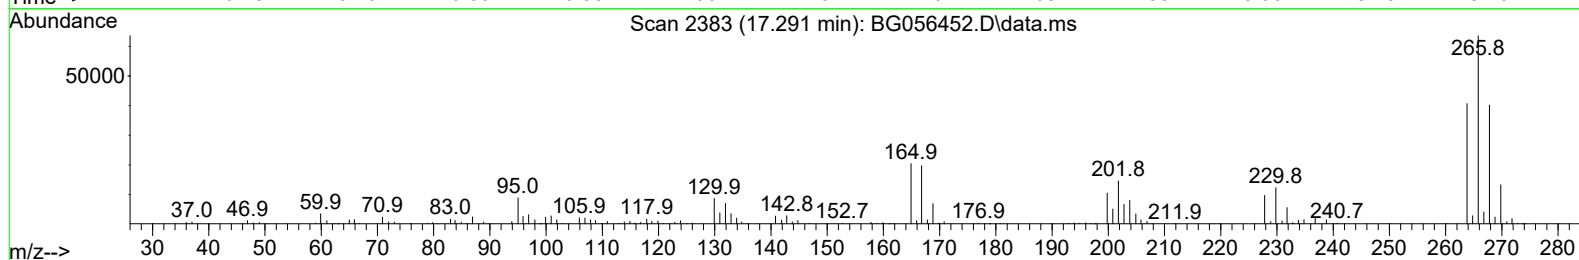


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012723\
Data File : BG056452.D
Acq On : 27 Jan 2023 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:54:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 00:39:13 2023
Response via : Initial Calibration

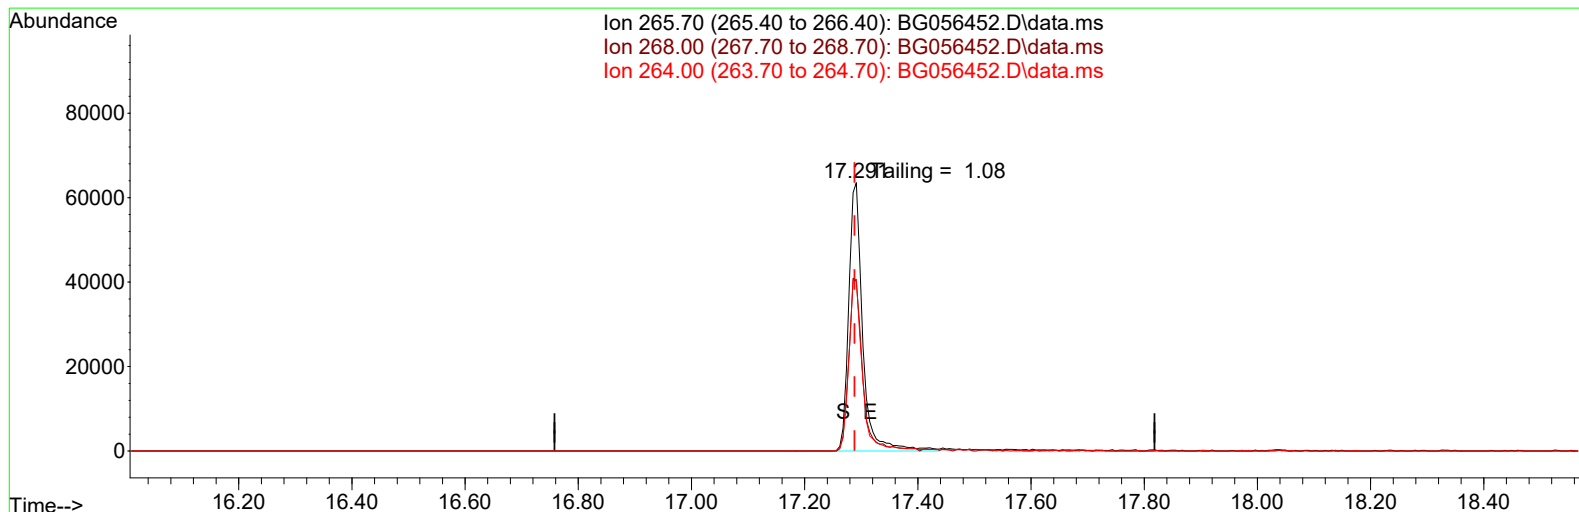

TIC: BG056452.D\data.ms

(70) Pentachlorophenol (C)




17.291min (+ 0.003) 26343.00 ng

response 108323

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.13
264.00	64.20	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012723\
Data File : BG056452.D
Acq On : 27 Jan 2023 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:54:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 00:39:13 2023
Response via : Initial Calibration

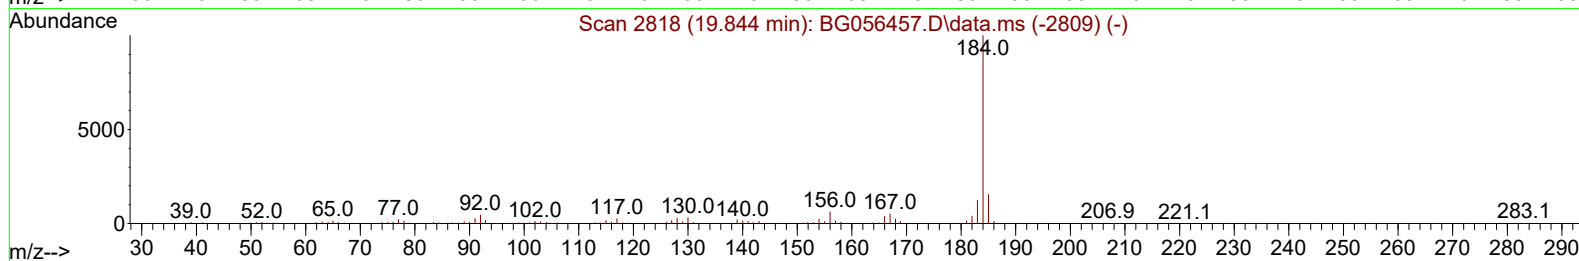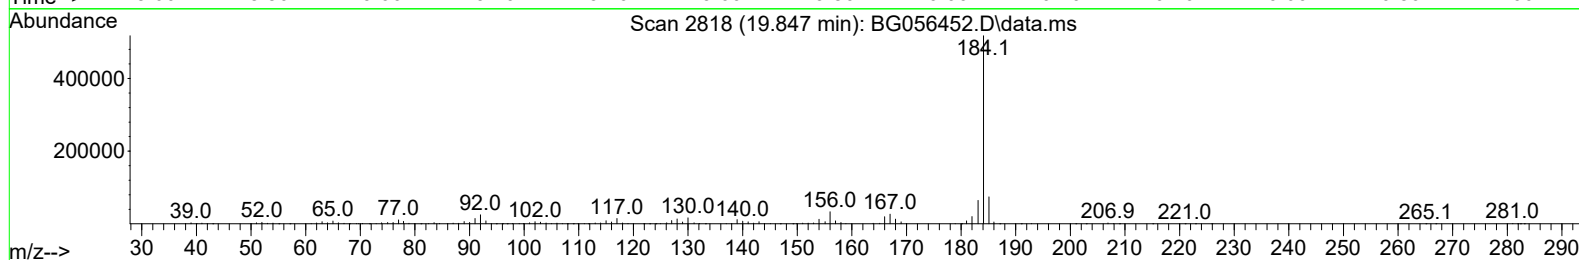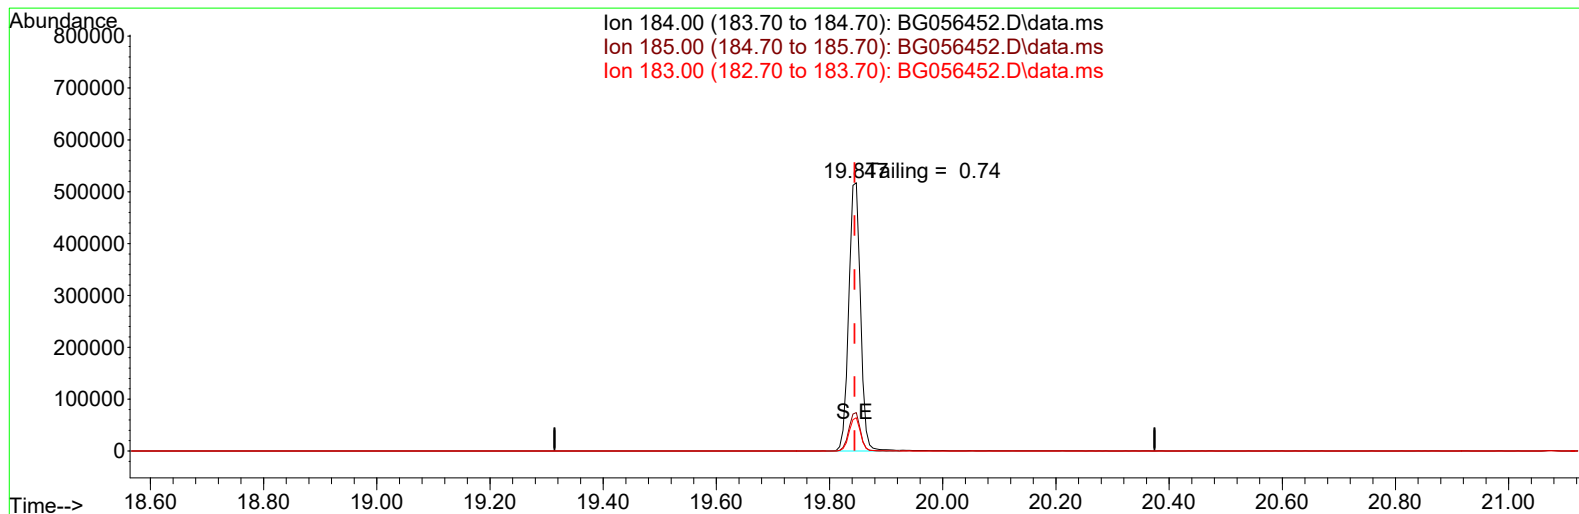

TIC: BG056452.D\data.ms

(77) Benzidine**19.847min (+ 0.003) 423811.29 ng****response 745475**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.33
183.00	12.30	12.43
0.00	0.00	0.00