


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012723\
 Data File : BG056452.D
 Acq On : 27 Jan 2023 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 28 00:39:13 2023

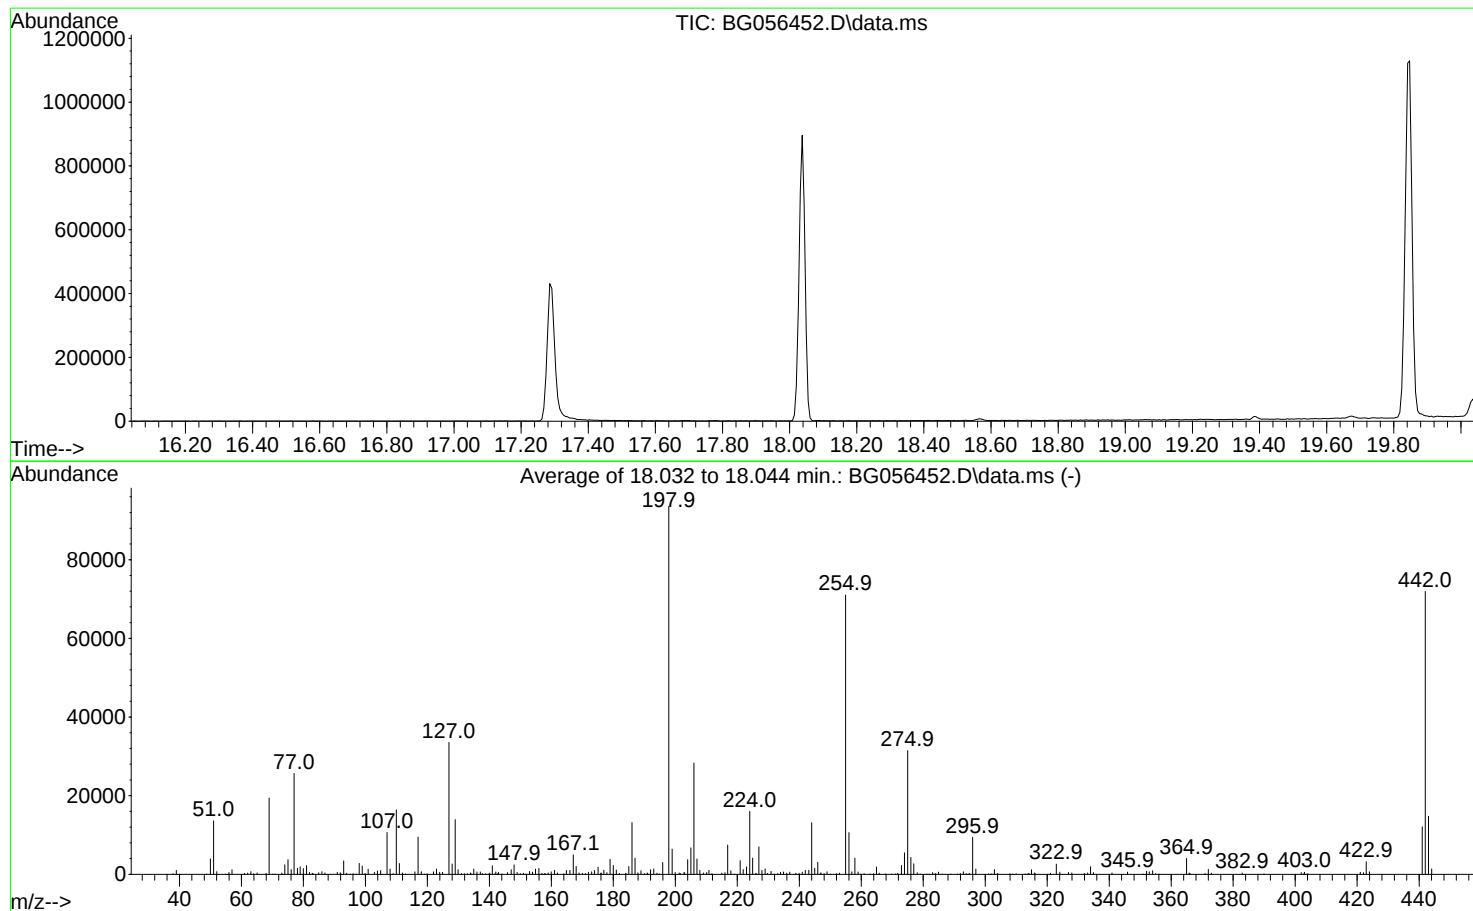




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.5	13601	PASS
68	69	0.00	2	1.3	261	PASS
69	198	0.00	100	20.7	19377	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	35.8	33536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93555	PASS
199	198	5	9	6.9	6416	PASS
275	198	10	60	33.6	31435	PASS
365	198	1	100	4.3	3992	PASS
441	198	0.01	100	12.9	12084	PASS
442	442	50	100	100.0	71923	PASS
443	442	15	24	20.5	14750	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012723\
Data File : BG056452.D
Acq On : 27 Jan 2023 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 28 04:54:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 00:39:13 2023
Response via : Initial Calibration

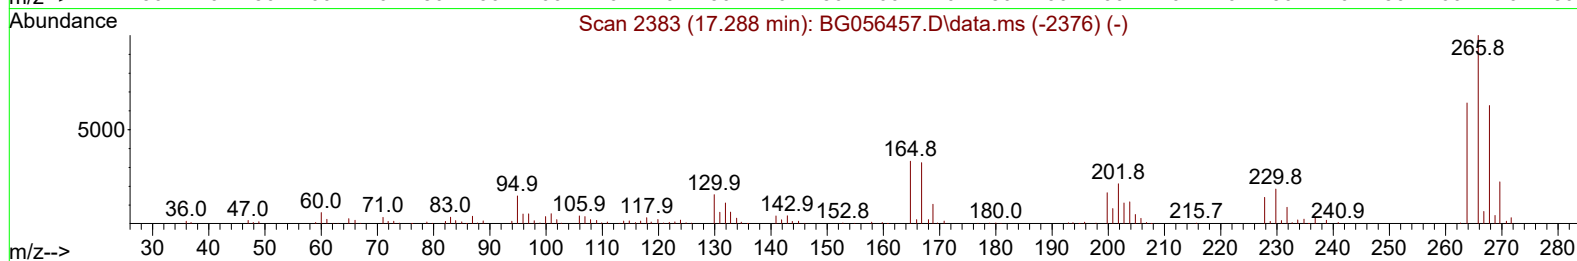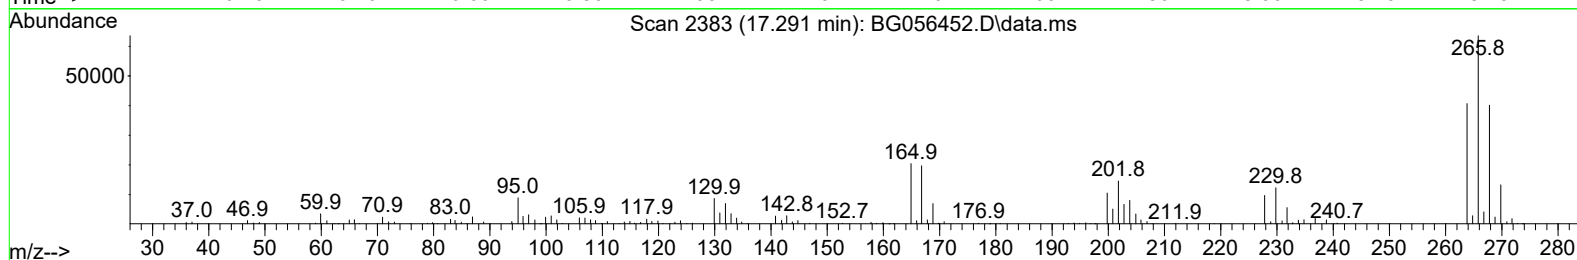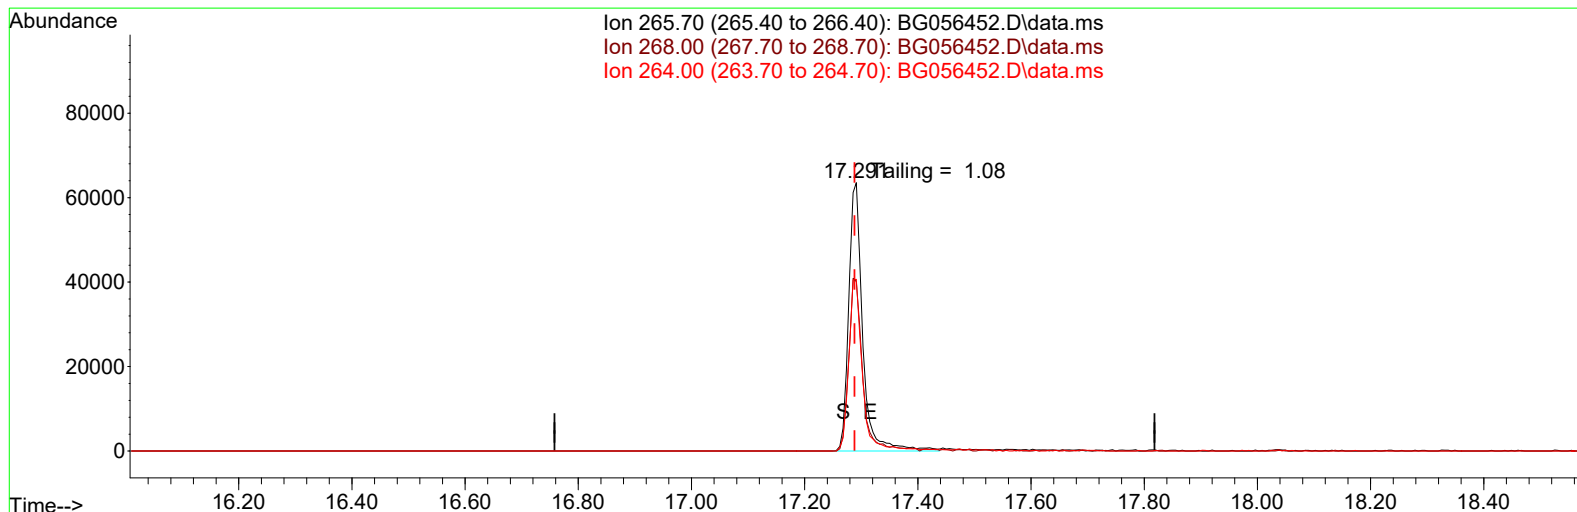

TIC: BG056452.D\data.ms

(70) Pentachlorophenol (C)

17.291min (+ 0.003) 26343.00 ng




response 108323

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.13
264.00	64.20	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012723\
Data File : BG056452.D
Acq On : 27 Jan 2023 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 28 04:54:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 00:39:13 2023
Response via : Initial Calibration

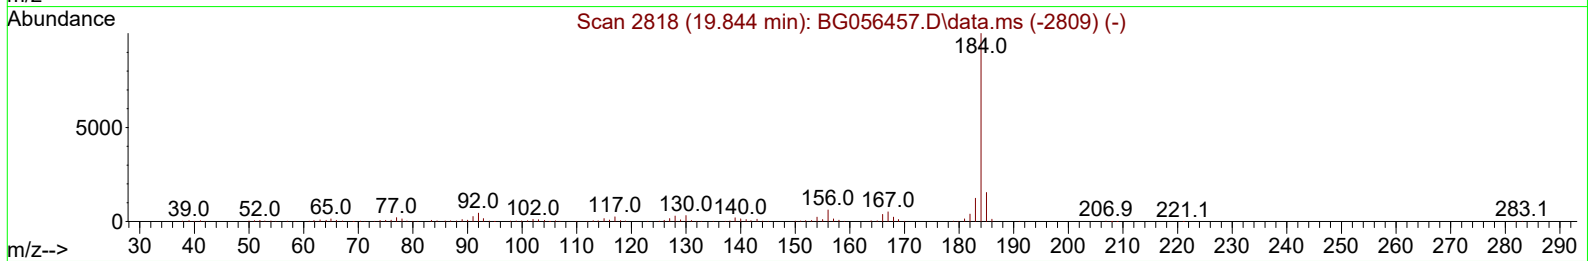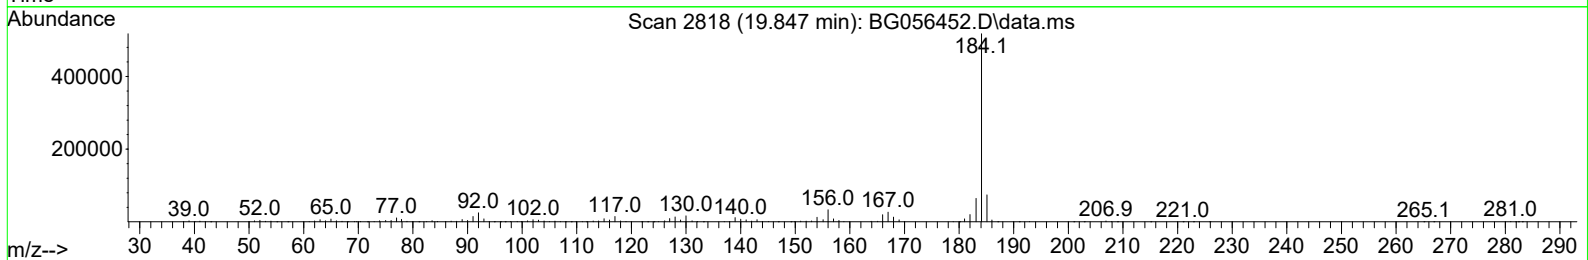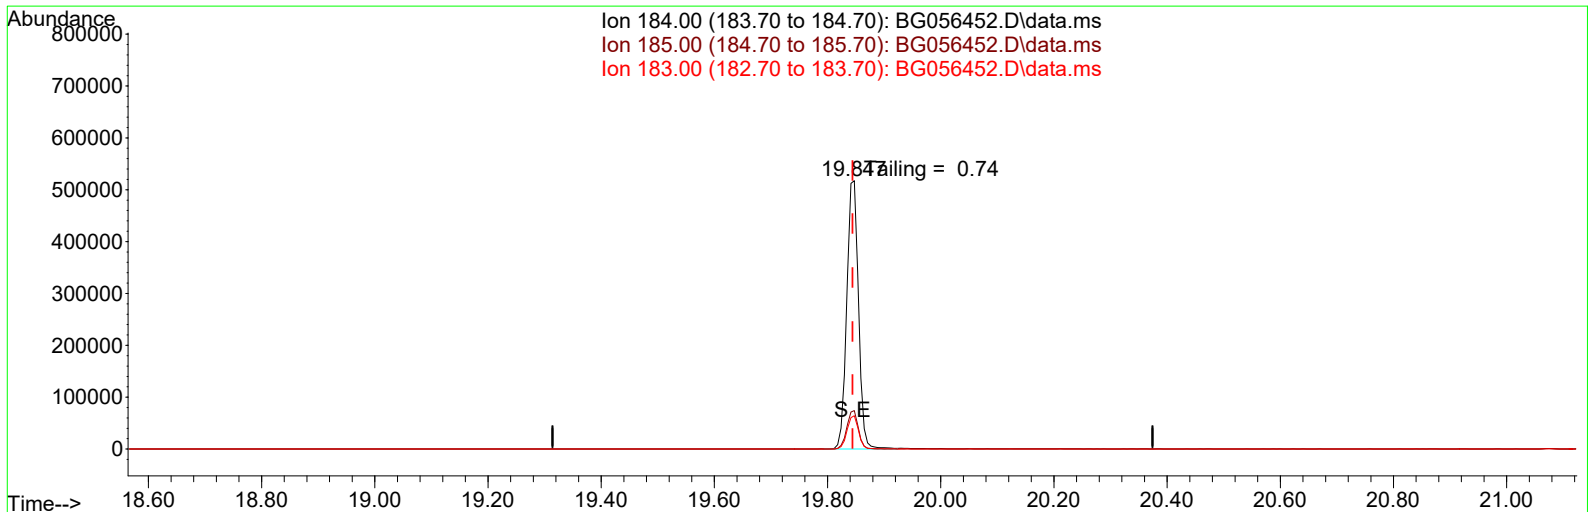

TIC: BG056452.D\data.ms

(77) Benzidine

19.847min (+ 0.003) 423811.29 ng

response 745475

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.33
183.00	12.30	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_G	<u>BG056452.D</u>
Compound Name	Response	Retention Time
DDT	348907	21.075
DDD	5227	20.676
DDE	210	20.129
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5437	354344	1.53

Instrument :
BNA_G
ClientSampleId :
DFTPP