
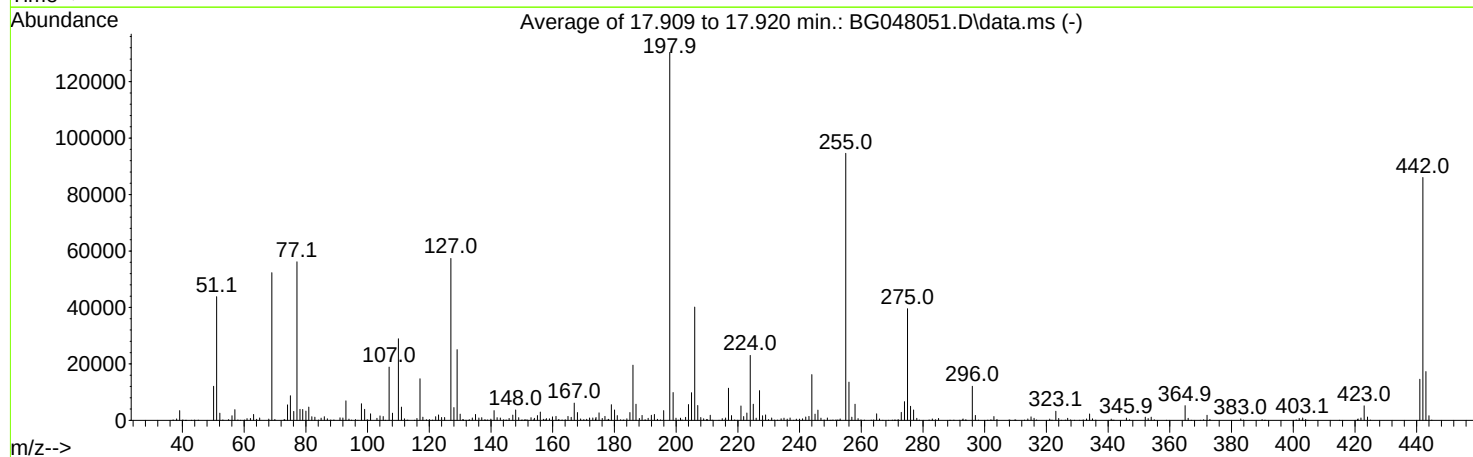


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012821\
 Data File : BG048051.D
 Acq On : 28 Jan 2021 9:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 19:39:42 2021

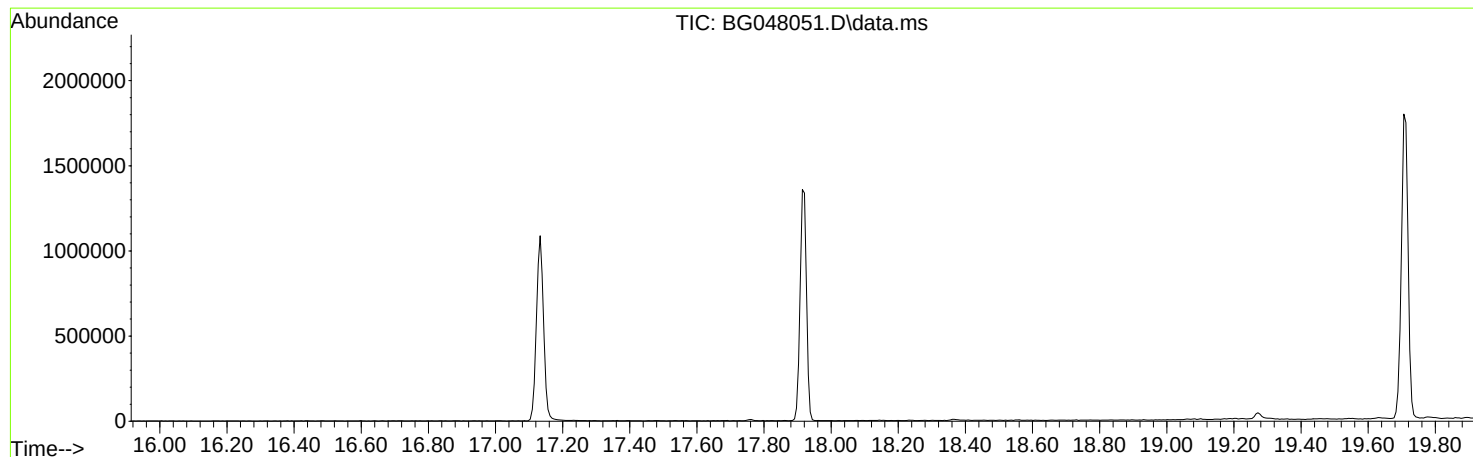

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	43843	PASS
68	69	0.00	2	0.9	472	PASS
69	198	0.00	100	40.1	52296	PASS
70	69	0.00	2	0.7	362	PASS
127	198	10	80	44.0	57368	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	130317	PASS
199	198	5	9	7.6	9853	PASS
275	198	10	60	30.4	39563	PASS
365	198	1	100	4.0	5226	PASS
441	198	0.01	100	11.2	14544	PASS
442	198	50	100	66.0	86072	PASS
443	442	15	24	20.1	17285	PASS