


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012916\
Data File : BG020766.D
Acq On : 29 Jan 2016 8:47
Operator : SJ/IZ
Sample : DFTPP26
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP26

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 27 17:29:07 2016

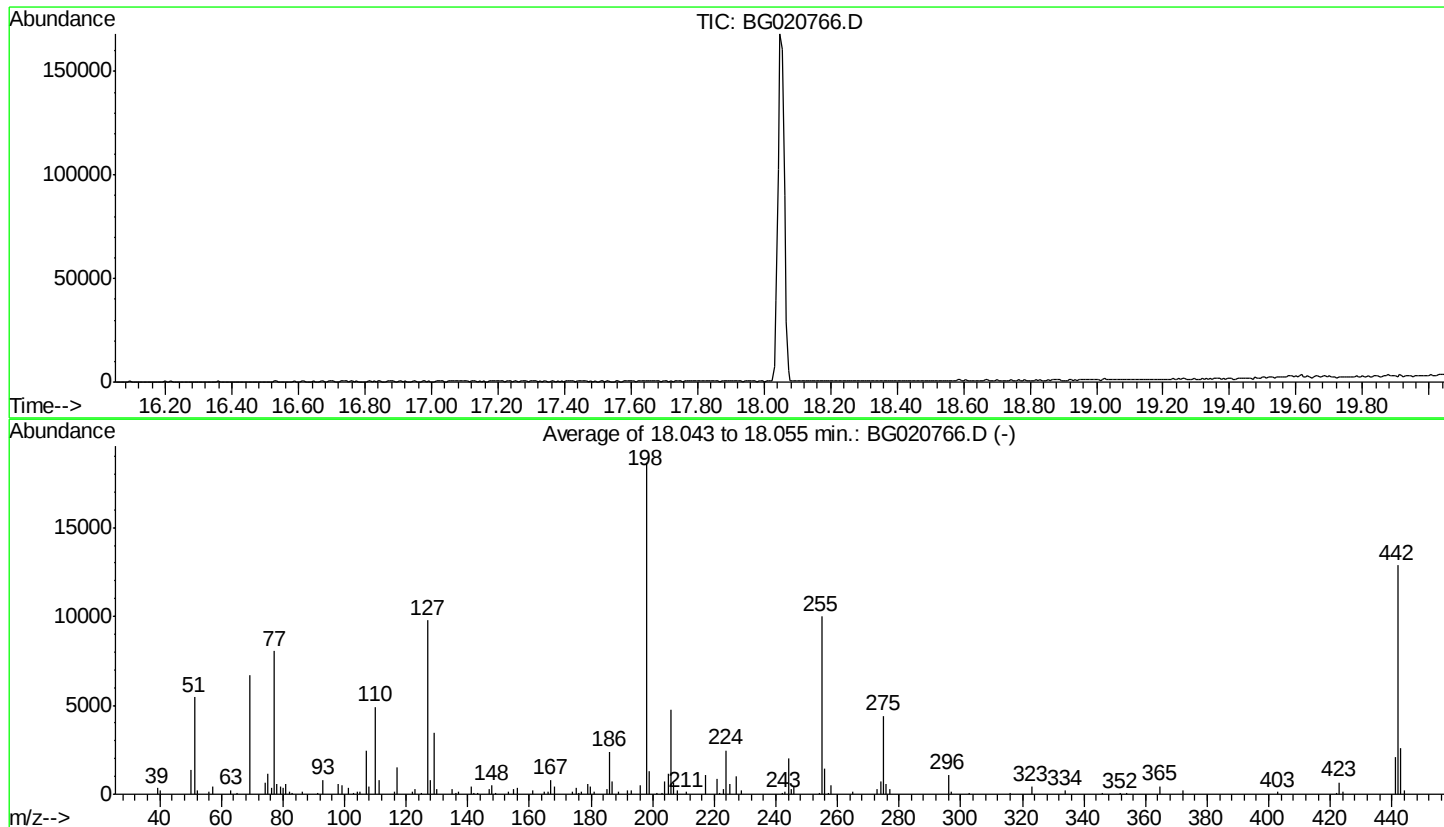

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	5437	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	6713	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	9778	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18645	PASS
199	198	5	9	6.8	1275	PASS
275	198	10	60	23.7	4422	PASS
365	198	1	100	2.5	459	PASS
441	442	0.01	100	16.3	2097	PASS
442	198	50	100	69.0	12869	PASS
443	442	15	24	20.1	2591	PASS

m/z	Abundance
39.05	329.0
40.05	229.0
50.15	1223.0
51.15	4474.0
52.05	212.0
56.05	191.0
57.05	296.0
63.05	235.0
69.05	5778.0
74.05	581.0
75.05	934.0
76.15	290.0
77.15	6410.0
78.15	418.0
79.05	328.0
79.95	352.0
81.05	538.0
86.05	150.0
93.05	626.0
98.05	491.0
98.95	361.0
101.05	267.0
107.05	1886.0
108.05	334.0
110.05	3912.0
111.05	658.0
117.05	1107.0
122.95	237.0
127.05	7637.0
128.05	688.0
129.05	2572.0
129.95	266.0
135.05	307.0
140.95	311.0
147.05	215.0
147.95	389.0
148.95	162.0
155.05	261.0
156.05	284.0
160.95	200.0
167.05	522.0
167.95	353.0
175.05	292.0
178.95	430.0
179.95	397.0
185.05	207.0
186.05	1695.0
186.95	515.0
191.95	214.0
192.95	152.0
195.95	381.0
197.95	13233.0
198.95	1080.0
203.95	466.0
204.95	793.0
206.05	3177.0
206.95	830.0
207.95	161.0
216.95	810.0
220.95	585.0
222.85	201.0
223.95	1869.0
224.95	438.0
226.95	796.0
228.85	156.0
243.95	1391.0
244.95	208.0
245.95	285.0
254.95	6980.0
255.95	1155.0
257.95	305.0
272.95	181.0
273.95	571.0
274.95	3040.0
275.95	360.0
276.95	206.0
295.95	710.0
322.95	223.0
333.95	158.0
364.85	331.0
371.95	179.0
422.95	364.0
440.95	1309.0
441.95	7037.0
442.95	1421.0
443.85	167.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26

m/z	Abundance
39.15	437.0
40.05	181.0
50.15	1575.0
51.15	6404.0
52.15	291.0
56.05	190.0
57.05	514.0
63.05	285.0
69.05	7547.0
74.05	771.0
75.05	1284.0
76.15	485.0
77.15	9380.0
78.05	663.0
79.05	440.0
79.95	344.0
81.05	695.0
82.05	183.0
86.05	182.0
91.05	172.0
93.05	901.0
97.95	746.0
99.05	698.0
101.05	355.0
104.05	172.0
105.05	182.0
107.05	2978.0
108.05	552.0
110.05	5758.0
111.05	823.0
115.95	201.0
117.05	1868.0
122.05	162.0
123.05	287.0
125.05	152.0
127.05	11432.0
128.05	828.0
129.05	3957.0
130.05	351.0
134.95	320.0
136.05	172.0
136.95	226.0
141.05	415.0
146.95	271.0
147.95	504.0
148.95	150.0
153.05	171.0
155.05	311.0
156.05	346.0
161.05	218.0
165.05	183.0
165.95	157.0
167.05	1102.0
168.05	507.0
173.95	227.0
174.95	420.0
176.05	185.0
176.95	225.0
178.95	642.0
179.95	563.0
180.95	252.0
185.05	326.0
186.05	2888.0
186.95	762.0
188.95	178.0
191.95	166.0
192.95	255.0
195.95	673.0
197.95	22280.0
198.95	1492.0
201.55	172.0
204.05	792.0
204.95	1489.0
206.05	5790.0
206.95	1102.0
208.05	270.0
210.95	193.0
216.95	1217.0
220.95	975.0
221.85	259.0
222.95	370.0
224.05	2821.0
224.95	642.0
226.95	1208.0
228.95	290.0
242.95	162.0
243.95	2314.0
244.95	336.0
245.95	386.0
254.95	11240.0
255.95	1664.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26

256.95	159.0
257.95	617.0
264.95	199.0
272.95	354.0
273.95	845.0
274.95	5189.0
275.95	696.0
276.95	392.0
295.95	1330.0
296.95	190.0
302.95	215.0
315.95	154.0
322.95	481.0
333.95	243.0
353.95	167.0
364.85	480.0
371.95	260.0
402.95	194.0
421.95	162.0
422.95	802.0
423.95	261.0
440.95	2232.0
441.95	14451.0
442.95	3182.0
443.95	240.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26

m/z	Abundance
39.05	286.0
40.05	172.0
50.15	1286.0
51.15	5435.0
52.05	222.0
57.05	439.0
63.05	239.0
65.05	187.0
69.05	6816.0
74.05	646.0
75.05	1155.0
76.05	398.0
77.15	8333.0
78.05	702.0
79.05	520.0
80.05	402.0
81.05	601.0
82.05	199.0
83.05	158.0
86.05	172.0
93.05	954.0
98.05	532.0
99.05	472.0
101.05	382.0
103.05	151.0
104.05	213.0
105.05	163.0
107.05	2492.0
108.05	476.0
110.05	5072.0
111.05	854.0
116.05	173.0
117.05	1642.0
121.95	199.0
122.95	281.0
127.05	10267.0
127.95	822.0
129.05	3805.0
130.05	282.0
135.05	323.0
137.05	193.0
141.05	501.0
142.05	184.0
143.05	159.0
147.05	314.0
147.95	528.0
152.95	212.0
154.95	254.0
156.05	381.0
160.95	214.0
164.95	238.0
165.95	186.0
166.95	849.0
167.95	395.0
173.95	178.0
175.05	404.0
176.95	212.0
178.95	735.0
179.95	452.0
180.95	216.0
185.05	333.0
185.95	2614.0
186.95	803.0
188.95	160.0
191.95	238.0
192.95	269.0
195.95	537.0
197.95	20424.0
198.95	1254.0
202.95	156.0
203.95	857.0
204.95	1236.0
206.05	5299.0
206.95	1097.0
207.95	210.0
211.05	206.0
216.95	1176.0
220.95	1137.0
222.95	249.0
224.05	2744.0
224.95	606.0
226.95	1030.0
228.95	318.0
241.95	162.0
242.85	182.0
244.05	2323.0
245.05	272.0
245.95	529.0
253.95	176.0
254.95	11695.0
255.95	1533.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26

257.95	595.0
264.95	246.0
272.95	401.0
273.95	794.0
274.95	5039.0
275.95	635.0
276.95	294.0
295.95	1299.0
296.95	208.0
322.95	547.0
333.95	218.0
345.95	155.0
351.85	205.0
364.85	566.0
371.95	183.0
402.95	207.0
422.95	846.0
423.95	189.0
440.95	2752.0
441.95	17120.0
442.95	3171.0
443.95	350.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26

m/z	Abundance
206.95	383.0

Instrument :
BNA_G
ClientSampleId :
DFTPP26