
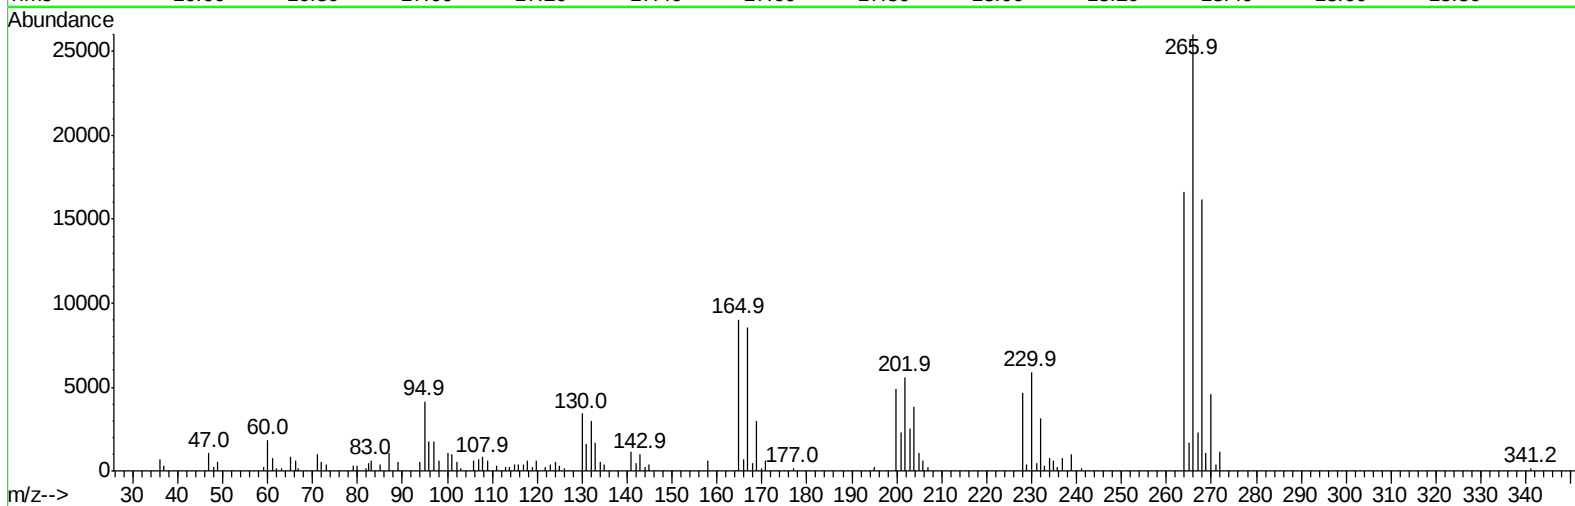


Data Path : U:\HPCHEM1\BNA G\DATA\BG012918\
Data File : BG032406.D
Acq On : 29 Jan 2018 9:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 07:14:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

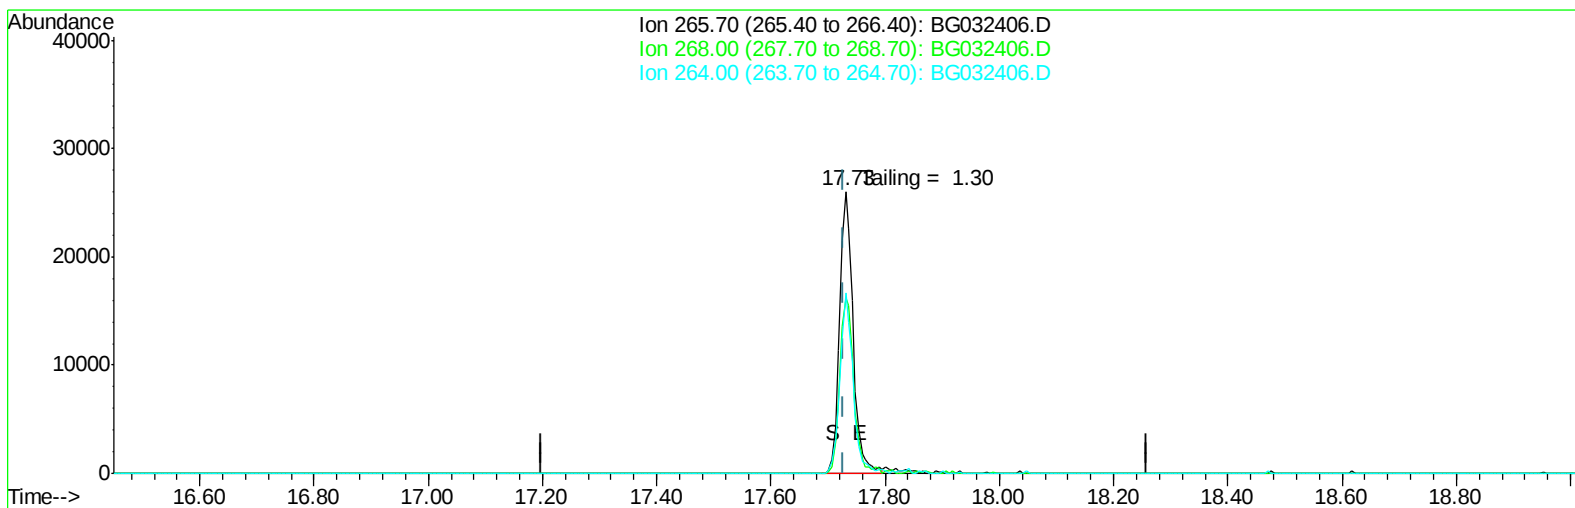

TIC: BG032406.D

(69) Pentachlorophenol (C)



17.730min (+0.002) 29654.90ng

response 42335

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.31
264.00	62.00	63.94
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012918\
Data File : BG032406.D
Acq On : 29 Jan 2018 9:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 07:14:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

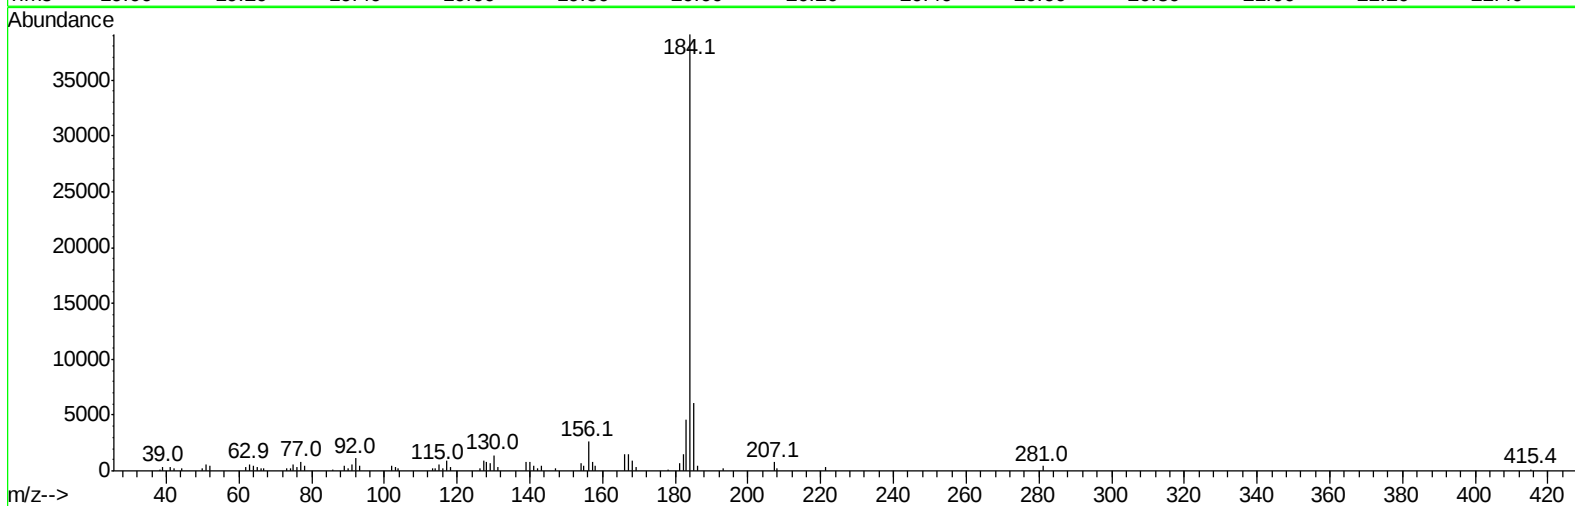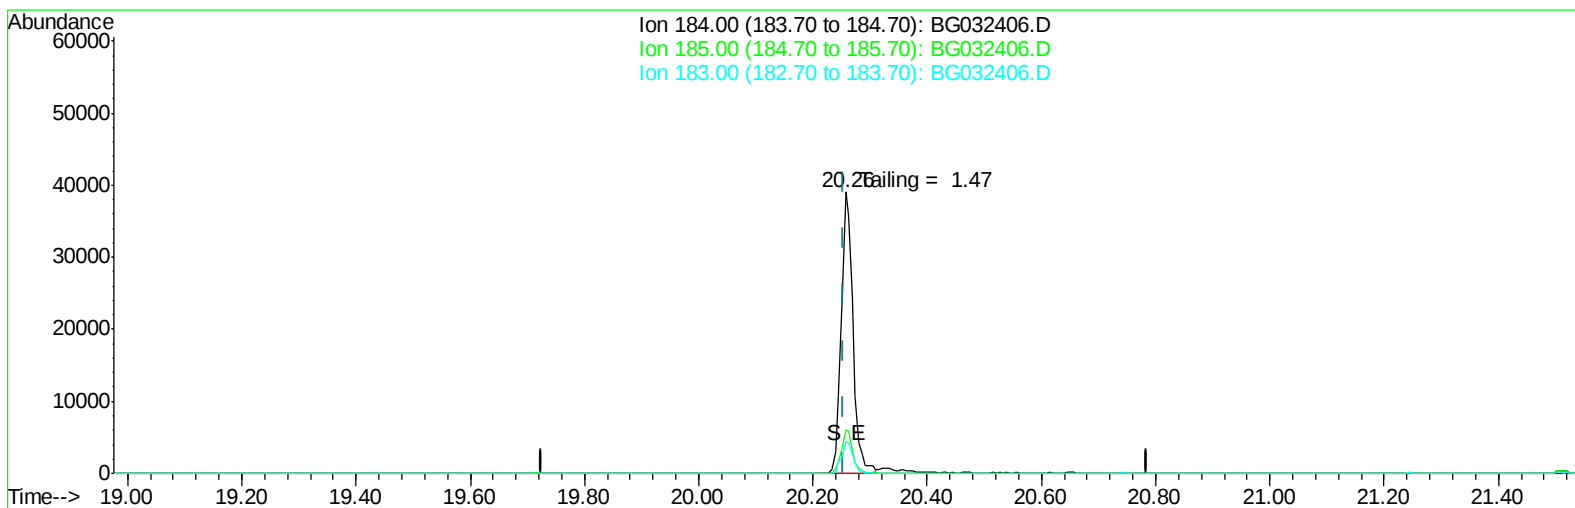

TIC: BG032406.D

(76) Benzidine

20.257min (+0.002) 54184.26ng

response 56390

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.58
183.00	13.30	11.60
0.00	0.00	0.00