
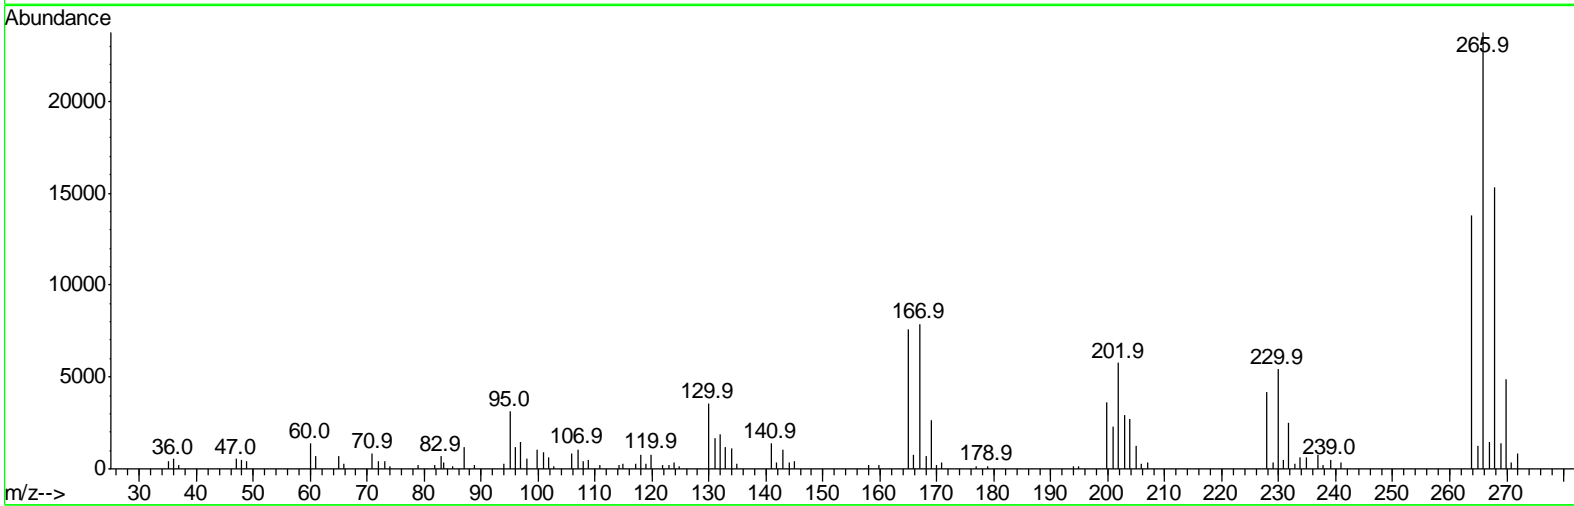


Data Path : U:\HPCHEM1\BNA G\DATA\BG012918\
 Data File : BG032422.D
 Acq On : 29 Jan 2018 19:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 07:16:31 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 15:32:55 2018
 Response via : Initial Calibration

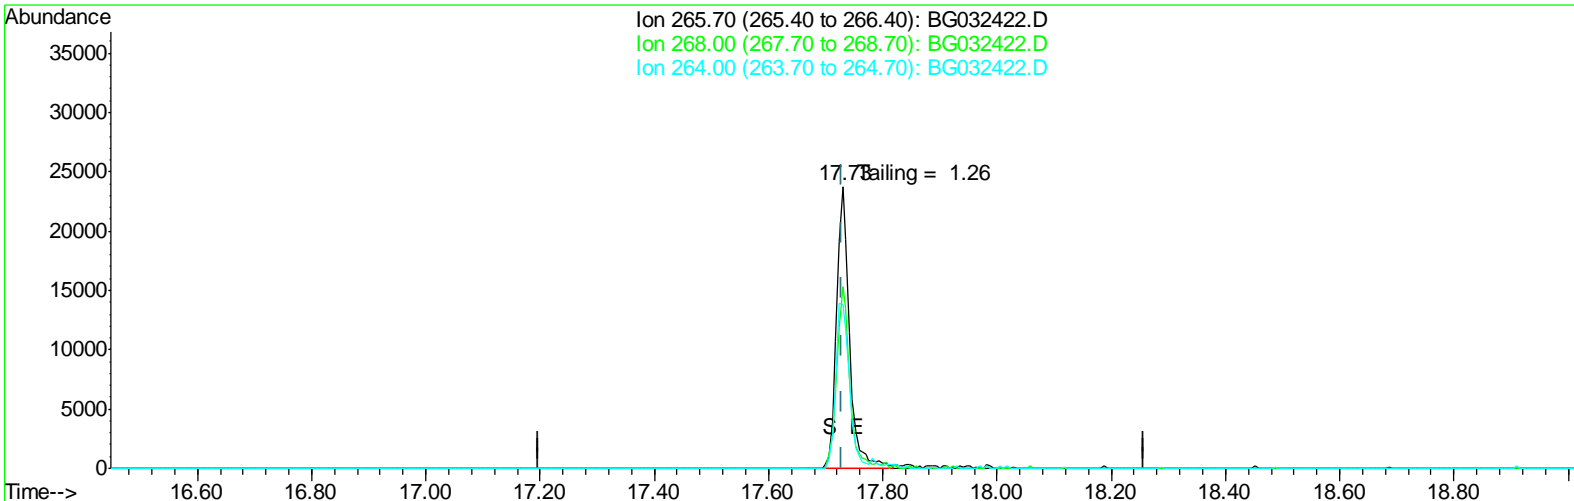

TIC: BG032422.D

(69) Pentachlorophenol (C)



17.729min (+0.001) 68059.53ng

response 37746

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.39
264.00	62.00	57.98
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012918\
 Data File : BG032422.D
 Acq On : 29 Jan 2018 19:56
 Operator : SJ/JU
 Sample : DF7PP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 07:16:31 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 15:32:55 2018
 Response via : Initial Calibration

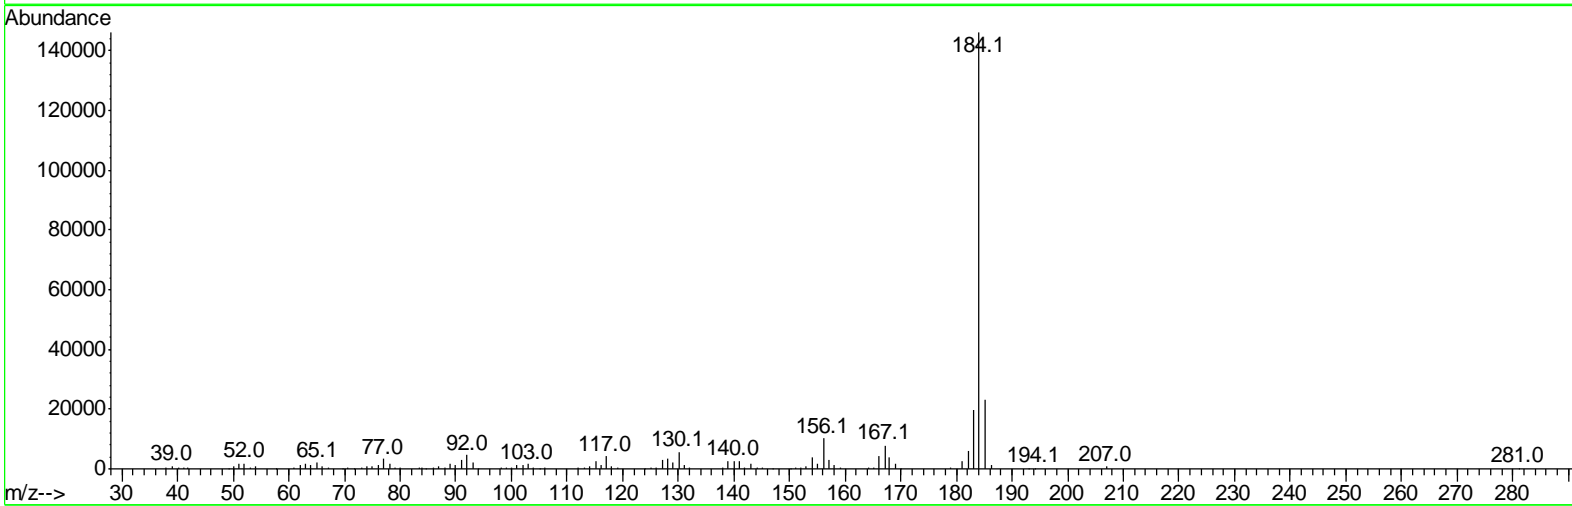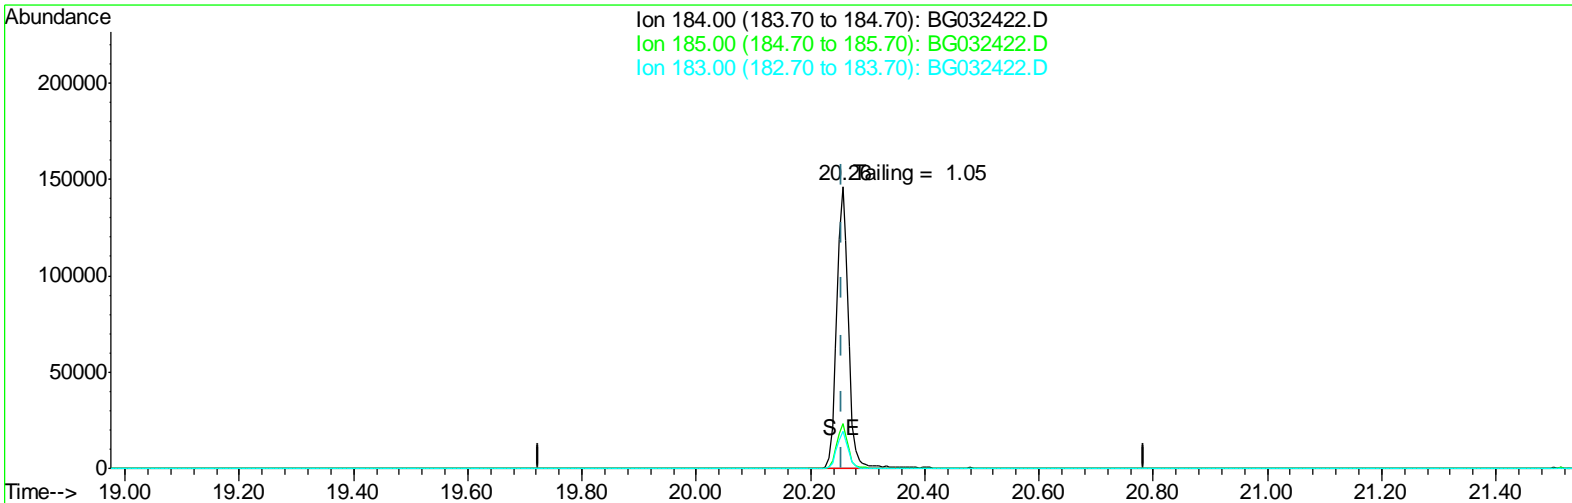

TIC: BG032422.D

(76) Benzidine

20.256min (+0.001) 0.00ng

response 207791

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.84
183.00	13.30	13.35
0.00	0.00	0.00