


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG012918\
 Data File : BG032406.D
 Acq On : 29 Jan 2018 9:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

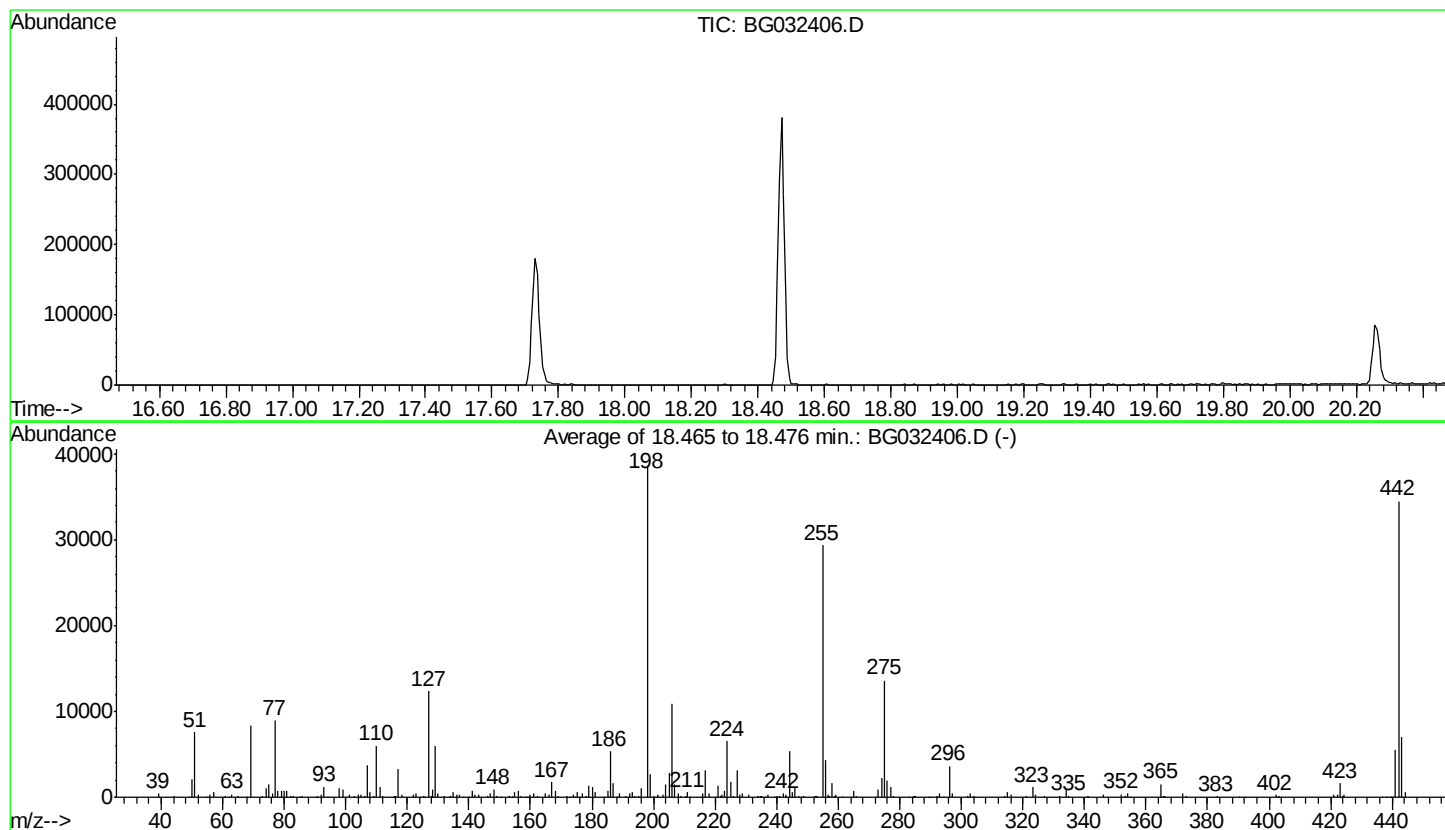

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	7571	PASS
68	69	0.00	2	0.6	53	PASS
69	198	0.00	100	21.5	8311	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.9	12316	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38616	PASS
199	198	5	9	7.2	2762	PASS
275	198	10	60	35.2	13595	PASS
365	198	1	100	3.9	1513	PASS
441	442	0.01	24	15.9	5482	PASS
442	198	50	100	89.4	34506	PASS
443	442	15	24	20.3	7008	PASS