


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG012918\
 Data File : BG032422.D
 Acq On : 29 Jan 2018 19:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

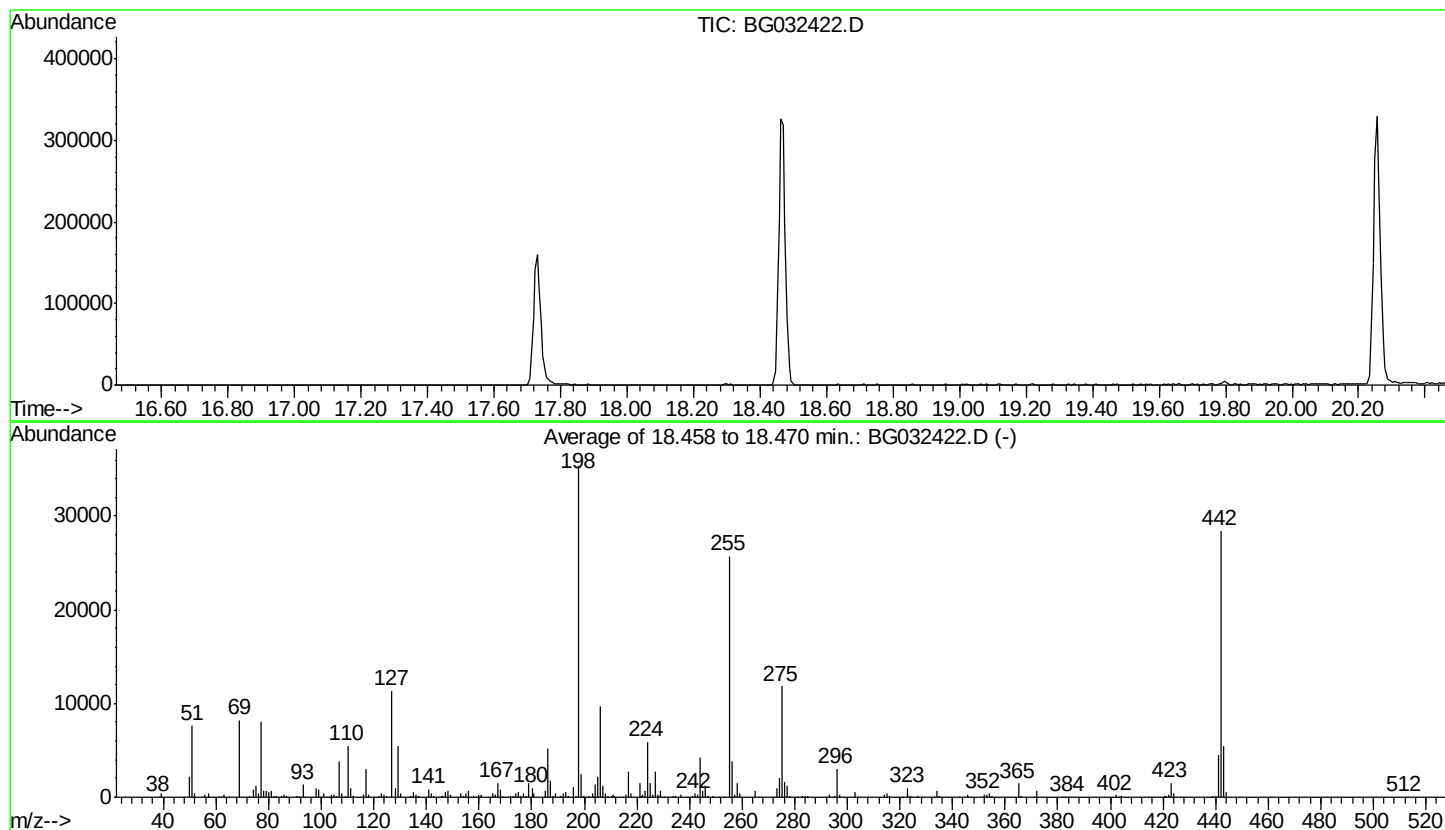

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	7635	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.3	8244	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	11341	PASS
197	198	0.00	2	0.3	118	PASS
198	198	100	100	100.0	35389	PASS
199	198	5	9	6.8	2410	PASS
275	198	10	60	33.5	11843	PASS
365	198	1	100	4.2	1483	PASS
441	442	0.01	24	16.1	4578	PASS
442	198	50	100	80.4	28455	PASS
443	442	15	24	19.1	5436	PASS