

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060473.D
 Acq On : 29 Jan 2024 22:22
 Operator : MA/JU
 Sample : PB158611BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS611

Quant Time: Jan 30 01:49:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 06:06:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	196877	20.000	ng/u1	0.00
20) Naphthalene-d8	10.729	136	840369	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.560	164	682939	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.309	188	1703089	20.000	ng/u1	0.00
79) Chrysene-d12	21.575	240	1490739	20.000	ng/u1	0.00
88) Perylene-d12	24.736	264	1612830	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.361	96	20096	5.115	ng/uL	0.00
4) Pyridine-d5	3.772	84	325100	26.158	ng/u1	0.00
7) Phenol-d5	7.092	99	454320	24.298	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.251	67	265977	22.637	ng/u1	0.00
11) 2-Chlorophenol-d4	7.456	132	302932	24.261	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	352152	22.864	ng/u1	0.00
21) Nitrobenzene-d5	9.090	128	156051	25.173	ng/u1	0.00
24) 2-Nitrophenol-d4	9.806	143	186357	25.730	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.347	165	404178	26.833	ng/u1	0.00
31) 4-Chloroaniline-d4	10.864	131	445509	22.546	ng/u1	0.00
46) Dimethylphthalate-d6	13.966	166	1320875	23.636	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	1548213	24.698	ng/u1	0.00
54) 4-Nitrophenol-d4	14.765	143	194187	24.261	ng/u1	0.00
60) Fluorene-d10	15.553	176	1228559	25.090	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.676	200	255677	24.244	ng/u1	0.00
73) Anthracene-d10	17.409	188	1983708	24.571	ng/u1	0.00
81) Pyrene-d10	19.701	212	2240963	25.082	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.519	264	2182098	25.791	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.396	88	46791	10.764	ng/uL	96
5) Pyridine	3.790	79	339735	26.887	ng/u1	96
6) Benzaldehyde	7.063	77	224841	31.635	ng/u1	94
8) Phenol	7.115	94	473802	24.242	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.345	93	362227	23.268	ng/u1	98
12) 2-Chlorophenol	7.491	128	322726	25.056	ng/u1	96
13) 2-Methylphenol	8.367	108	359501	23.802	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.449	45	486589	23.684	ng/u1	98
16) Acetophenone	8.743	105	578445	23.567	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.731	70	309460	23.381	ng/u1	96
18) 4-Methylphenol	8.696	108	390316	24.034	ng/u1	97
19) Hexachloroethane	9.001	117	129835	22.800	ng/u1	94
22) Nitrobenzene	9.131	77	432545	25.507	ng/u1	96
23) Isophorone	9.648	82	904611	24.605	ng/u1	99
25) 2-Nitrophenol	9.842	139	199081	27.040	ng/u1	98
26) 2,4-Dimethylphenol	9.895	107	326359	21.481	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.130	93	533993	25.514	ng/u1	99
29) 2,4-Dichlorophenol	10.376	162	393088	27.149	ng/u1	94
30) Naphthalene	10.776	128	1132459	24.974	ng/u1	97
32) 4-Chloroaniline	10.887	127	388551	20.042	ng/u1	98
33) Hexachlorobutadiene	11.058	225	302007	25.120	ng/u1	98
34) Caprolactam	11.645	113	88705	18.403	ng/u1	91
35) 4-Chloro-3-methylphenol	12.016	107	422495	29.105	ng/u1	98
36) 2-Methylnaphthalene	12.386	142	880493	27.622	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060473.D
 Acq On : 29 Jan 2024 22:22
 Operator : MA/JU
 Sample : PB158611BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS611

Quant Time: Jan 30 01:49:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 26 06:06:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.603	142	882489	27.391	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.750	216	636753	25.618	ng/ul	97
40) Hexachlorocyclopentadiene	12.732	237	300940	20.023	ng/ul	99
41) 2,4,6-Trichlorophenol	12.997	196	393109	25.945	ng/ul	97
42) 2,4,5-Trichlorophenol	13.067	196	406710	25.403	ng/ul	93
43) 1,1'-Biphenyl	13.396	154	1295322	25.604	ng/ul	99
44) 2-Chloronaphthalene	13.437	162	1091733	25.559	ng/ul	98
45) 2-Nitroaniline	13.643	65	282815	26.306	ng/ul	95
47) Dimethylphthalate	14.013	163	1373479	24.622	ng/ul	99
48) 2,6-Dinitrotoluene	14.137	165	277416	26.370	ng/ul	99
50) Acenaphthylene	14.283	152	1738567	25.139	ng/ul	98
51) 3-Nitroaniline	14.471	138	241046	27.258	ng/ul	98
52) Acenaphthene	14.624	153	1153415	25.003	ng/ul	99
53) 2,4-Dinitrophenol	14.677	184	126231	21.984	ng/ul	97
55) 4-Nitrophenol	14.783	109	138637	25.440	ng/ul	91
56) Dibenzofuran	14.959	168	1645792	25.271	ng/ul	97
57) 2,4-Dinitrotoluene	14.924	165	415489	26.952	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.188	232	390770	26.263	ng/ul#	97
59) Diethylphthalate	15.376	149	1329261	24.783	ng/ul	100
61) Fluorene	15.611	166	1341456	25.107	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.600	204	754997	25.600	ng/ul	97
63) 4-Nitroaniline	15.635	138	267180	30.840	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.688	198	268998	24.386	ng/ul#	92
67) N-Nitrosodiphenylamine	15.817	169	1178816	25.519	ng/ul	98
68) 4-Bromophenyl-phenylether	16.499	248	492623	24.898	ng/ul	97
69) Hexachlorobenzene	16.616	284	580272	25.283	ng/ul	99
70) Atrazine	16.763	200	391103	20.595	ng/ul	99
71) Pentachlorophenol	16.963	266	284555	22.511	ng/ul	95
72) Phenanthrene	17.350	178	2314653	25.850	ng/ul	99
74) Anthracene	17.444	178	2272431	24.905	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.361	216	651036	26.358	ng/ul	97
76) Pentachlorobenzene	14.883	250	653745	25.196	ng/ul	98
77) Carbazole	17.715	167	2044926	27.135	ng/ul	98
78) Di-n-butylphthalate	18.267	149	2305883	25.955	ng/ul	100
80) Fluoranthene	19.366	202	2535098	25.426	ng/ul	98
82) Pyrene	19.730	202	2603396	25.089	ng/ul	99
83) Butylbenzylphthalate	20.617	149	931940	25.197	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.475	252	924412	26.878	ng/ul	99
85) Benzo(a)anthracene	21.551	228	2661632	25.893	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.457	149	1382216	25.037	ng/ul	100
87) Chrysene	21.622	228	2540470	26.310	ng/ul	99
89) Di-n-octyl phthalate	22.644	149	2355446	27.367	ng/ul	100
90) Benzo(b)fluoranthene	23.731	252	2635366	26.332	ng/ul	100
91) Benzo(k)fluoranthene	23.796	252	2748553	26.893	ng/ul	99
93) Benzo(a)pyrene	24.589	252	2565099	26.642	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.338	276	3093200	26.208	ng/ul	99
95) Dibenzo(a,h)anthracene	28.396	278	2540476	26.383	ng/ul	99
96) Benzo(g,h,i)perylene	29.466	276	2488944	26.046	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 10.764 ng/uL
 RT: 3.396 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22




Instrument :
 BNA_G
 ClientSampleId :
 SLCS611


Tgt Ion: 88 Resp: 46791
 Ion Ratio Lower Upper
 88 100
 43 21.9 15.4 23.0
 58 69.1 57.8 86.8



#5
 Pyridine
 Concen: 26.887 ng/uL
 RT: 3.790 min Scan# 119
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22

Tgt Ion: 79 Resp: 339735
 Ion Ratio Lower Upper
 79 100
 52 66.6 55.8 83.6
 51 26.8 23.1 34.7









#6
Benzaldehyde
Concen: 31.635 ng/ul
RT: 7.063 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion: 77 Resp: 224841
Ion Ratio Lower Upper
77 100
105 100.1 73.1 109.7
106 91.4 71.1 106.7



#8
Phenol
Concen: 24.242 ng/ul
RT: 7.115 min Scan# 685
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion: 94 Resp: 473802
Ion Ratio Lower Upper
94 100
65 27.0 20.8 31.2
66 30.5 26.3 39.5









#10
 Bis(2-Chloroethyl)ether
 Concen: 23.268 ng/ul
 RT: 7.345 min Scan# 71
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22




Instrument :
 BNA_G
 ClientSampleId :
 SLCS611


Tgt Ion: 93 Resp: 362227
 Ion Ratio Lower Upper
 93 100
 63 77.2 61.4 92.0
 95 29.3 26.2 39.2

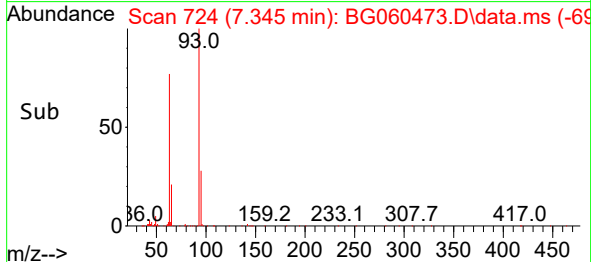

#12
 2-Chlorophenol
 Concen: 25.056 ng/ul
 RT: 7.491 min Scan# 749
 Delta R.T. 0.006 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22

Tgt Ion:128 Resp: 322726
 Ion Ratio Lower Upper
 128 100
 64 51.1 39.6 59.4
 130 33.3 23.8 35.8









#13
2-Methylphenol
Concen: 23.802 ng/ul
RT: 8.367 min Scan# 898
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:108 Resp: 359501
Ion Ratio Lower Upper
108 100
107 89.5 68.9 103.3

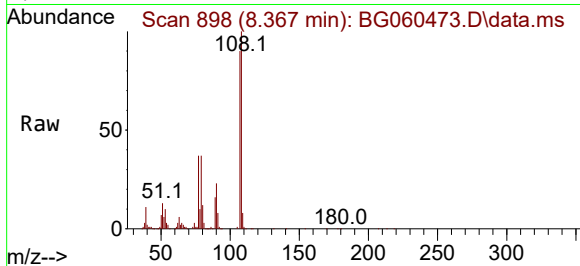

#14
2,2'-oxybis(1-Chloropropane)
Concen: 23.684 ng/ul
RT: 8.449 min Scan# 912
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion: 45 Resp: 486589
Ion Ratio Lower Upper
45 100
77 18.4 14.2 21.4
79 12.5 10.9 16.3




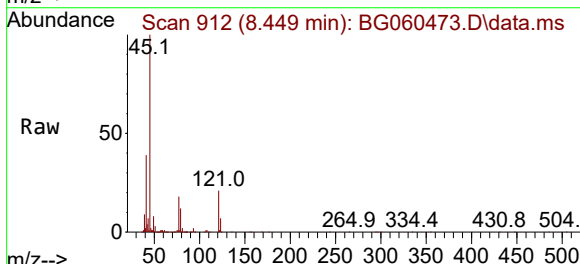




#16
Acetophenone
Concen: 23.567 ng/ul
RT: 8.743 min Scan# 90
Delta R.T. -0.005 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:105 Resp: 578445
Ion Ratio Lower Upper
105 100
77 74.6 59.1 88.7
51 20.3 18.2 27.2



#17
N-Nitroso-di-n-propylamine
Concen: 23.381 ng/ul
RT: 8.731 min Scan# 960
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion: 70 Resp: 309460
Ion Ratio Lower Upper
70 100
42 45.4 33.8 50.8
101 7.3 6.9 10.3
130 15.6 12.6 18.8



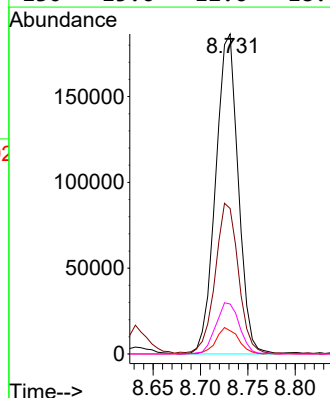





#18
4-Methylphenol
Concen: 24.034 ng/ul
RT: 8.696 min Scan# 91
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:108 Resp: 390316
Ion Ratio Lower Upper
108 100
107 113.7 88.2 132.4

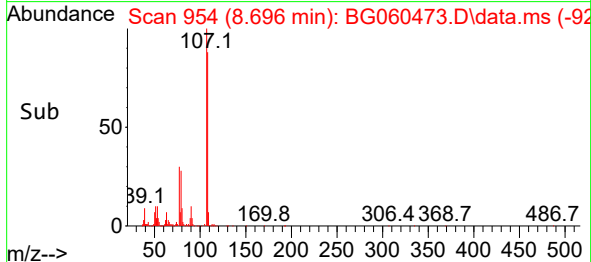

#19
Hexachloroethane
Concen: 22.800 ng/ul
RT: 9.001 min Scan# 1006
Delta R.T. -0.005 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:117 Resp: 129835
Ion Ratio Lower Upper
117 100
201 147.2 110.8 166.2
199 91.5 75.7 113.5




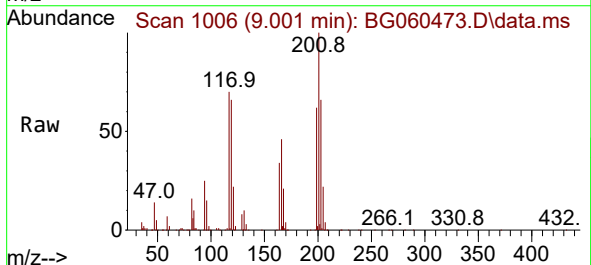




#22
Nitrobenzene
Concen: 25.507 ng/ul
RT: 9.131 min Scan# 1028
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion: 77 Resp: 432545
Ion Ratio Lower Upper
77 100
123 40.8 35.0 52.6
65 12.5 10.5 15.7



#23
Isophorone
Concen: 24.605 ng/ul
RT: 9.648 min Scan# 1116
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion: 82 Resp: 904611
Ion Ratio Lower Upper
82 100
95 6.0 4.9 7.3
138 16.1 12.5 18.7









#25
2-Nitrophenol
Concen: 27.040 ng/ul
RT: 9.842 min Scan# 1149
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:139 Resp: 199081
Ion Ratio Lower Upper
139 100
65 51.9 41.0 61.4
109 24.5 21.4 32.0



#26
2,4-Dimethylphenol
Concen: 21.481 ng/ul
RT: 9.895 min Scan# 1158
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:107 Resp: 326359
Ion Ratio Lower Upper
107 100
121 49.3 39.2 58.8
122 85.5 68.6 102.8




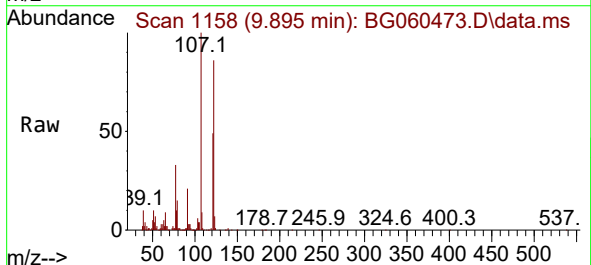




#27
 Bis(2-Chloroethoxy)methane
 Concen: 25.514 ng/ul
 RT: 10.130 min Scan# 1199
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22




Instrument :
 BNA_G
 ClientSampleId :
 SLCS611


Tgt Ion: 93 Resp: 533993
 Ion Ratio Lower Upper
 93 100
 95 32.7 25.5 38.3
 123 8.4 7.0 10.6



#29
 2,4-Dichlorophenol
 Concen: 27.149 ng/ul
 RT: 10.376 min Scan# 1240
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22

Tgt Ion:162 Resp: 393088
 Ion Ratio Lower Upper
 162 100
 164 63.4 55.2 82.8
 98 31.7 27.0 40.6



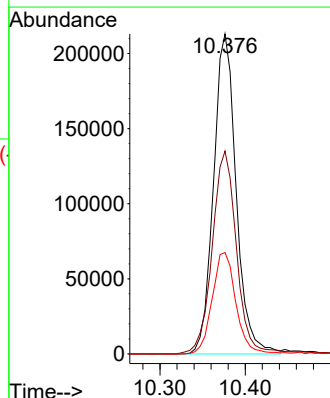





#30
Naphthalene
Concen: 24.974 ng/ul
RT: 10.776 min Scan# 11
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:128 Resp: 1132459
Ion Ratio Lower Upper
128 100
129 11.4 8.5 12.7
127 13.5 9.5 14.3



#32
4-Chloroaniline
Concen: 20.042 ng/ul
RT: 10.887 min Scan# 1327
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:127 Resp: 388551
Ion Ratio Lower Upper
127 100
129 33.0 27.2 40.8





#33

Hexachlorobutadiene

Concen: 25.120 ng/ul

RT: 11.058 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:225 Resp: 302007

Ion Ratio Lower Upper

225 100

223 63.4 52.0 78.0

227 64.7 52.8 79.2

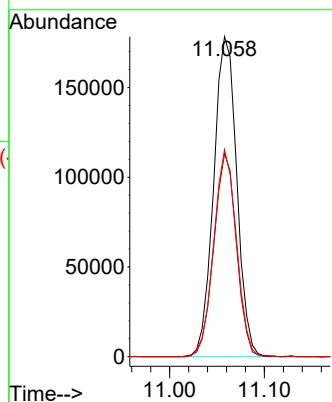

#34

Caprolactam

Concen: 18.403 ng/ul

RT: 11.645 min Scan# 1456

Delta R.T. -0.011 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:113 Resp: 88705


Ion Ratio Lower Upper

113 100

55 180.3 154.2 231.4

56 136.0 100.6 150.8









#35
4-Chloro-3-methylphenol
Concen: 29.105 ng/ul
RT: 12.016 min Scan# 1519
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:107 Resp: 422495
Ion Ratio Lower Upper
107 100
144 27.6 21.4 32.2
142 81.8 64.1 96.1



#36
2-Methylnaphthalene
Concen: 27.622 ng/ul
RT: 12.386 min Scan# 1582
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:142 Resp: 880493
Ion Ratio Lower Upper
142 100
141 92.3 72.6 108.8

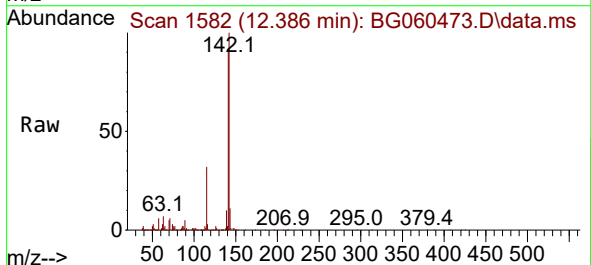



#37

1-Methylnaphthalene

Concen: 27.391 ng/ul

RT: 12.603 min Scan# 1

Delta R.T. -0.005 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:142 Resp: 882489

Ion Ratio Lower Upper

142 100

141 93.0 73.6 110.4

116 3.2 2.3 3.5

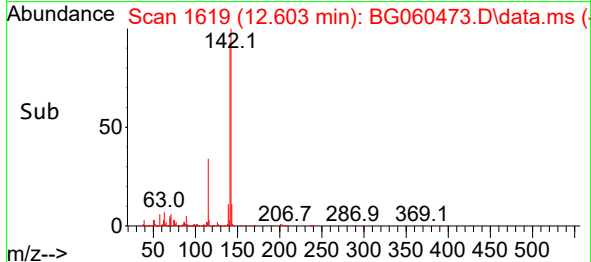

#39

1,2,4,5-Tetrachlorobenzene

Concen: 25.618 ng/ul

RT: 12.750 min Scan# 1644

Delta R.T. -0.005 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Tgt Ion:216 Resp: 636753




Ion Ratio Lower Upper


216 100

214 75.9 63.0 94.4

179 17.3 15.2 22.8

108 10.7 9.2 13.8


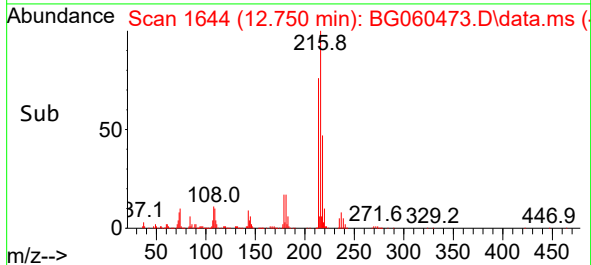






#40
Hexachlorocyclopentadiene
Concen: 20.023 ng/ul
RT: 12.732 min Scan# 1641
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:237 Resp: 300940
Ion Ratio Lower Upper
237 100
235 61.0 49.4 74.0
272 12.1 10.0 15.0

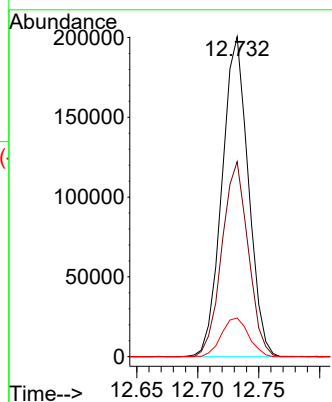

#41
2,4,6-Trichlorophenol
Concen: 25.945 ng/ul
RT: 12.997 min Scan# 1686
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:196 Resp: 393109
Ion Ratio Lower Upper
196 100
198 92.6 76.3 114.5
200 32.5 24.4 36.6









#42
 2,4,5-Trichlorophenol
 Concen: 25.403 ng/ul
 RT: 13.067 min Scan# 1699
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22




Instrument :
 BNA_G
 ClientSampleId :
 SLCS611


Tgt Ion:196 Resp: 406710
 Ion Ratio Lower Upper
 196 100
 198 102.4 75.7 113.5
 200 33.2 24.9 37.3

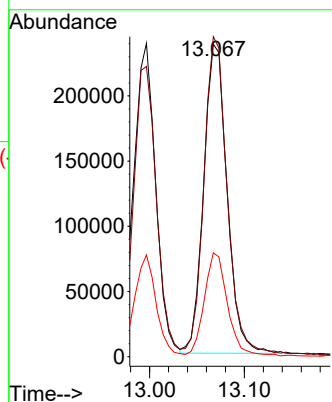

#43
 1,1'-Biphenyl
 Concen: 25.604 ng/ul
 RT: 13.396 min Scan# 1754
 Delta R.T. 0.001 min
 Lab File: BG060473.D
 Acq: 29 Jan 2024 22:22

Tgt Ion:154 Resp: 1295322
 Ion Ratio Lower Upper
 154 100
 153 40.5 31.8 47.8
 76 13.5 10.4 15.6









#44
2-Chloronaphthalene
Concen: 25.559 ng/ul
RT: 13.437 min Scan# 1761
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:162 Resp: 1091733
Ion Ratio Lower Upper
162 100
164 33.4 27.7 41.5
127 29.4 24.5 36.7

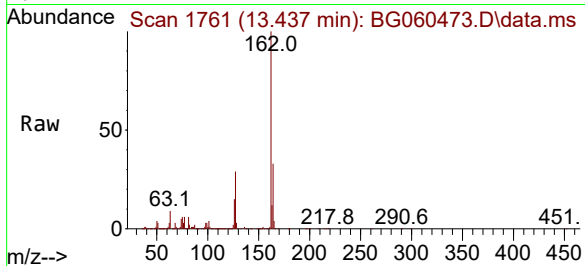

#45
2-Nitroaniline
Concen: 26.306 ng/ul
RT: 13.643 min Scan# 1796
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion: 65 Resp: 282815
Ion Ratio Lower Upper
65 100
92 74.8 57.7 86.5
138 102.9 87.0 130.6




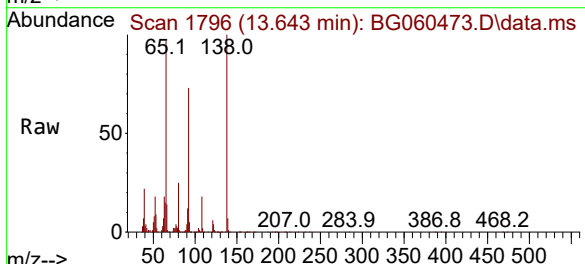




#47
Dimethylphthalate
Concen: 24.622 ng/ul
RT: 14.013 min Scan# 1859
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:163 Resp: 1373479
Ion Ratio Lower Upper
163 100
194 3.3 2.6 3.8
164 10.1 8.4 12.6



#48
2,6-Dinitrotoluene
Concen: 26.370 ng/ul
RT: 14.137 min Scan# 1880
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:165 Resp: 277416
Ion Ratio Lower Upper
165 100
89 49.7 40.2 60.2
121 17.9 15.0 22.6









#50
Acenaphthylene
Concen: 25.139 ng/ul
RT: 14.283 min Scan# 1906
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:152 Resp: 1738567
Ion Ratio Lower Upper
152 100
151 19.5 16.3 24.5
153 13.3 10.4 15.6

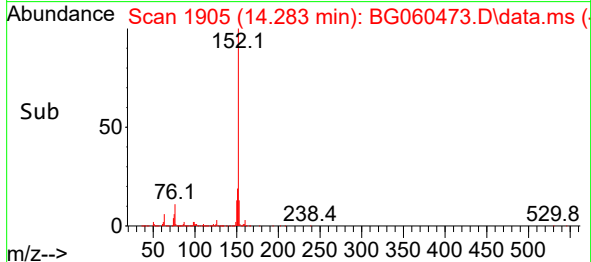

#51
3-Nitroaniline
Concen: 27.258 ng/ul
RT: 14.471 min Scan# 1937
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:138 Resp: 241046
Ion Ratio Lower Upper
138 100
108 10.0 9.5 14.3
92 125.8 98.9 148.3









#52
Acenaphthene
Concen: 25.003 ng/ul
RT: 14.624 min Scan# 1963
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:153 Resp: 1153415
Ion Ratio Lower Upper
153 100
152 45.8 37.0 55.6
154 87.0 70.0 105.0

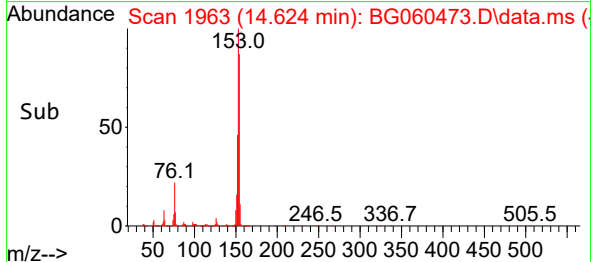

#53
2,4-Dinitrophenol
Concen: 21.984 ng/ul
RT: 14.677 min Scan# 1972
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:184 Resp: 126231
Ion Ratio Lower Upper
184 100
63 48.7 39.2 58.8
154 46.9 40.3 60.5



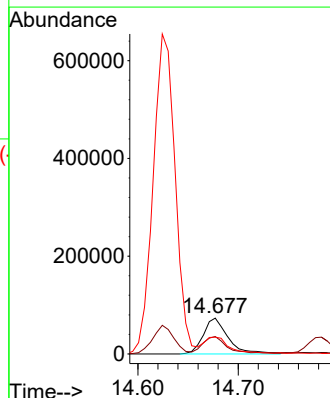





#55
4-Nitrophenol
Concen: 25.440 ng/ul
RT: 14.783 min Scan# 1989
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:109 Resp: 138637
Ion Ratio Lower Upper
109 100
139 147.4 124.5 186.7
65 154.2 112.4 168.6

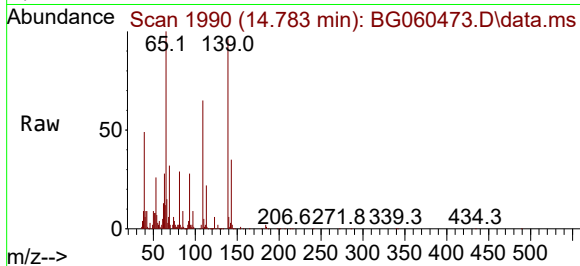

#56
Dibenzofuran
Concen: 25.271 ng/ul
RT: 14.959 min Scan# 2020
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:168 Resp: 1645792
Ion Ratio Lower Upper
168 100
139 28.7 21.6 32.4

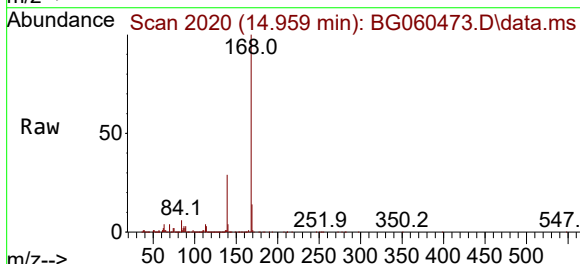



#57

2,4-Dinitrotoluene

Concen: 26.952 ng/ul

RT: 14.924 min Scan# 2015

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:165 Resp: 415489

Ion Ratio Lower Upper

165 100

63 34.7 29.9 44.9

182 1.8 1.8 2.6

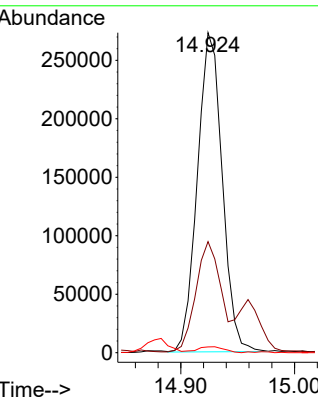

#58

2,3,4,6-Tetrachlorophenol

Concen: 26.263 ng/ul

RT: 15.188 min Scan# 2059

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Tgt Ion:232 Resp: 390770




Ion Ratio Lower Upper


232 100

131 28.0 23.4 35.0

130 1.4 0.8 1.2#

166 27.4 20.0 30.0



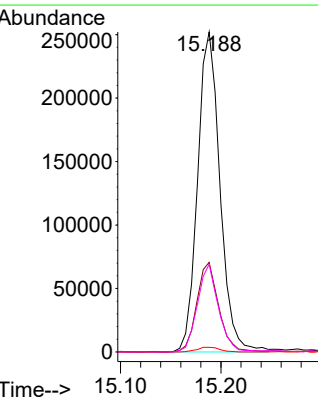
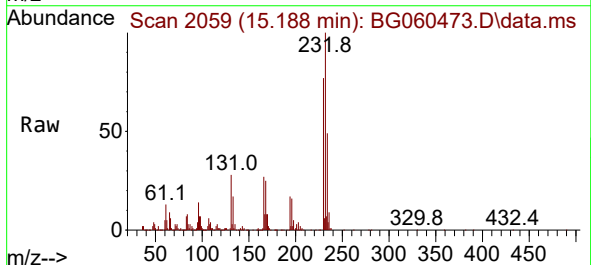




#59
Diethylphthalate
Concen: 24.783 ng/ul
RT: 15.376 min Scan# 2091
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:149 Resp: 1329261
Ion Ratio Lower Upper
149 100
177 24.2 19.4 29.0
150 11.8 9.8 14.8



#61
Fluorene
Concen: 25.107 ng/ul
RT: 15.611 min Scan# 2131
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:166 Resp: 1341456
Ion Ratio Lower Upper
166 100
165 101.5 81.0 121.6
167 14.3 11.3 16.9









#62
4-Chlorophenyl-phenylether
Concen: 25.600 ng/ul
RT: 15.600 min Scan# 2130
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:204 Resp: 754997
Ion Ratio Lower Upper
204 100
206 31.7 27.5 41.3
141 41.1 33.4 50.0



#63
4-Nitroaniline
Concen: 30.840 ng/ul
RT: 15.635 min Scan# 2135
Delta R.T. 0.006 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:138 Resp: 267180
Ion Ratio Lower Upper
138 100
92 55.5 45.5 68.3
108 65.7 51.8 77.6









#66
4,6-Dinitro-2-methylphenol
Concen: 24.386 ng/ul
RT: 15.688 min Scan# 2144
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:198 Resp: 268998
Ion Ratio Lower Upper
198 100
182 3.5 4.1 6.1#
77 20.0 13.0 19.6#



#67
N-Nitrosodiphenylamine
Concen: 25.519 ng/ul
RT: 15.817 min Scan# 2166
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:169 Resp: 1178816
Ion Ratio Lower Upper
169 100
168 67.4 55.4 83.0
167 36.9 31.0 46.4







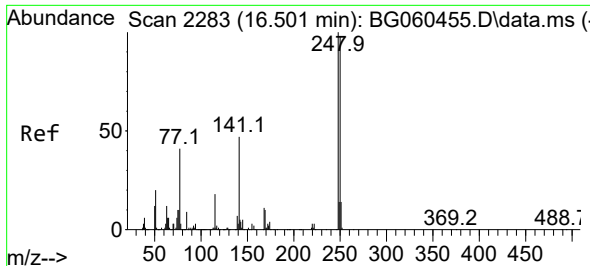

#68
4-Bromophenyl-phenylether
Concen: 24.898 ng/ul
RT: 16.499 min Scan# 21
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:248 Resp: 492623
Ion Ratio Lower Upper
248 100
250 99.1 77.3 115.9
141 47.3 36.5 54.7

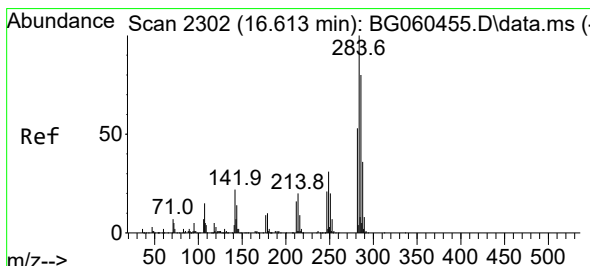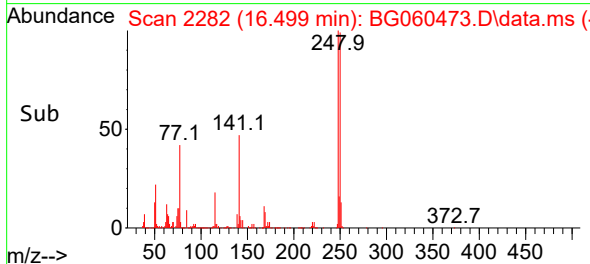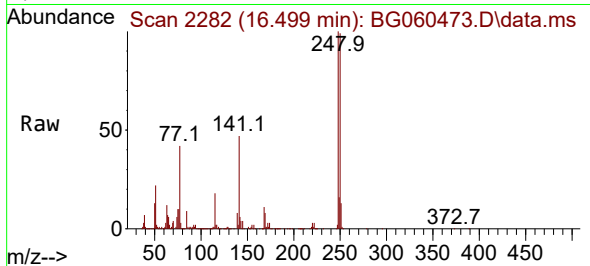

#69
Hexachlorobenzene
Concen: 25.283 ng/ul
RT: 16.616 min Scan# 2302
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:284 Resp: 580272
Ion Ratio Lower Upper
284 100
142 20.5 17.1 25.7
249 30.3 24.1 36.1

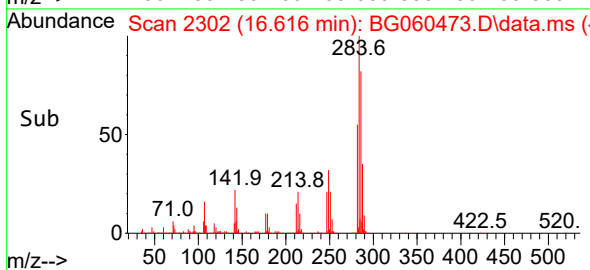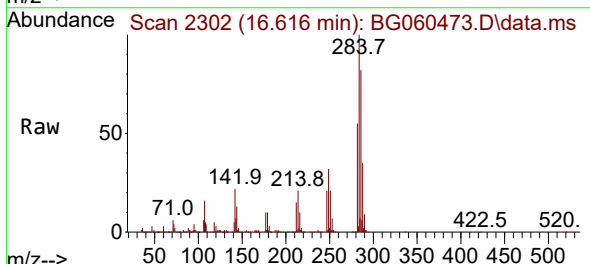



#70

Atrazine

Concen: 20.595 ng/ul

RT: 16.763 min Scan# 21

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:200 Resp: 391103

Ion Ratio Lower Upper

200 100

173 24.9 20.3 30.5

215 45.6 36.3 54.5



#71

Pentachlorophenol

Concen: 22.511 ng/ul

RT: 16.963 min Scan# 2361

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:266 Resp: 284555


Ion Ratio Lower Upper

266 100

264 62.2 47.0 70.6

268 63.9 48.2 72.2









#72
Phenanthrene
Concen: 25.850 ng/ul
RT: 17.350 min Scan# 2428
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:178 Resp: 2314653
Ion Ratio Lower Upper
178 100
179 15.5 12.7 19.1
176 19.3 15.7 23.5

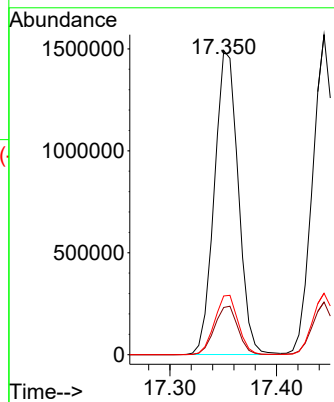

#74
Anthracene
Concen: 24.905 ng/ul
RT: 17.444 min Scan# 2443
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:178 Resp: 2272431
Ion Ratio Lower Upper
178 100
179 16.5 12.2 18.2
176 19.2 15.5 23.3

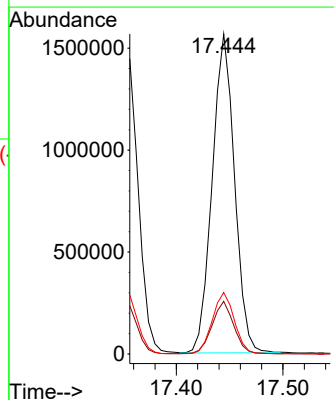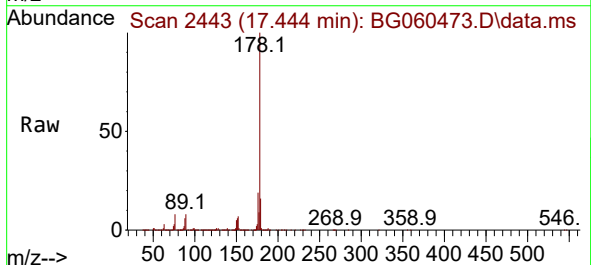



#75

1,2,3,4-Tetrachlorobenzene

Concen: 26.358 ng/uL

RT: 13.361 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:216 Resp: 651036

Ion Ratio Lower Upper

216 100

214 74.7 63.0 94.4

218 48.8 39.8 59.6

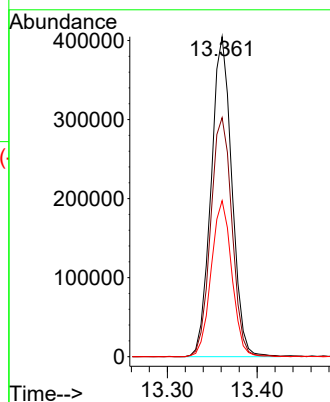

#76

Pentachlorobenzene

Concen: 25.196 ng/uL

RT: 14.883 min Scan# 2007

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:250 Resp: 653745


Ion Ratio Lower Upper

250 100

248 61.2 49.8 74.6

252 63.9 52.6 79.0





#77

Carbazole

Concen: 27.135 ng/ul

RT: 17.715 min Scan# 2490

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:167 Resp: 2044926

Ion Ratio Lower Upper

167 100

166 23.3 17.6 26.4

139 10.2 8.0 12.0

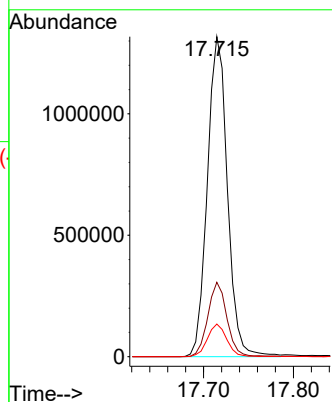

#78

Di-n-butylphthalate

Concen: 25.955 ng/ul

RT: 18.267 min Scan# 2583

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:149 Resp: 2305883


Ion Ratio Lower Upper

149 100

150 9.6 7.7 11.5

104 4.5 3.4 5.0









#80
Fluoranthene
Concen: 25.426 ng/ul
RT: 19.366 min Scan# 21
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22




Instrument :
BNA_G
ClientSampleId :
SLCS611


Tgt Ion:202 Resp: 2535098
Ion Ratio Lower Upper
202 100
101 10.9 7.9 11.9
100 8.4 6.4 9.6



#82
Pyrene
Concen: 25.089 ng/ul
RT: 19.730 min Scan# 2832
Delta R.T. 0.001 min
Lab File: BG060473.D
Acq: 29 Jan 2024 22:22

Tgt Ion:202 Resp: 2603396
Ion Ratio Lower Upper
202 100
101 12.2 10.0 15.0
100 10.8 8.4 12.6





#83

Butylbenzylphthalate

Concen: 25.197 ng/ul

RT: 20.617 min Scan# 2983

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:149 Resp: 931940

Ion Ratio Lower Upper

149 100

91 68.5 56.3 84.5

206 22.3 18.1 27.1

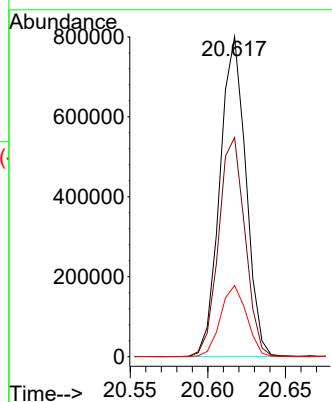

#84

3,3'-Dichlorobenzidine

Concen: 26.878 ng/ul

RT: 21.475 min Scan# 3129

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:252 Resp: 924412


Ion Ratio Lower Upper

252 100

254 65.3 52.8 79.2

126 6.5 6.2 9.4





#85

Benzo(a)anthracene

Concen: 25.893 ng/ul

RT: 21.551 min Scan# 3143

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:228 Resp: 2661632

Ion Ratio Lower Upper

228 100

229 20.3 16.2 24.2

226 28.8 22.1 33.1



#86

Bis(2-ethylhexyl)phthalate

Concen: 25.037 ng/ul

RT: 21.457 min Scan# 3126

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:149 Resp: 1382216


Ion Ratio Lower Upper

149 100

167 27.9 22.2 33.4

279 3.7 3.0 4.4

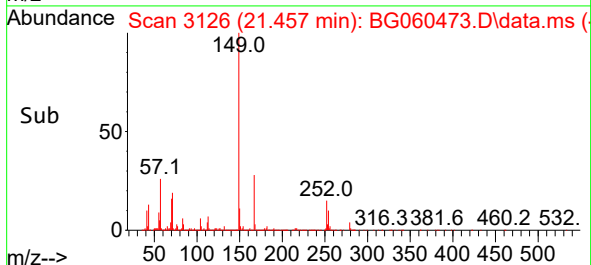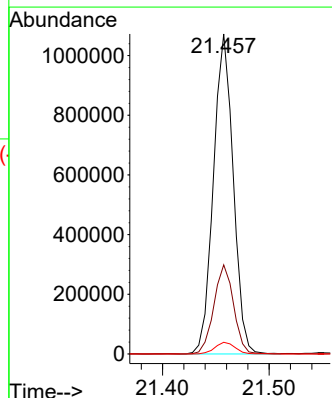

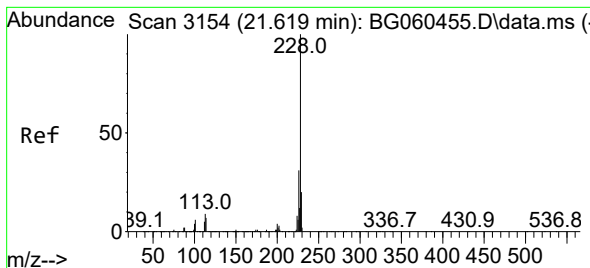

#87

Chrysene

Concen: 26.310 ng/ul

RT: 21.622 min Scan# 3154

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:228 Resp: 2540470

Ion Ratio Lower Upper

228 100

226 31.7 25.0 37.6

229 20.4 16.2 24.4

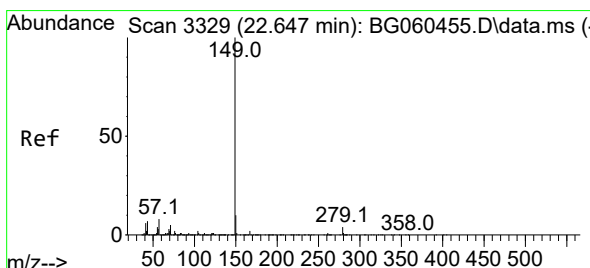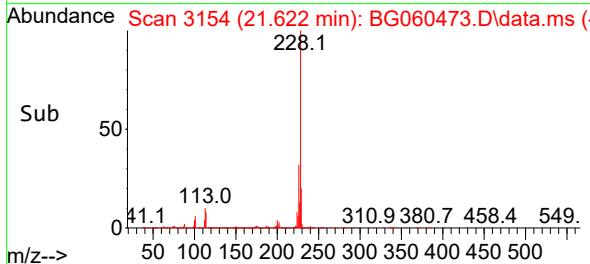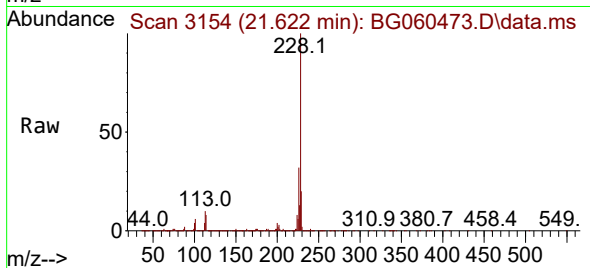

#89

Di-n-octyl phthalate

Concen: 27.367 ng/ul




RT: 22.644 min Scan# 3328


Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Tgt Ion:149 Resp: 2355446

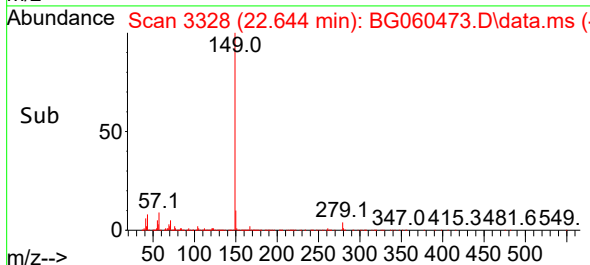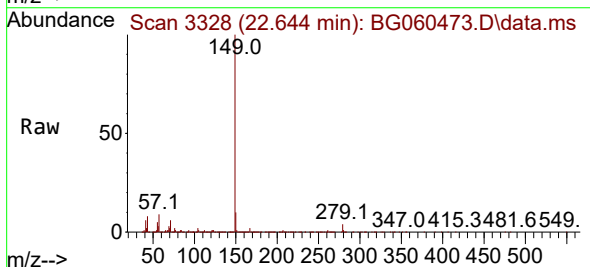



#90

Benzo(b)fluoranthene

Concen: 26.332 ng/ul

RT: 23.731 min Scan# 3

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:252 Resp: 2635366

Ion Ratio Lower Upper

252 100

253 22.5 18.0 27.0

125 8.2 6.2 9.4

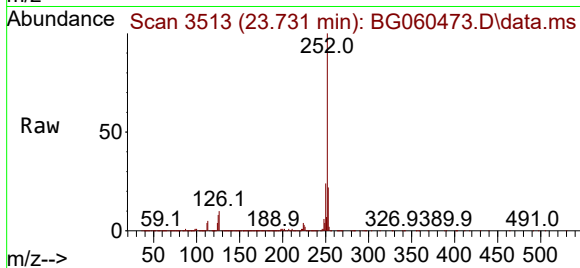

#91

Benzo(k)fluoranthene

Concen: 26.893 ng/ul

RT: 23.796 min Scan# 3524

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:252 Resp: 2748553


Ion Ratio Lower Upper

252 100

253 23.2 17.8 26.8

125 8.4 6.8 10.2

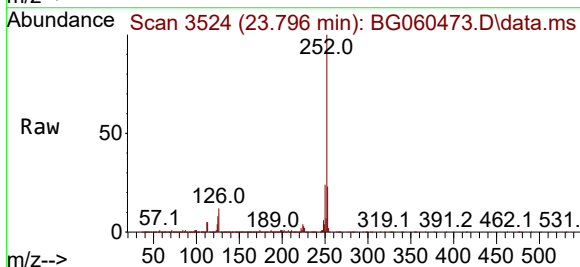



#93

Benzo(a)pyrene

Concen: 26.642 ng/ul

RT: 24.589 min Scan# 3

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:252 Resp: 2565099

Ion Ratio Lower Upper

252 100

253 22.3 18.3 27.5

125 9.5 7.4 11.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 26.208 ng/ul

RT: 28.338 min Scan# 4297

Delta R.T. 0.001 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22




Tgt Ion:276 Resp: 3093200


Ion Ratio Lower Upper

276 100

138 16.2 13.0 19.4

277 24.1 18.9 28.3





#95

Dibenzo(a,h)anthracene

Concen: 26.383 ng/ul

RT: 28.396 min Scan# 41

Delta R.T. 0.006 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Instrument :

BNA_G

ClientSampleId :

SLCS611





Tgt Ion:278 Resp: 2540476

Ion Ratio Lower Upper

278 100

139 12.7 9.9 14.9

279 23.8 18.9 28.3



#96

Benzo(g,h,i)perylene

Concen: 26.046 ng/ul

RT: 29.466 min Scan# 4489

Delta R.T. 0.018 min

Lab File: BG060473.D

Acq: 29 Jan 2024 22:22

Tgt Ion:276 Resp: 2488944

Ion Ratio Lower Upper

276 100

138 17.4 14.6 22.0

277 23.1 18.3 27.5

