

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060462.D
Acq On : 29 Jan 2024 14:57
Operator : MA/JU
Sample : P1239-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M

Title : SVOA CALIBRATION

Signal : TIC: BG060462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	39	47	51	rVV4	34305	63654	0.81%	0.102%
2	3.775	113	117	131	rBV	136431	254444	3.25%	0.408%
3	4.110	170	174	182	rVB5	11811	20642	0.26%	0.033%
4	7.089	673	681	690	rBV	116537	235810	3.01%	0.378%
5	7.248	701	708	720	rBV	544843	977125	12.49%	1.568%
6	7.453	737	743	756	rBV	448273	821789	10.51%	1.318%
7	7.923	816	823	835	rBV	575901	1057723	13.52%	1.697%
8	8.628	935	943	959	rBV2	391416	738763	9.45%	1.185%
9	9.087	1014	1021	1032	rBV	636471	1170998	14.97%	1.879%
10	9.486	1087	1089	1095	rVB4	7982	10758	0.14%	0.017%
11	9.809	1135	1144	1157	rBV	468778	903513	11.55%	1.449%
12	10.350	1228	1236	1247	rBV	757886	1435069	18.35%	2.302%
13	10.726	1293	1300	1314	rBV	892379	1633936	20.89%	2.621%
14	10.861	1316	1323	1337	rBV	616733	1240239	15.86%	1.990%
15	12.248	1551	1559	1564	rBV4	17826	34832	0.45%	0.056%
16	12.312	1566	1570	1574	rBV2	12544	20293	0.26%	0.033%
17	13.446	1759	1763	1770	rVB4	24062	36523	0.47%	0.059%
18	13.963	1845	1851	1862	rBV	1983113	2862840	36.60%	4.593%
19	14.257	1890	1901	1916	rBV	2251777	3592105	45.93%	5.763%
20	14.563	1946	1953	1961	rBV	1918388	2941697	37.61%	4.719%
21	14.768	1983	1988	1995	rBV2	76043	158053	2.02%	0.254%
22	15.556	2113	2122	2135	rBV	3265679	4906850	62.74%	7.872%
23	15.667	2135	2141	2154	rVV	789066	1220312	15.60%	1.958%
24	15.791	2160	2162	2168	rVB7	17225	24428	0.31%	0.039%
25	16.120	2216	2218	2222	rVB5	6991	9052	0.12%	0.015%
26	16.255	2238	2241	2245	rVB6	8746	14377	0.18%	0.023%
27	16.337	2252	2255	2261	rVB5	16957	23560	0.30%	0.038%
28	17.095	2381	2384	2386	rBV4	7786	8173	0.10%	0.013%
29	17.312	2412	2421	2429	rBV	2400361	3746159	47.90%	6.010%
30	17.412	2429	2438	2449	rVV	3849427	6117723	78.22%	9.814%
31	17.970	2529	2533	2535	rBV4	7677	10038	0.13%	0.016%
32	18.200	2568	2572	2577	rBV6	21540	38201	0.49%	0.061%
33	18.429	2608	2611	2614	rBV5	5886	9057	0.12%	0.015%
34	18.617	2640	2643	2646	rVB5	11526	13081	0.17%	0.021%
35	19.269	2749	2754	2761	rBV4	65652	110741	1.42%	0.178%
36	19.334	2761	2765	2769	rVV2	63015	85491	1.09%	0.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060462.D
 Acq On : 29 Jan 2024 14:57
 Operator : MA/JU
 Sample : P1239-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	19.381	2771	2773	2779	rVB7	17324	21276	0.27%	0.034%
38	19.616	2810	2813	2818	rVB5	35752	34061	0.44%	0.055%
39	19.704	2821	2828	2838	rBV	5331896	7742970	99.00%	12.422%
40	20.661	2988	2991	2994	rBV5	28808	38706	0.49%	0.062%
41	20.708	2997	2999	3000	rBV2	16204	11091	0.14%	0.018%
42	21.220	3082	3086	3091	rBV3	87865	149331	1.91%	0.240%
43	21.455	3122	3126	3131	rBV	66358	95890	1.23%	0.154%
44	21.572	3139	3146	3159	rBV2	2518455	4213185	53.87%	6.759%
45	22.348	3276	3278	3282	rVB4	38477	44862	0.57%	0.072%
46	22.500	3302	3304	3305	rBV2	20416	11382	0.15%	0.018%
47	23.023	3390	3393	3398	rVB3	62617	103869	1.33%	0.167%
48	23.211	3423	3425	3432	rVB6	45068	63928	0.82%	0.103%
49	23.811	3523	3527	3534	rVB2	92329	179129	2.29%	0.287%
50	24.522	3637	3648	3664	rBV2	2745830	7821236	100.00%	12.547%
51	24.739	3674	3685	3702	rVB2	1636826	4753015	60.77%	7.625%
52	25.844	3866	3873	3880	rBV4	92058	232345	2.97%	0.373%
53	27.095	4084	4086	4087	rBV2	14495	9015	0.12%	0.014%
54	27.171	4092	4099	4107	rVB4	75042	245241	3.14%	0.393%
55	30.039	4585	4587	4590	rBV3	15656	15825	0.20%	0.025%




Sum of corrected areas: 62334406

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060462.D
Acq On : 29 Jan 2024 14:57
Operator : MA/JU
Sample : P1239-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

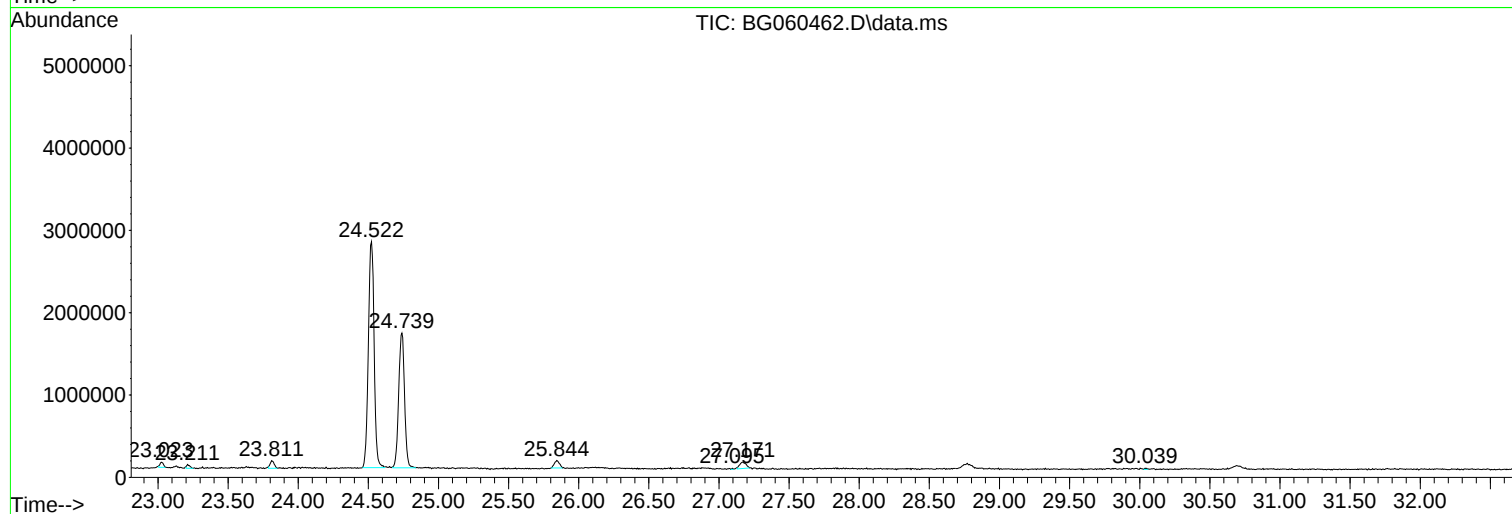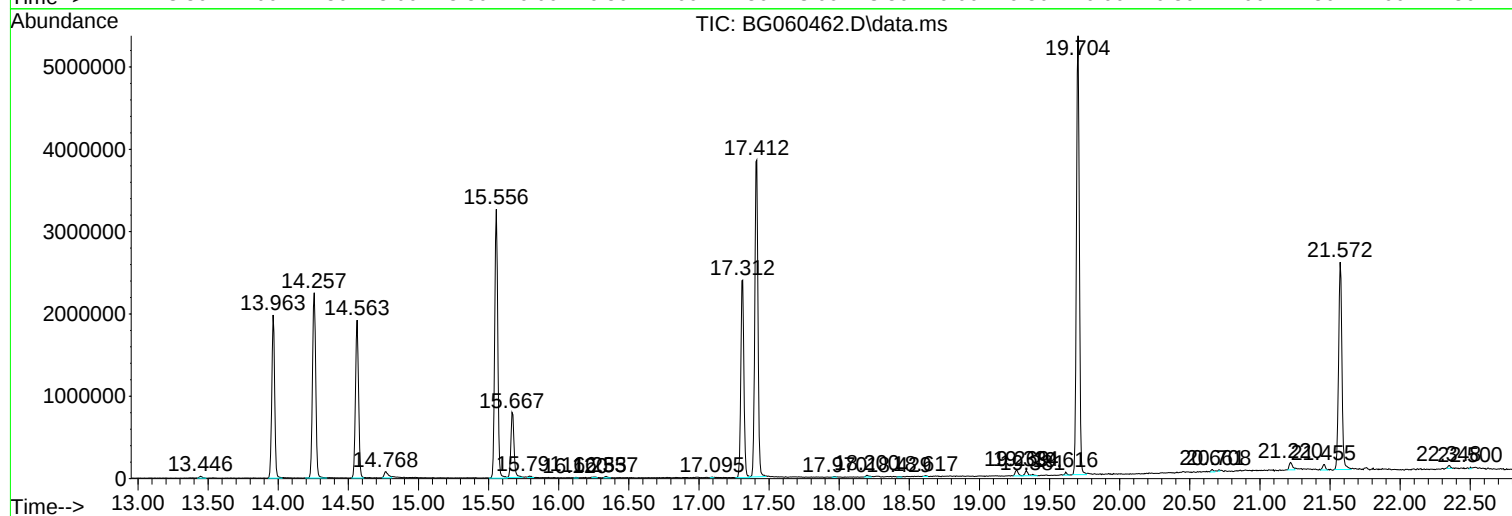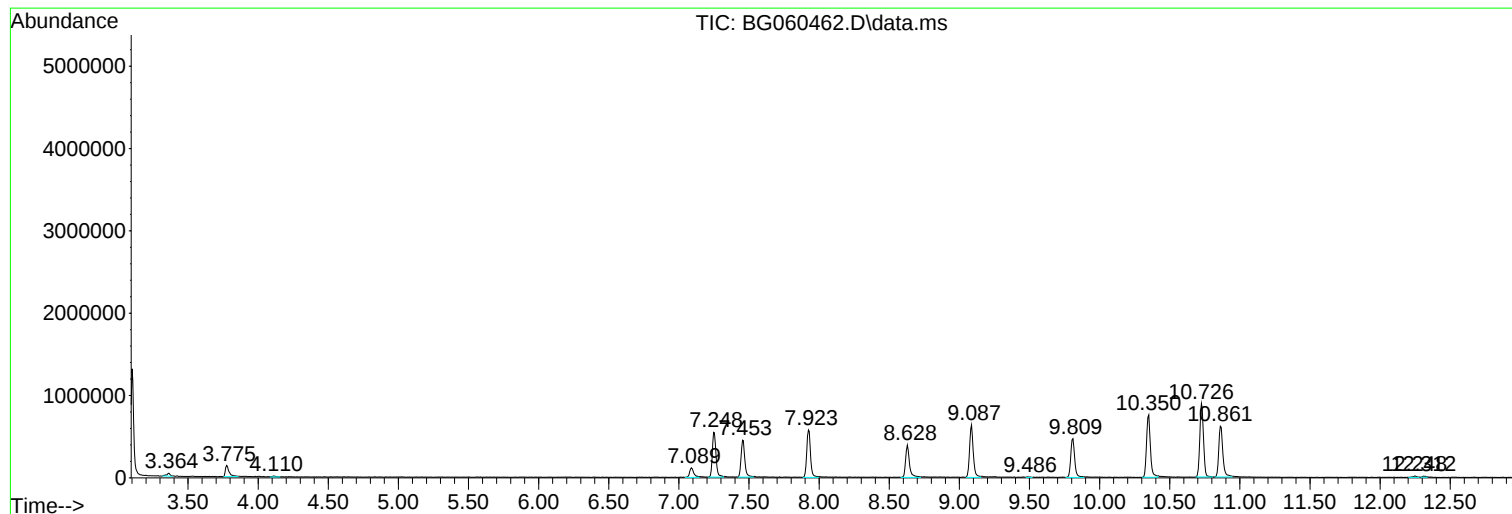

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060462.D
Acq On : 29 Jan 2024 14:57
Operator : MA/JU
Sample : P1239-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060462.D
Acq On : 29 Jan 2024 14:57
Operator : MA/JU
Sample : P1239-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------