

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060465.D
 Acq On : 29 Jan 2024 16:59
 Operator : MA/JU
 Sample : PB158661BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	42	47	51	rBV	47855	69650	1.02%	0.110%
2	3.769	112	116	130	rBV	601346	1007495	14.73%	1.595%
3	4.110	171	174	178	rVV3	9420	14429	0.21%	0.023%
4	7.089	674	681	690	rBV	609303	1107312	16.18%	1.753%
5	7.248	702	708	722	rBV	581237	1011798	14.79%	1.602%
6	7.453	735	743	756	rBV	650078	1143111	16.71%	1.810%
7	7.923	816	823	836	rBV	574843	1041376	15.22%	1.649%
8	8.628	934	943	958	rBV	807105	1460191	21.34%	2.312%
9	9.087	1013	1021	1036	rBV	631325	1163967	17.01%	1.843%
10	9.809	1137	1144	1152	rBV	507386	933236	13.64%	1.478%
11	10.344	1227	1235	1248	rBV	840001	1612848	23.57%	2.554%
12	10.726	1292	1300	1312	rBV	919660	1654768	24.19%	2.620%
13	10.861	1315	1323	1339	rBV	800910	1576837	23.05%	2.497%
14	12.318	1565	1571	1582	rBV3	14563	33265	0.49%	0.053%
15	13.446	1757	1763	1770	rVB5	19079	31192	0.46%	0.049%
16	13.963	1844	1851	1861	rBV	1924792	2725583	39.84%	4.316%
17	14.257	1893	1901	1918	rBV	2203975	3548838	51.87%	5.620%
18	14.563	1945	1953	1964	rBV	1830675	2841928	41.54%	4.500%
19	14.762	1981	1987	2006	rBV	535343	1053030	15.39%	1.668%
20	14.886	2006	2008	2013	rVB5	8238	12651	0.18%	0.020%
21	15.103	2042	2045	2048	rBV5	5335	8232	0.12%	0.013%
22	15.556	2115	2122	2134	rBV	3077585	4662316	68.14%	7.383%
23	15.667	2136	2141	2151	rBV	668538	1036783	15.15%	1.642%
24	15.796	2159	2163	2166	rVB4	14467	21803	0.32%	0.035%
25	16.337	2250	2255	2261	rBV3	9991	19093	0.28%	0.030%
26	17.312	2414	2421	2431	rBV	2398306	3771793	55.13%	5.973%
27	17.406	2431	2437	2450	rVV	3451561	5386539	78.73%	8.530%
28	17.547	2459	2461	2467	rVB6	5367	7523	0.11%	0.012%
29	17.706	2485	2488	2492	rVB4	6385	6895	0.10%	0.011%
30	19.269	2749	2754	2760	rVB	61410	88008	1.29%	0.139%
31	19.339	2760	2766	2771	rBV	47466	75934	1.11%	0.120%
32	19.533	2796	2799	2804	rVB7	4023	7473	0.11%	0.012%
33	19.621	2810	2814	2817	rVB5	18282	21976	0.32%	0.035%
34	19.704	2821	2828	2841	rVV	4662285	6776754	99.05%	10.731%
35	20.068	2888	2890	2894	rVB5	5767	7731	0.11%	0.012%
36	20.109	2894	2897	2901	rBV6	9601	14802	0.22%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060465.D
 Acq On : 29 Jan 2024 16:59
 Operator : MA/JU
 Sample : PB158661BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	20.362	2938	2940	2942	rBV3	8589	7190	0.11%	0.011%
38	20.656	2988	2990	2993	rBV4	12187	11311	0.17%	0.018%
39	20.767	3007	3009	3012	rBV4	8396	10591	0.15%	0.017%
40	21.572	3139	3146	3161	rBV2	2656455	4403706	64.36%	6.973%
41	22.477	3298	3300	3301	rBV2	12637	9770	0.14%	0.015%
42	23.029	3388	3394	3399	rBV3	57035	100364	1.47%	0.159%
43	23.111	3406	3408	3410	rBV3	15558	11747	0.17%	0.019%
44	23.194	3420	3422	3423	rBV2	11578	8685	0.13%	0.014%
45	23.423	3459	3461	3462	rBV2	11973	8555	0.13%	0.014%
46	23.817	3522	3528	3534	rVB3	72798	151016	2.21%	0.239%
47	24.516	3637	3647	3666	rBV2	2488250	6841810	100.00%	10.834%
48	24.739	3673	3685	3696	rBV	1748307	4896994	71.57%	7.755%
49	25.133	3750	3752	3754	rBV3	13891	12212	0.18%	0.019%
50	25.397	3795	3797	3798	rBV2	13969	11775	0.17%	0.019%
51	25.849	3867	3874	3882	rVB5	85858	242507	3.54%	0.384%
52	27.166	4090	4098	4109	rVB5	90176	303048	4.43%	0.480%
53	27.794	4203	4205	4207	rBV3	12294	10458	0.15%	0.017%
54	28.764	4362	4370	4372	rBV7	51574	119180	1.74%	0.189%
55	29.163	4436	4438	4439	rBV	13218	8963	0.13%	0.014%
56	29.668	4522	4524	4526	rBV2	14155	15011	0.22%	0.024%
57	29.821	4548	4550	4552	rBV3	11238	7817	0.11%	0.012%




Sum of corrected areas: 63149870

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060465.D
Acq On : 29 Jan 2024 16:59
Operator : MA/JU
Sample : PB158661BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK661

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

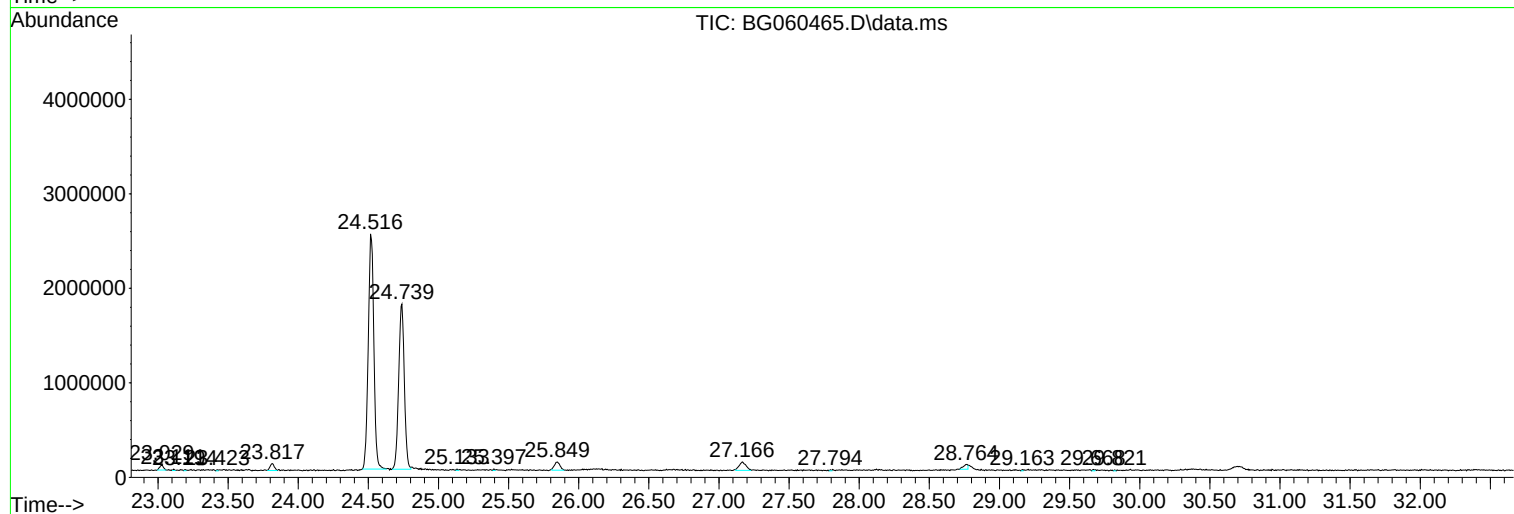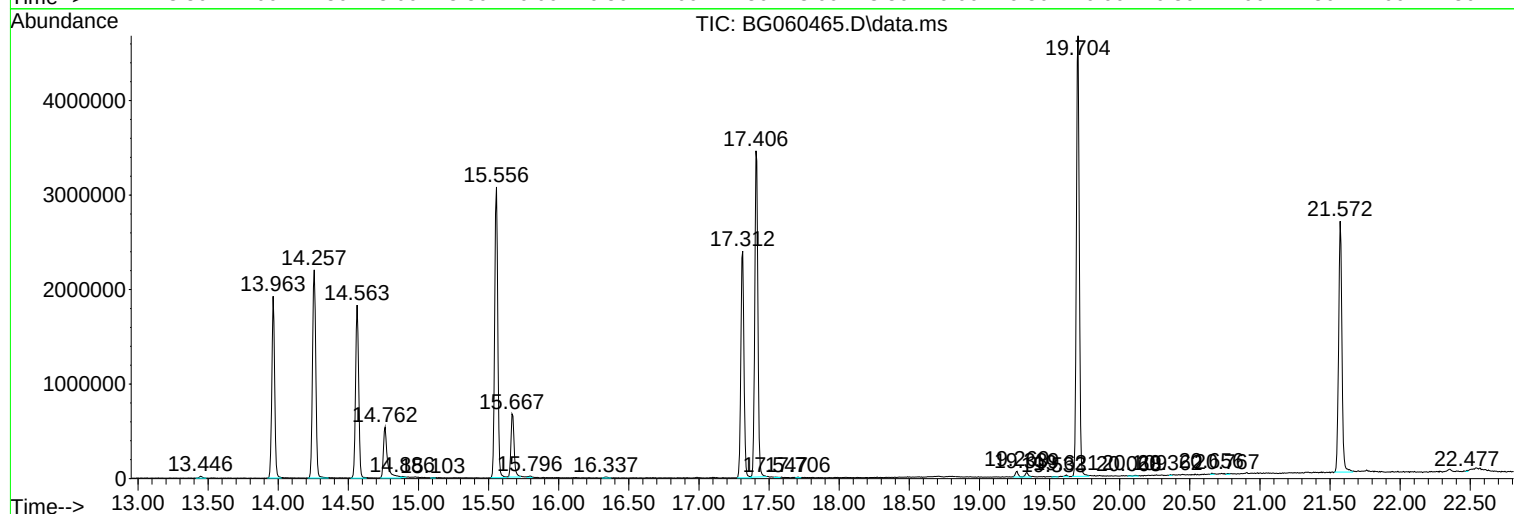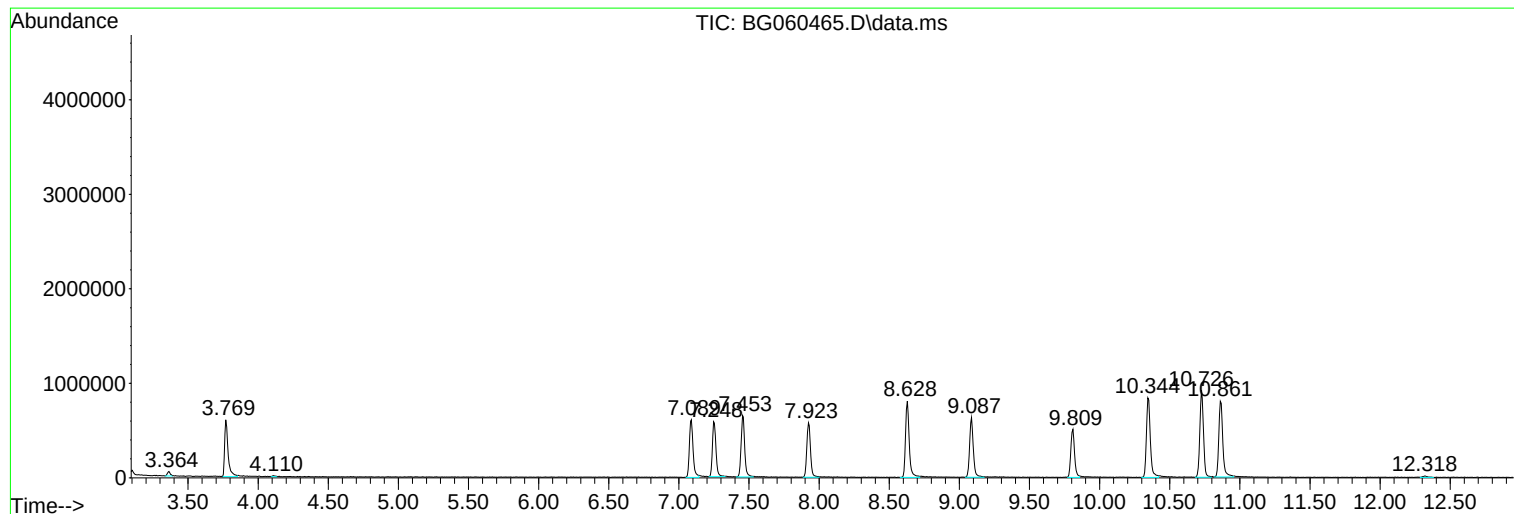

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060465.D
Acq On : 29 Jan 2024 16:59
Operator : MA/JU
Sample : PB158661BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK661

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060465.D
Acq On : 29 Jan 2024 16:59
Operator : MA/JU
Sample : PB158661BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK661

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc