

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060466.D
 Acq On : 29 Jan 2024 17:40
 Operator : MA/JU
 Sample : PB158663BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	42	47	54	rVB	50714	76005	1.13%	0.121%
2	3.769	112	116	130	rBV	580175	992395	14.70%	1.575%
3	4.110	170	174	179	rVB3	12506	18114	0.27%	0.029%
4	7.083	674	680	695	rBV	650812	1238237	18.34%	1.965%
5	7.248	700	708	718	rBV	590575	1020901	15.12%	1.620%
6	7.453	736	743	758	rBV	641591	1164853	17.25%	1.849%
7	7.923	815	823	834	rBV	614515	1083567	16.05%	1.720%
8	8.106	853	854	860	rVB4	5153	8848	0.13%	0.014%
9	8.628	935	943	958	rBV	843769	1536504	22.76%	2.438%
10	9.087	1012	1021	1034	rBV	632180	1192392	17.66%	1.892%
11	9.809	1136	1144	1154	rBV	505365	962298	14.25%	1.527%
12	10.344	1229	1235	1245	rBV	834168	1574341	23.32%	2.498%
13	10.726	1291	1300	1314	rBV	894405	1642536	24.33%	2.607%
14	10.861	1316	1323	1337	rBV	798042	1547384	22.92%	2.456%
15	12.318	1565	1571	1575	rBV4	13458	25822	0.38%	0.041%
16	13.440	1759	1762	1763	rBV2	8153	8125	0.12%	0.013%
17	13.534	1776	1778	1782	rVB2	6329	6814	0.10%	0.011%
18	13.963	1845	1851	1863	rBV	1860387	2696996	39.95%	4.280%
19	14.257	1893	1901	1917	rBV	2235145	3502131	51.87%	5.558%
20	14.375	1920	1921	1928	rVV4	5808	10683	0.16%	0.017%
21	14.563	1945	1953	1966	rBV	1764581	2777757	41.14%	4.408%
22	14.762	1980	1987	2001	rBV	525791	1003489	14.86%	1.593%
23	15.556	2114	2122	2134	rBV	3047069	4596096	68.08%	7.294%
24	15.673	2136	2142	2155	rVV	649872	1062557	15.74%	1.686%
25	15.791	2158	2162	2169	rVB8	14555	33242	0.49%	0.053%
26	16.343	2252	2256	2260	rVB6	9545	15300	0.23%	0.024%
27	16.989	2361	2366	2369	rBV4	8943	13285	0.20%	0.021%
28	17.312	2410	2421	2430	rBV	2389052	3725815	55.18%	5.913%
29	17.412	2431	2438	2454	rVV	3337356	5302722	78.54%	8.415%
30	18.276	2583	2585	2590	rVB5	5290	7668	0.11%	0.012%
31	18.693	2653	2656	2659	rBV4	7908	10574	0.16%	0.017%
32	19.263	2748	2753	2761	rBV2	51778	89129	1.32%	0.141%
33	19.339	2761	2766	2770	rVV	44439	70707	1.05%	0.112%
34	19.375	2770	2772	2778	rVV7	8681	14605	0.22%	0.023%
35	19.616	2809	2813	2817	rBV7	14209	20178	0.30%	0.032%
36	19.704	2821	2828	2840	rBV	4620972	6692377	99.12%	10.621%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060466.D
 Acq On : 29 Jan 2024 17:40
 Operator : MA/JU
 Sample : PB158663BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	20.033	2881	2884	2887	rBV5	8822	9752	0.14%	0.015%
38	20.233	2916	2918	2920	rBV3	5644	6766	0.10%	0.011%
39	20.426	2949	2951	2952	rBV2	9589	7189	0.11%	0.011%
40	20.667	2988	2992	2997	rVB8	13613	18980	0.28%	0.030%
41	20.902	3030	3032	3035	rVB4	10898	7709	0.11%	0.012%
42	21.131	3069	3071	3072	rBV2	8518	6863	0.10%	0.011%
43	21.572	3139	3146	3161	rBV	2597374	4260978	63.11%	6.762%
44	21.748	3174	3176	3180	rVB5	16520	19502	0.29%	0.031%
45	22.130	3238	3241	3244	rBV5	12491	16181	0.24%	0.026%
46	22.348	3274	3278	3283	rBV7	30147	59830	0.89%	0.095%
47	23.029	3389	3394	3400	rVB4	61838	114891	1.70%	0.182%
48	23.811	3522	3527	3533	rVB4	84069	158645	2.35%	0.252%
49	24.322	3612	3614	3616	rBV3	13235	12214	0.18%	0.019%
50	24.516	3637	3647	3665	rBV2	2480389	6751504	100.00%	10.714%
51	24.733	3673	3684	3697	rVB	1726562	4795872	71.03%	7.611%
52	25.844	3864	3873	3882	rBV3	107876	298470	4.42%	0.474%
53	27.166	4091	4098	4111	rVB5	92311	330900	4.90%	0.525%
54	27.700	4187	4189	4190	rBV	11777	7143	0.11%	0.011%
55	27.906	4222	4224	4226	rBV3	12400	8207	0.12%	0.013%
56	28.059	4248	4250	4251	rBV2	9766	7019	0.10%	0.011%
57	28.206	4273	4275	4278	rBV4	12517	11175	0.17%	0.018%
58	28.699	4357	4359	4361	rBV3	12816	12945	0.19%	0.021%
59	28.764	4361	4370	4382	rVB6	64899	259425	3.84%	0.412%
60	30.691	4689	4698	4699	rBV7	36139	86774	1.29%	0.138%




Sum of corrected areas: 63013381

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060466.D
Acq On : 29 Jan 2024 17:40
Operator : MA/JU
Sample : PB158663BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

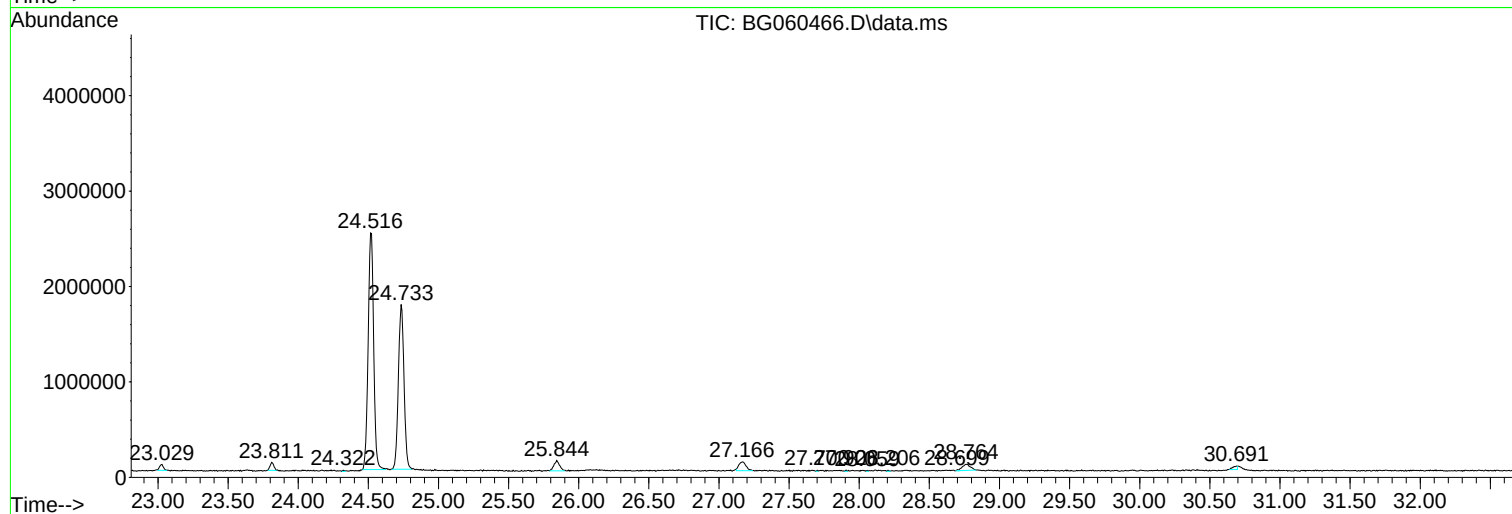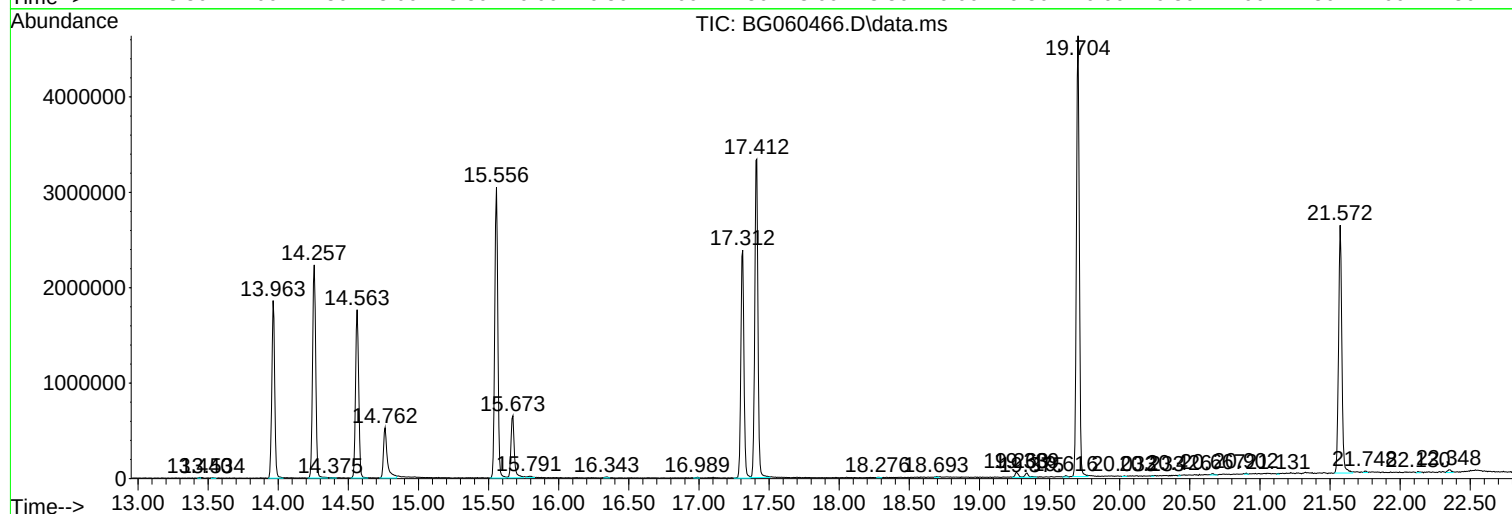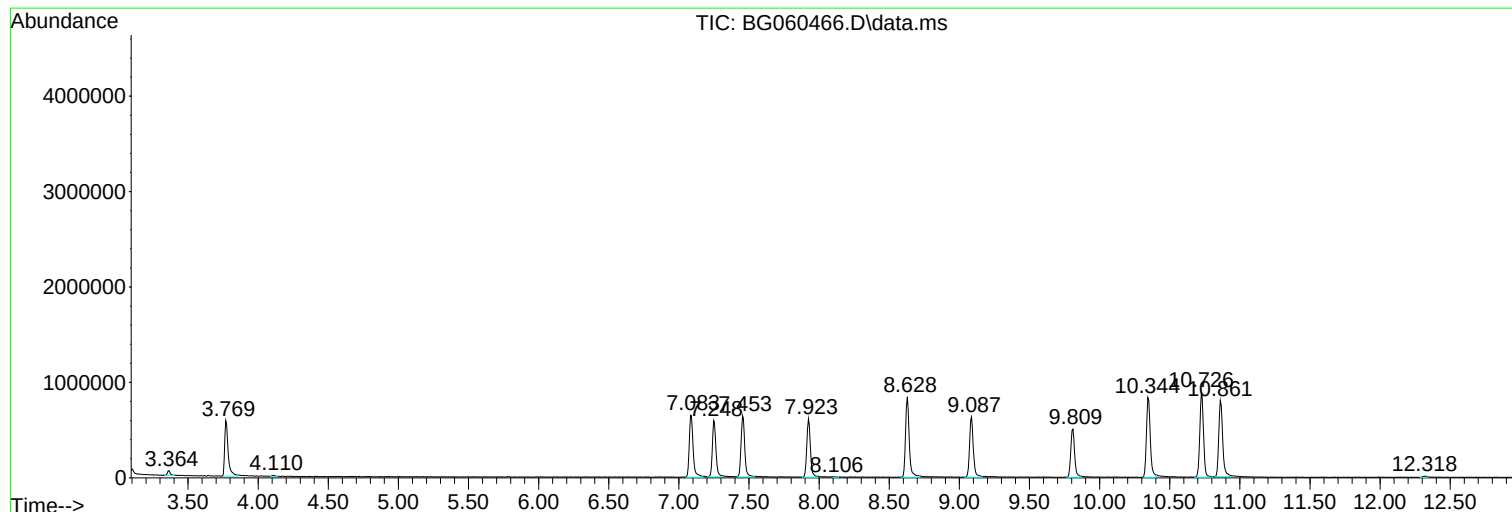

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060466.D
Acq On : 29 Jan 2024 17:40
Operator : MA/JU
Sample : PB158663BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060466.D
Acq On : 29 Jan 2024 17:40
Operator : MA/JU
Sample : PB158663BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc