

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060470.D
 Acq On : 29 Jan 2024 20:21
 Operator : MA/JU
 Sample : P1239-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.338	37	42	57	rBV2	385929	669536	8.47%	0.962%
2	3.638	91	93	98	rBV5	7503	10169	0.13%	0.015%
3	3.773	112	116	120	rBV	181334	307580	3.89%	0.442%
4	4.108	170	173	178	rVB	10849	12079	0.15%	0.017%
5	4.214	187	191	194	rVB3	5639	8547	0.11%	0.012%
6	7.087	673	680	691	rBV	152974	293145	3.71%	0.421%
7	7.251	700	708	724	rBV	696179	1189435	15.04%	1.709%
8	7.457	734	743	756	rBV	601835	1067168	13.49%	1.534%
9	7.921	815	822	836	rBV	629317	1129574	14.28%	1.623%
10	8.632	936	943	951	rBV	534392	968223	12.24%	1.391%
11	9.084	1010	1020	1035	rBV	793164	1476086	18.66%	2.121%
12	9.484	1085	1088	1093	rVB4	8916	17037	0.22%	0.024%
13	9.648	1113	1116	1122	rVB5	8536	14517	0.18%	0.021%
14	9.807	1135	1143	1156	rBV	636794	1157882	14.64%	1.664%
15	10.348	1227	1235	1249	rBV	1093366	2049492	25.92%	2.945%
16	10.729	1290	1300	1312	rBV	1018992	1873931	23.70%	2.693%
17	10.865	1314	1323	1336	rBV	741774	1500706	18.98%	2.157%
18	11.476	1419	1427	1434	rBV4	19435	49292	0.62%	0.071%
19	12.310	1563	1569	1576	rBV4	22366	47161	0.60%	0.068%
20	12.903	1665	1670	1671	rBV4	7878	9528	0.12%	0.014%
21	13.168	1712	1715	1717	rBV4	6695	8070	0.10%	0.012%
22	13.385	1747	1752	1754	rBV5	7110	10712	0.14%	0.015%
23	13.444	1759	1762	1767	rBV5	24344	40756	0.52%	0.059%
24	13.967	1843	1851	1859	rBV	2435750	3624330	45.83%	5.209%
25	14.084	1866	1871	1876	rBV8	18228	27326	0.35%	0.039%
26	14.196	1887	1890	1893	rBV4	9722	14098	0.18%	0.020%
27	14.255	1893	1900	1907	rBV2	2954478	4628056	58.52%	6.651%
28	14.443	1930	1932	1936	rVB5	9787	11209	0.14%	0.016%
29	14.560	1945	1952	1963	rBV	1930585	3040015	38.44%	4.369%
30	14.772	1981	1988	1996	rBV	110197	240892	3.05%	0.346%
31	15.036	2031	2033	2037	rBV4	10914	10897	0.14%	0.016%
32	15.083	2037	2041	2047	rVB8	15315	22082	0.28%	0.032%
33	15.212	2059	2063	2067	rBV7	23143	34182	0.43%	0.049%
34	15.277	2072	2074	2077	rVB4	9109	8627	0.11%	0.012%
35	15.365	2087	2089	2091	rBV2	8767	8810	0.11%	0.013%
36	15.553	2114	2121	2131	rBV	3874745	6057521	76.60%	8.706%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
 Data File : BG060470.D
 Acq On : 29 Jan 2024 20:21
 Operator : MA/JU
 Sample : P1239-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	15.671	2135	2141	2151	rVB	986811	1472290	18.62%	2.116%
38	15.882	2175	2177	2180	rBV4	7303	7920	0.10%	0.011%
39	16.088	2209	2212	2216	rVV6	8186	13885	0.18%	0.020%
40	16.335	2252	2254	2260	rVB7	12081	14063	0.18%	0.020%
41	16.599	2297	2299	2302	rBV3	9287	12691	0.16%	0.018%
42	17.310	2414	2420	2428	rBV	2630477	3934096	49.75%	5.654%
43	17.410	2430	2437	2448	rVV2	4324198	6567751	83.05%	9.439%
44	18.197	2567	2571	2578	rBV3	149365	263833	3.34%	0.379%
45	19.267	2750	2753	2757	rVB5	77275	100798	1.27%	0.145%
46	19.331	2761	2764	2769	rBV2	73989	113491	1.44%	0.163%
47	19.701	2821	2827	2835	rBV	5485733	7874579	99.57%	11.317%
48	21.217	3082	3085	3093	rVB3	148760	233829	2.96%	0.336%
49	21.576	3139	3146	3156	rBV	2619227	4232412	53.52%	6.083%
50	23.215	3421	3425	3432	rVB	159201	264074	3.34%	0.380%
51	23.808	3524	3526	3533	rVB4	66775	112563	1.42%	0.162%
52	24.519	3636	3647	3662	rBV2	2822429	7908374	100.00%	11.366%
53	24.737	3674	3684	3698	rVB	1657364	4611519	58.31%	6.627%
54	25.841	3867	3872	3884	rVB6	76079	204923	2.59%	0.295%




Sum of corrected areas: 69581762

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060470.D
Acq On : 29 Jan 2024 20:21
Operator : MA/JU
Sample : P1239-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

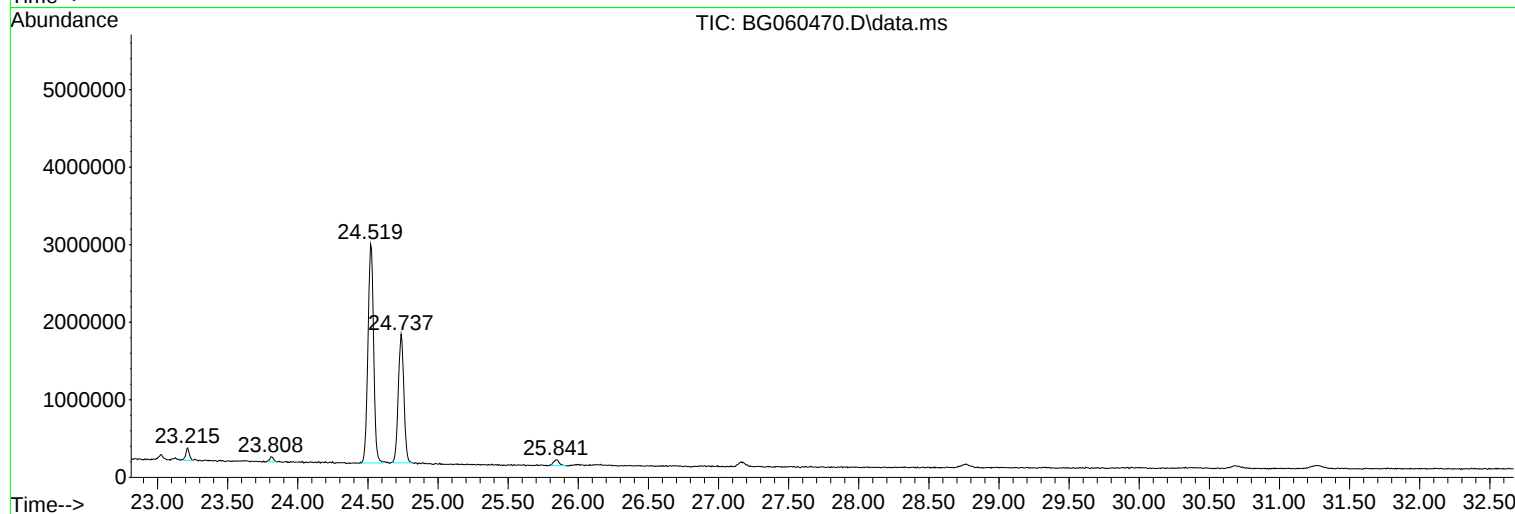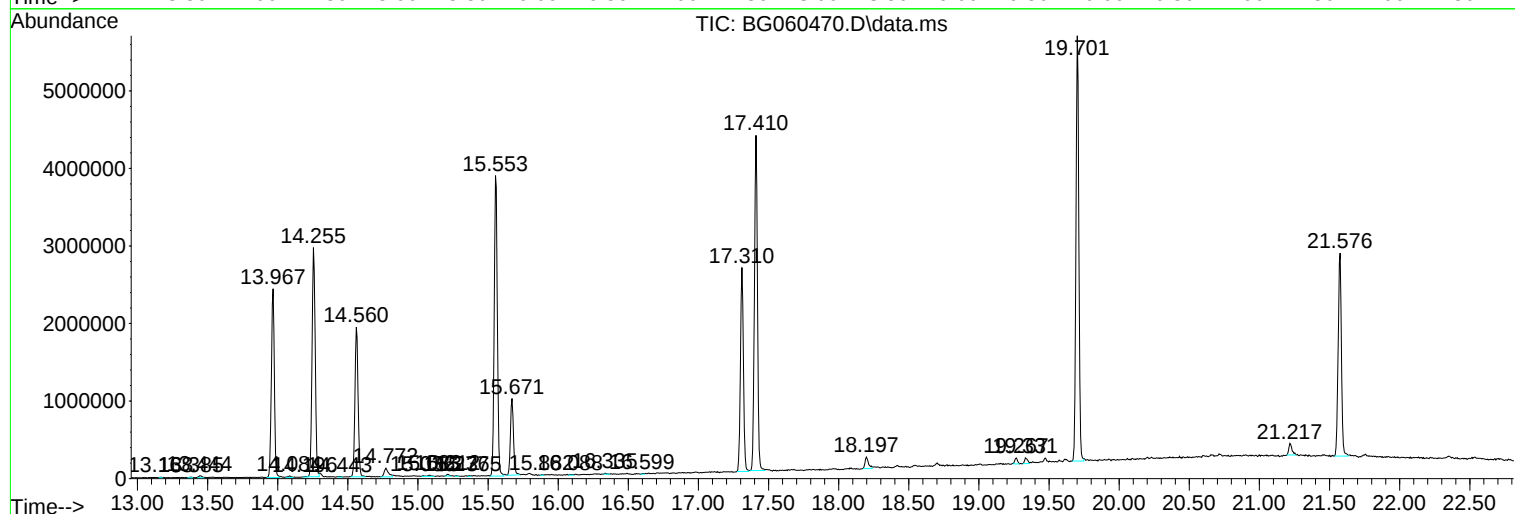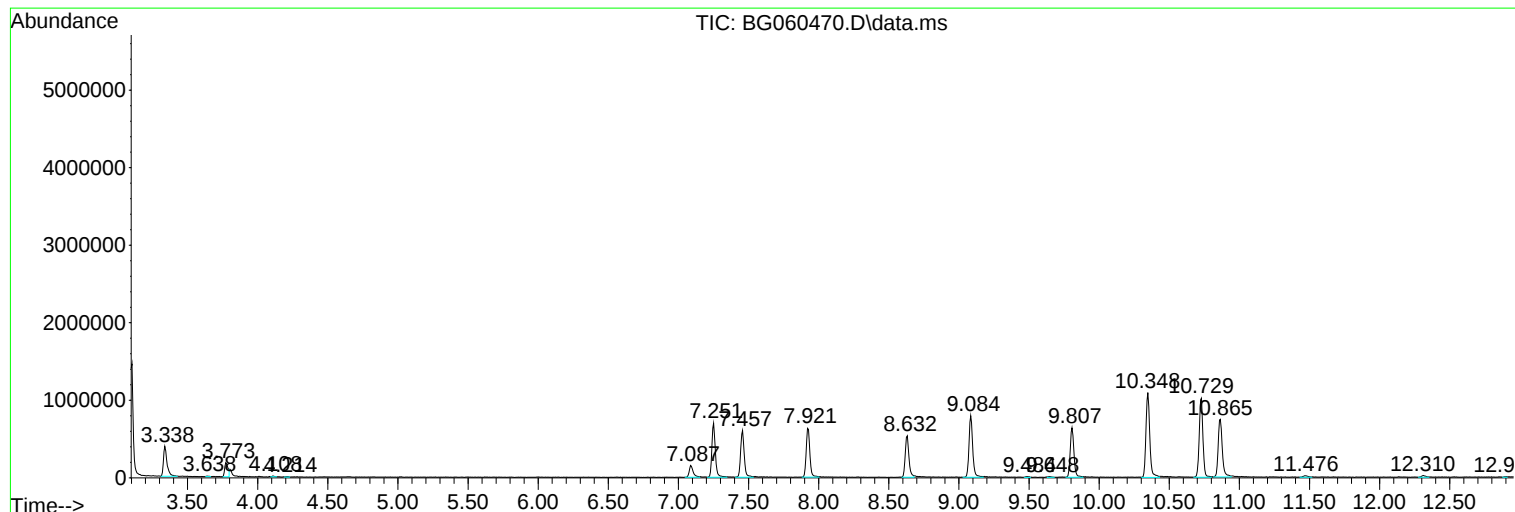

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060470.D
Acq On : 29 Jan 2024 20:21
Operator : MA/JU
Sample : P1239-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012924\
Data File : BG060470.D
Acq On : 29 Jan 2024 20:21
Operator : MA/JU
Sample : P1239-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc