
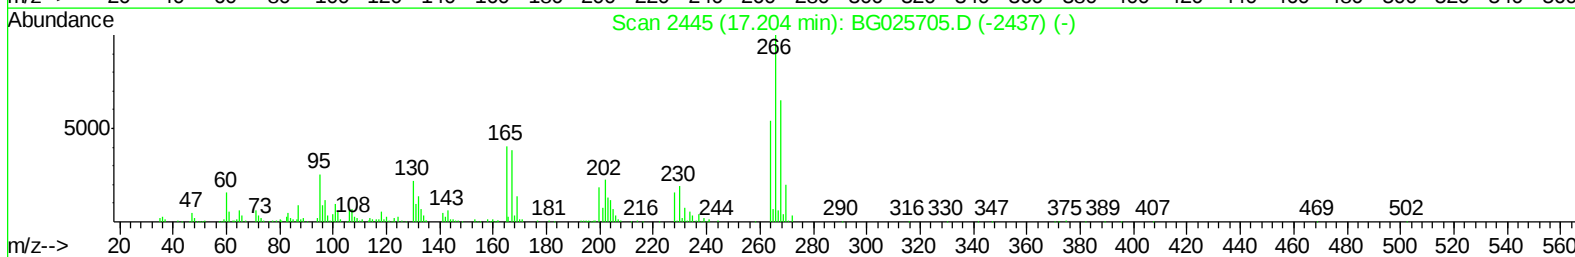
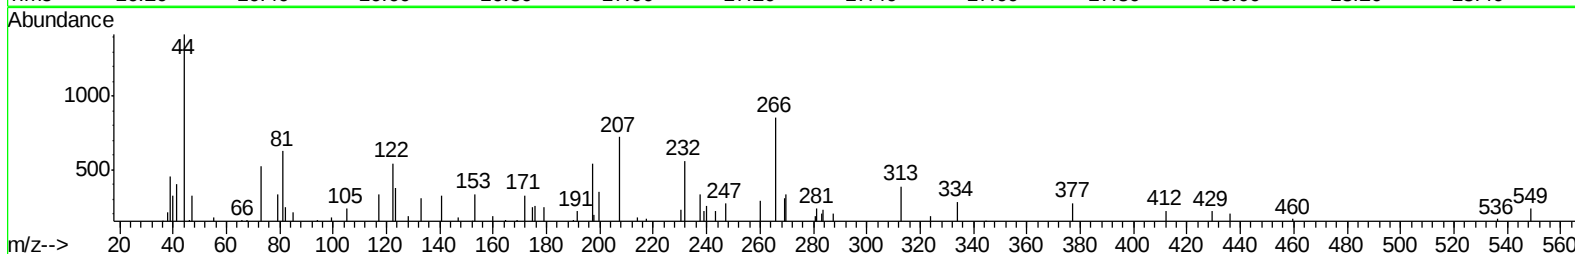


Data Path : Z:\HPCHEM1\BNA_G\Data\BG013017\
 Data File : BG025701.D
 Acq On : 30 Jan 2017 12:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:31:02 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 18:29:38 2017
 Response via : Initial Calibration

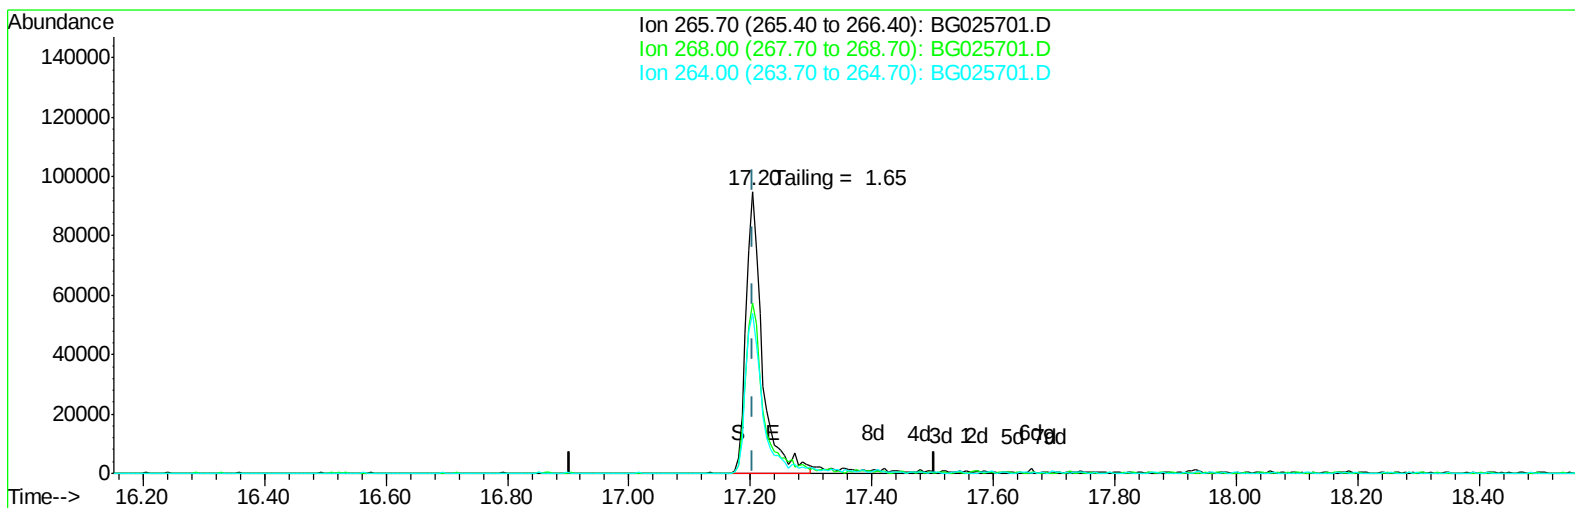

TIC: BG025701.D

(69) Pentachlorophenol (C)




17.556min (+0.352) 1082.56ng

response 566

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG013017\
Data File : BG025701.D
Acq On : 30 Jan 2017 12:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:31:02 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 18:29:38 2017
Response via : Initial Calibration

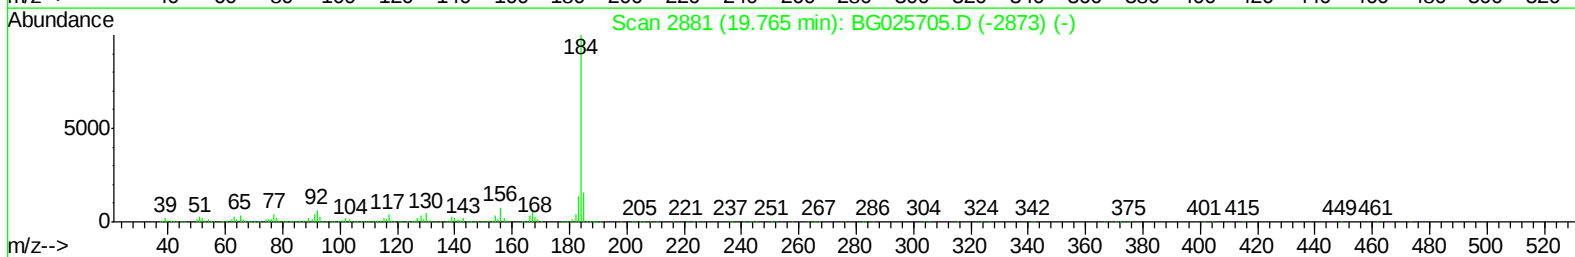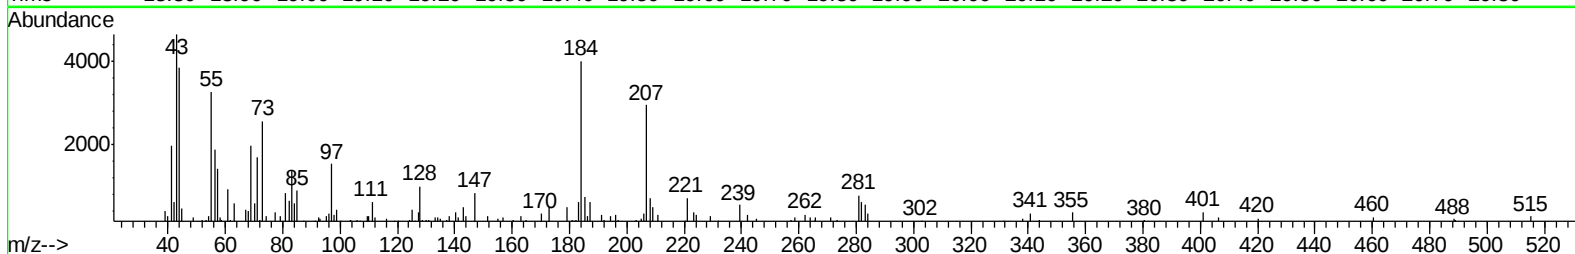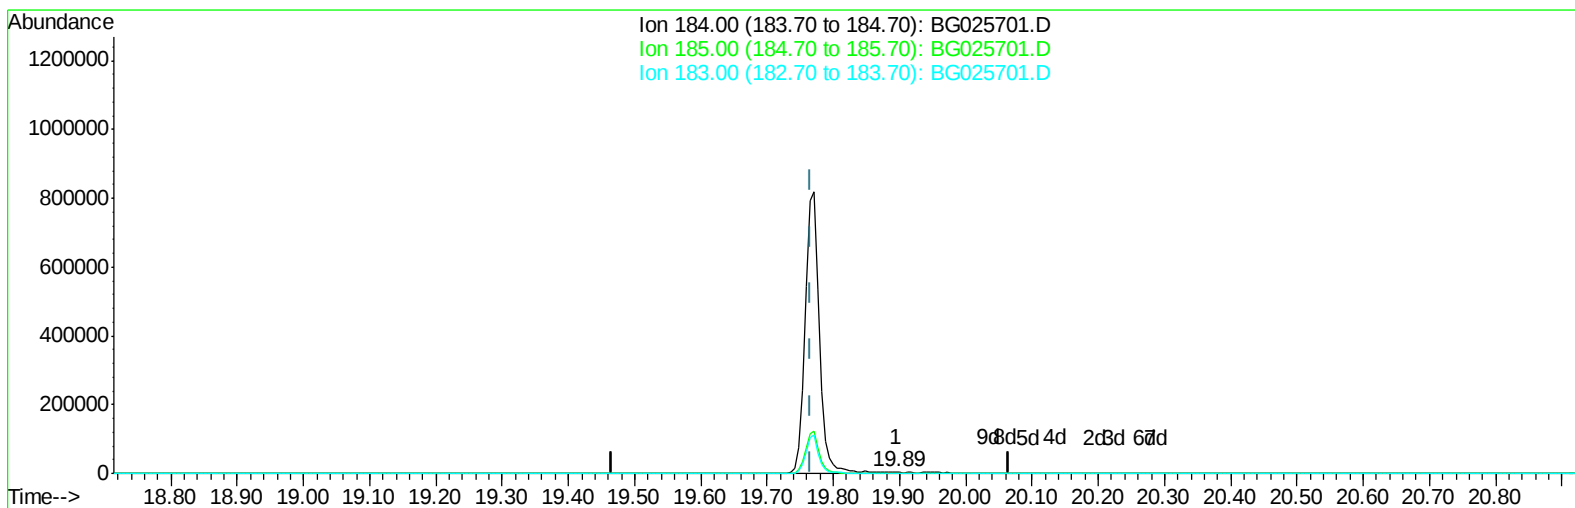

TIC: BG025701.D

(76) Benzidine

19.894min (+0.129) 650.44ng

response 3864

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	18.55
183.00	13.80	15.59
0.00	0.00	0.00